
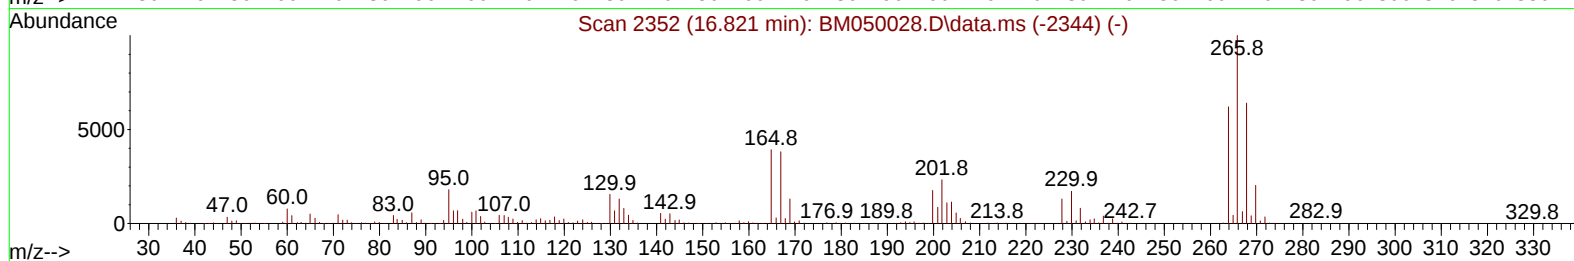
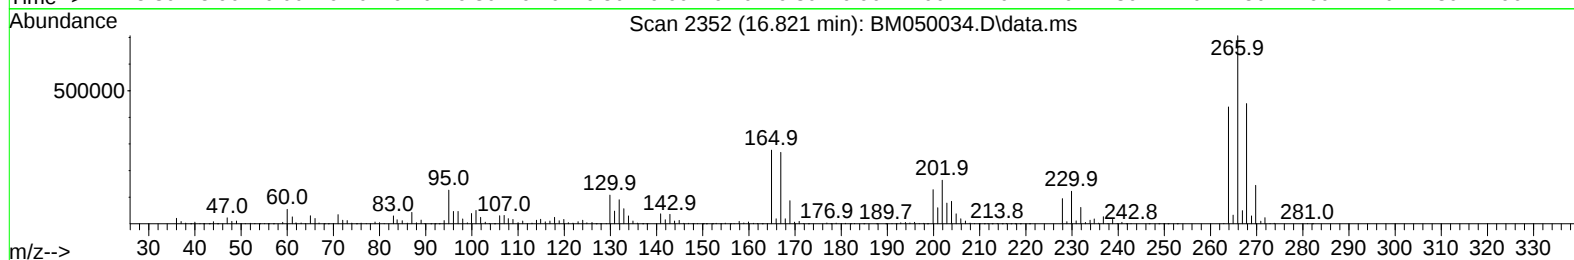


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042925\
Data File : BM050034.D
Acq On : 29 Apr 2025 08:34
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 29 10:46:30 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 28 18:09:16 2025
Response via : Initial Calibration

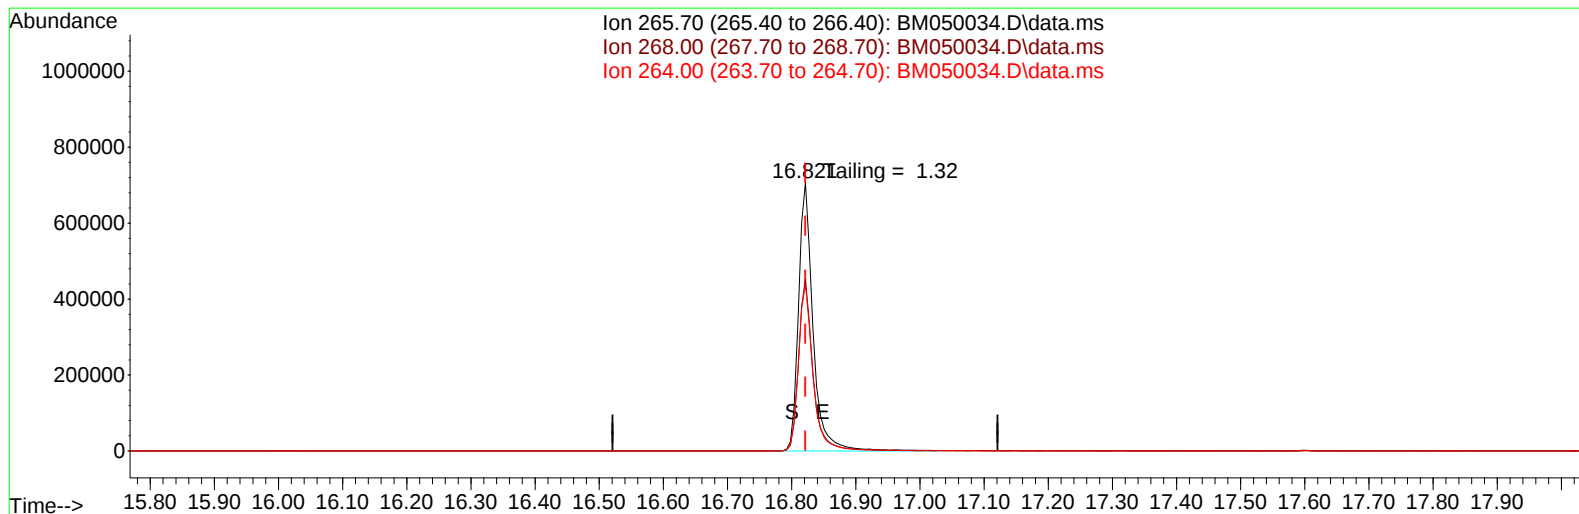

TIC: BM050034.D\data.ms




(70) Pentachlorophenol (C)

16.821min (+ 0.000) 30619.08 ng

response 1122917

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.00	63.94
264.00	62.00	62.11
0.00	0.00	0.00

Quant Time: Apr 29 10:46:30 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 28 18:09:16 2025
Response via : Initial Calibration

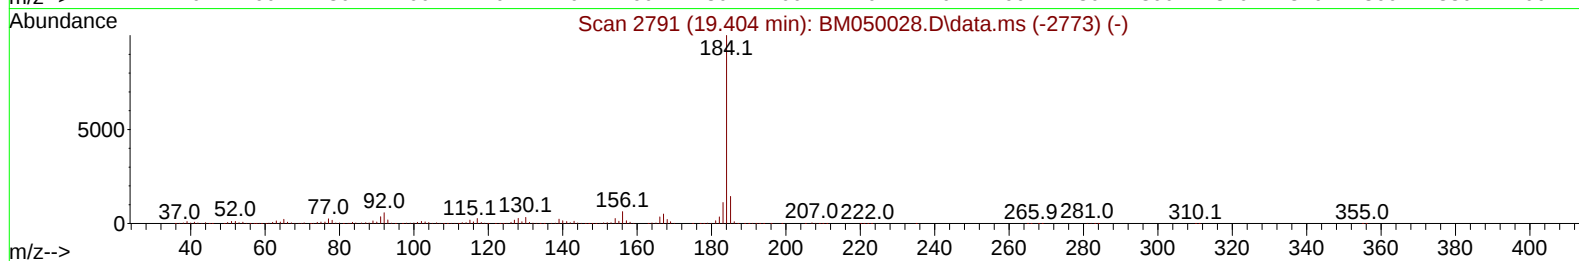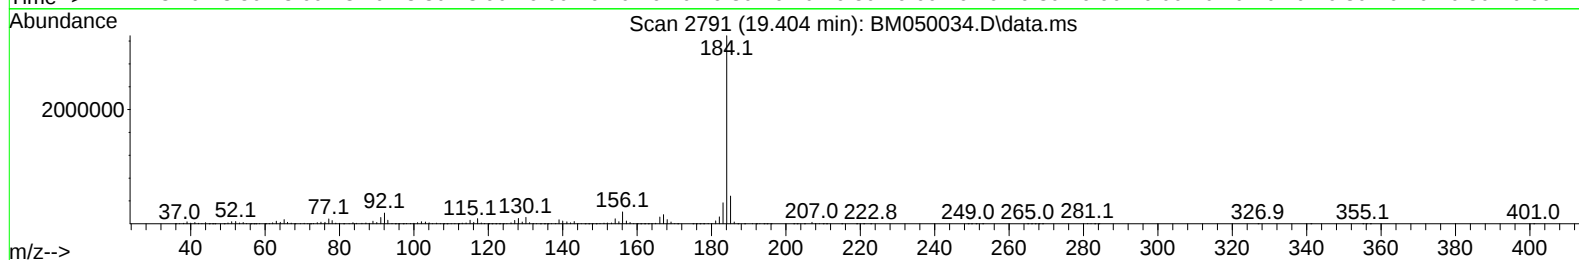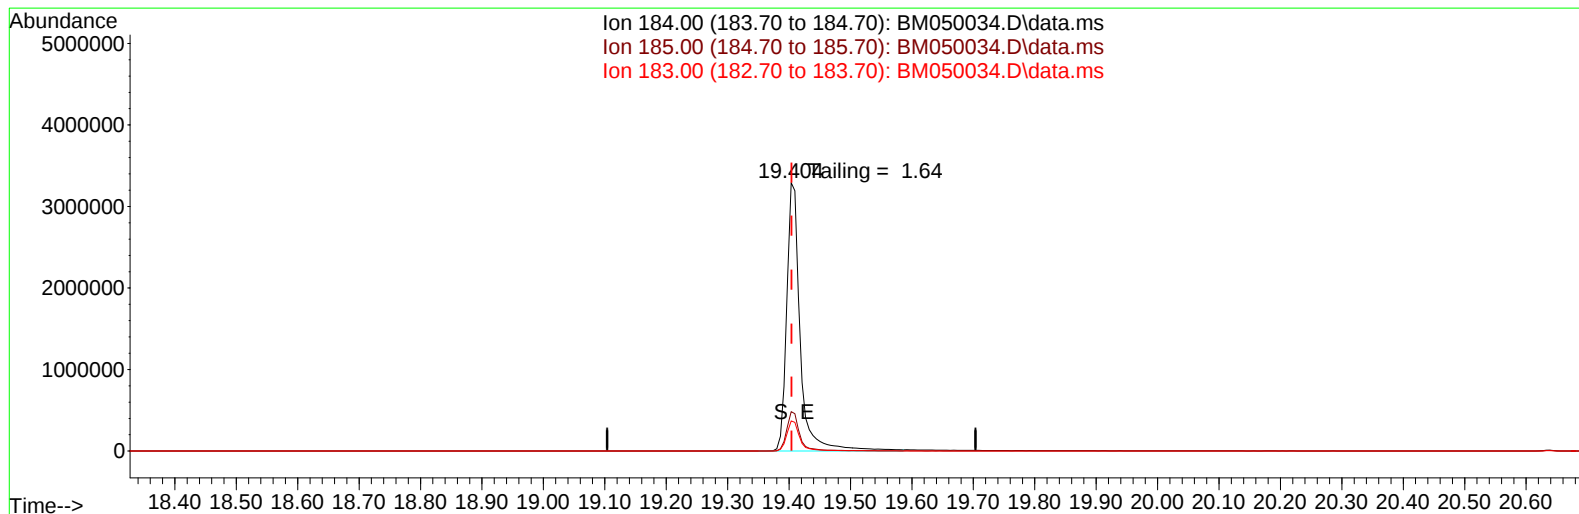

TIC: BM050034.D\data.ms

(77) Benzidine

19.404min (-0.000) 11929.52 ng

response **5130701**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.69
183.00	11.10	11.20
0.00	0.00	0.00