

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM043025\
 Data File : BM050049.D
 Acq On : 30 Apr 2025 17:23
 Operator : RC/JU
 Sample : Q1889-02
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 COMP-2

Quant Time: Apr 30 17:58:40 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042825.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 28 18:09:16 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.763	152	252068	20.000	ng	0.00
21) Naphthalene-d8	10.563	136	894770	20.000	ng	0.00
39) Acenaphthene-d10	14.410	164	606447	20.000	ng	0.00
64) Phenanthrene-d10	17.157	188	1171426	20.000	ng	0.00
76) Chrysene-d12	21.398	240	1105914	20.000	ng	0.00
86) Perylene-d12	24.397	264	1173847	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.352	112	1371063	95.245	ng	0.00
7) Phenol-d6	6.946	99	1732188	95.739	ng	0.00
23) Nitrobenzene-d5	8.922	82	1037353	57.129	ng	0.00
42) 2,4,6-Tribromophenol	15.904	330	829360	92.489	ng	0.00
45) 2-Fluorobiphenyl	13.028	172	2660312	51.894	ng	0.00
79) Terphenyl-d14	19.780	244	4448897	59.527	ng	0.00


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM043025\
Data File : BM050049.D
Acq On : 30 Apr 2025 17:23
Operator : RC/JU
Sample : Q1889-02
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
COMP-2

Quant Time: Apr 30 17:58:40 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 28 18:09:16 2025
Response via : Initial Calibration

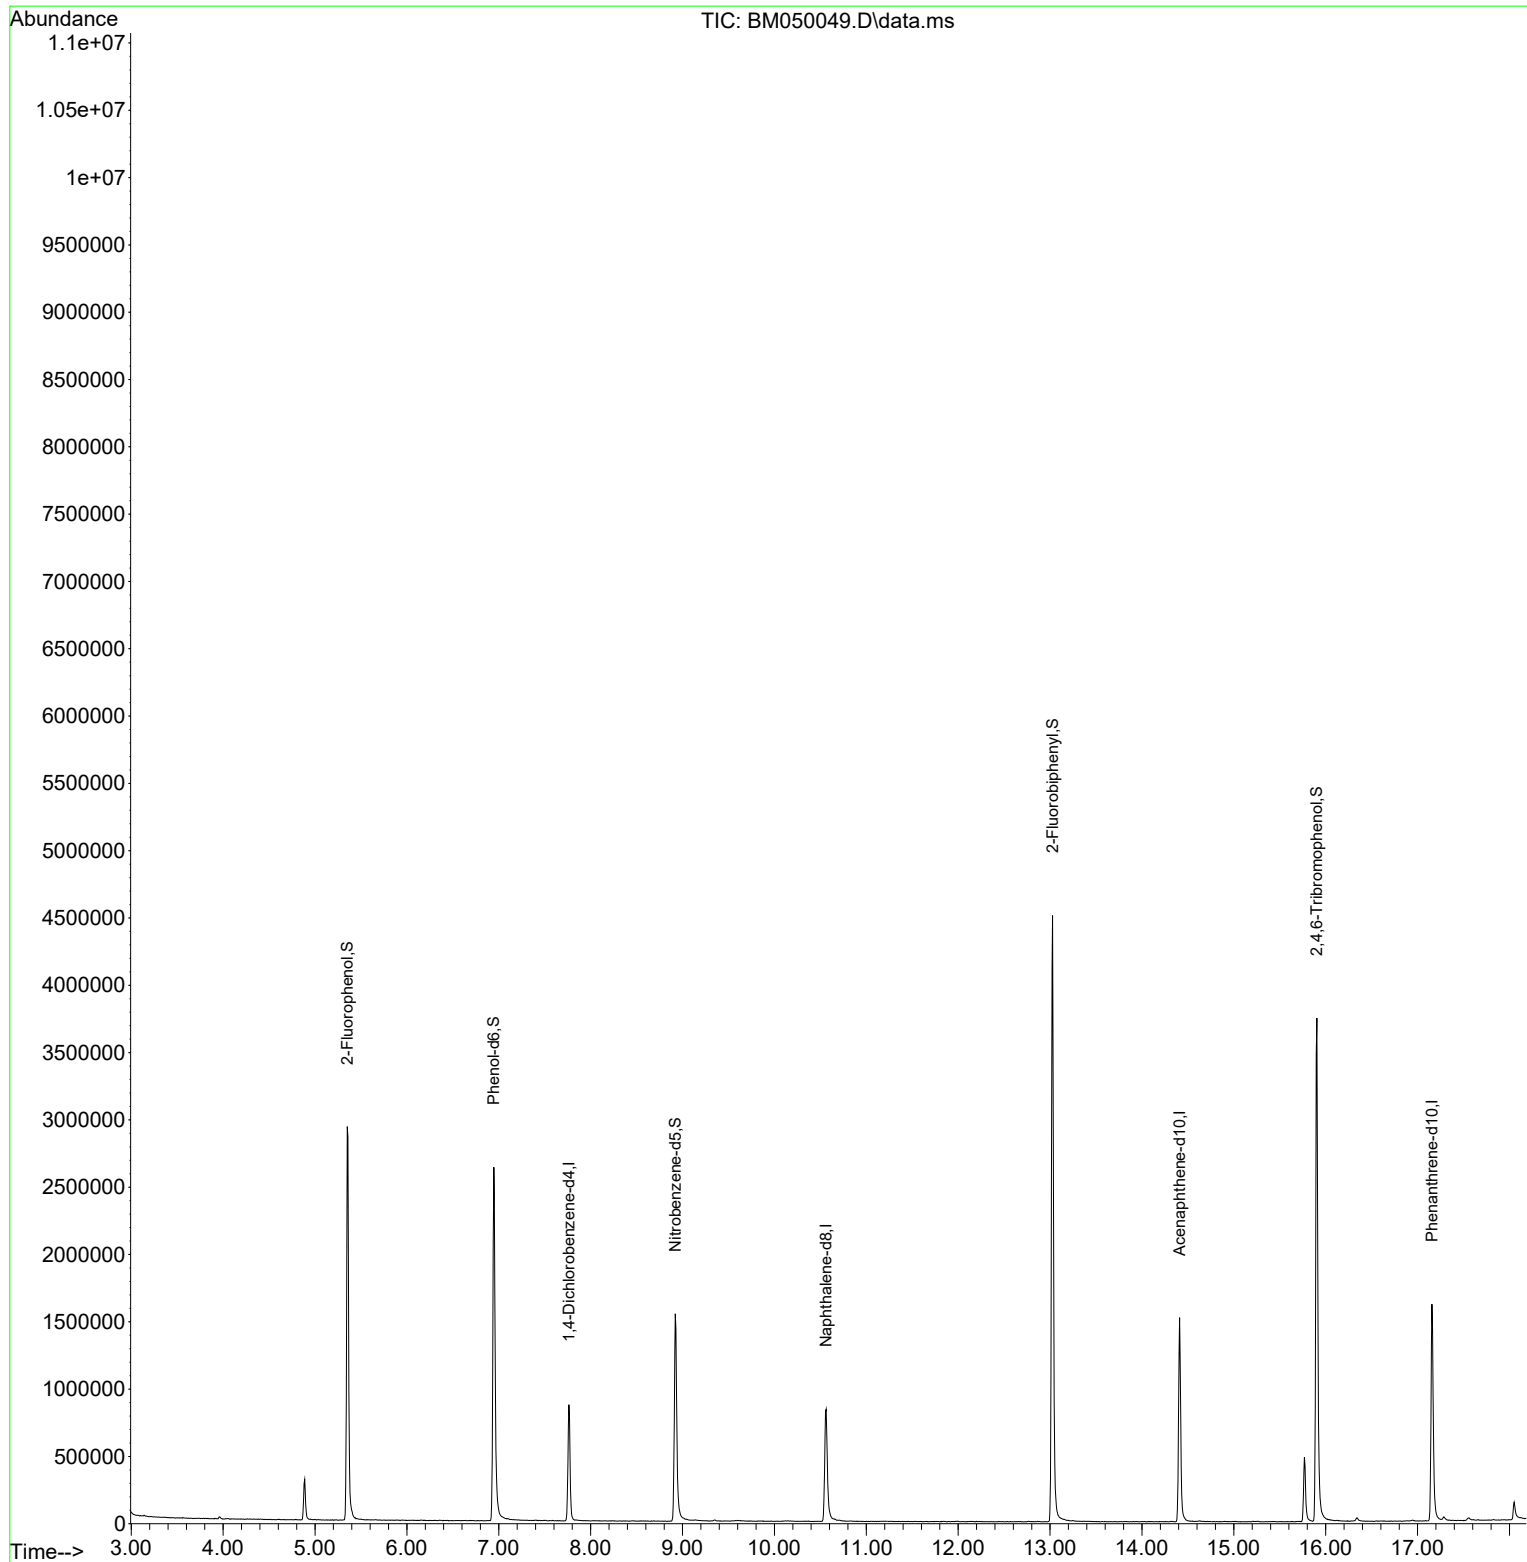

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM043025\
Data File : BM050049.D
Acq On : 30 Apr 2025 17:23
Operator : RC/JU
Sample : Q1889-02
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
COMP-2

Quant Time: Apr 30 17:58:40 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 28 18:09:16 2025
Response via : Initial Calibration

