
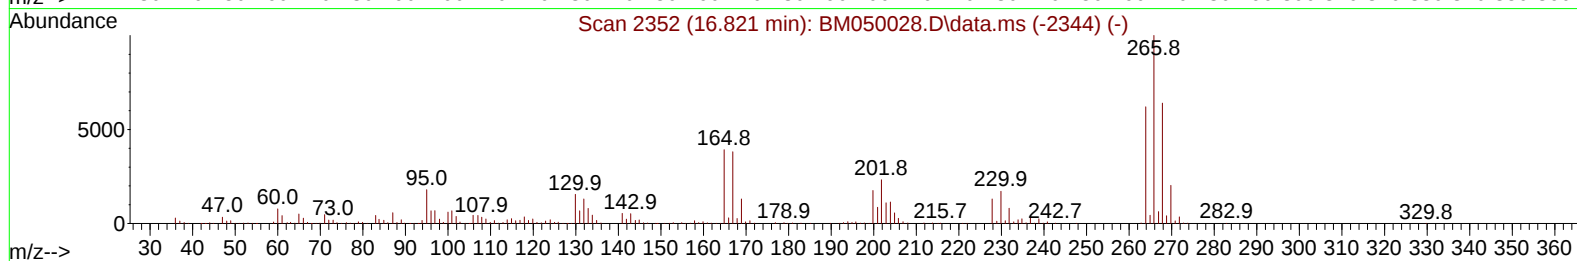
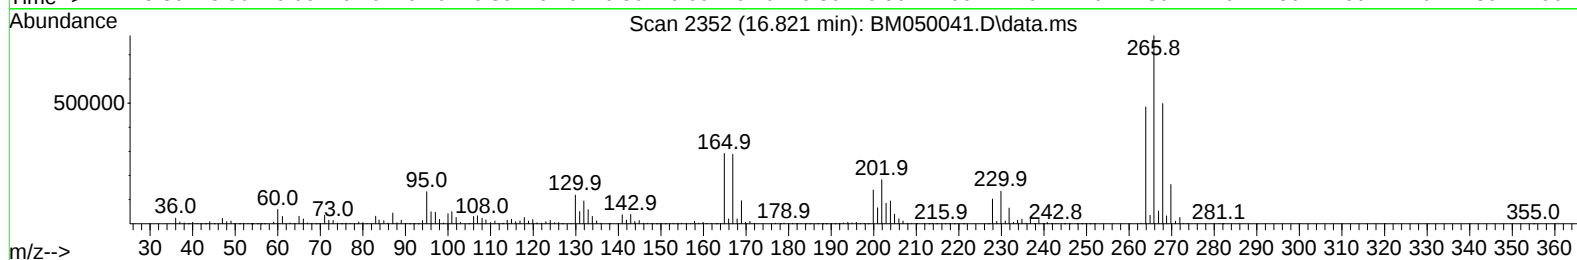


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM043025\
Data File : BM050041.D
Acq On : 30 Apr 2025 10:14
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 30 11:54:32 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 28 18:09:16 2025
Response via : Initial Calibration

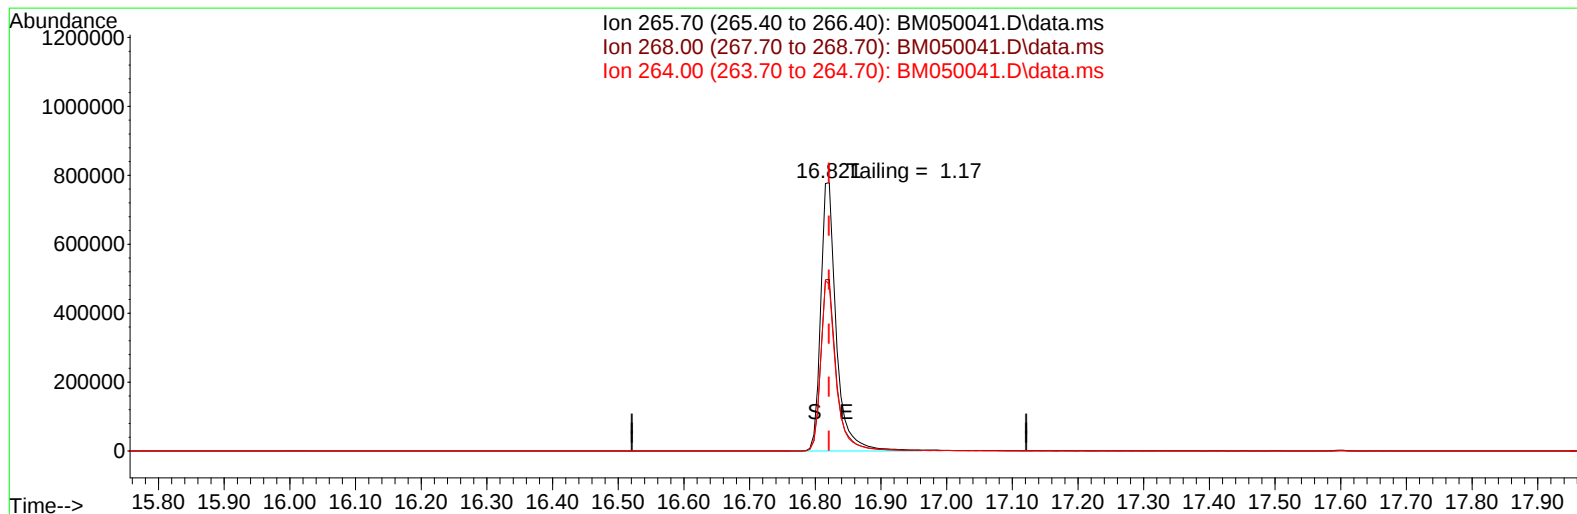

TIC: BM050041.D\data.ms




(70) Pentachlorophenol (C)

16.821min (+ 0.000) 47790.89 ng

response 1282068

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.00	63.93
264.00	62.00	62.12
0.00	0.00	0.00

Quant Time: Apr 30 11:54:32 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 28 18:09:16 2025
Response via : Initial Calibration

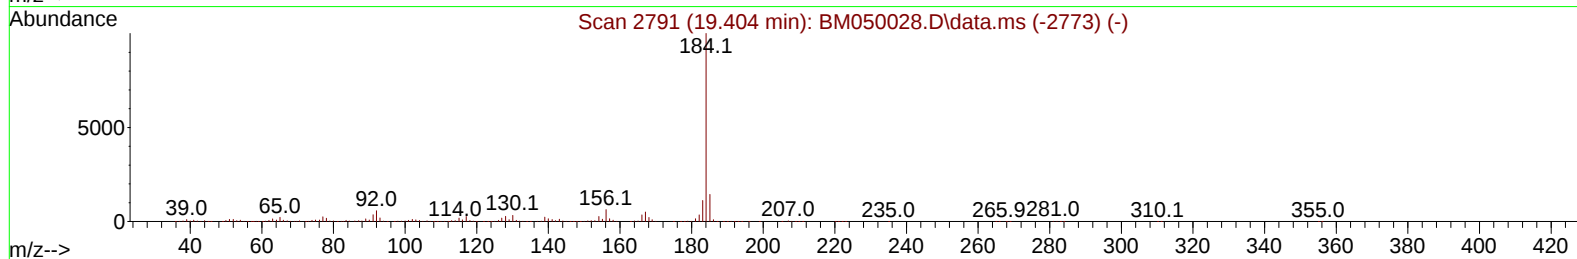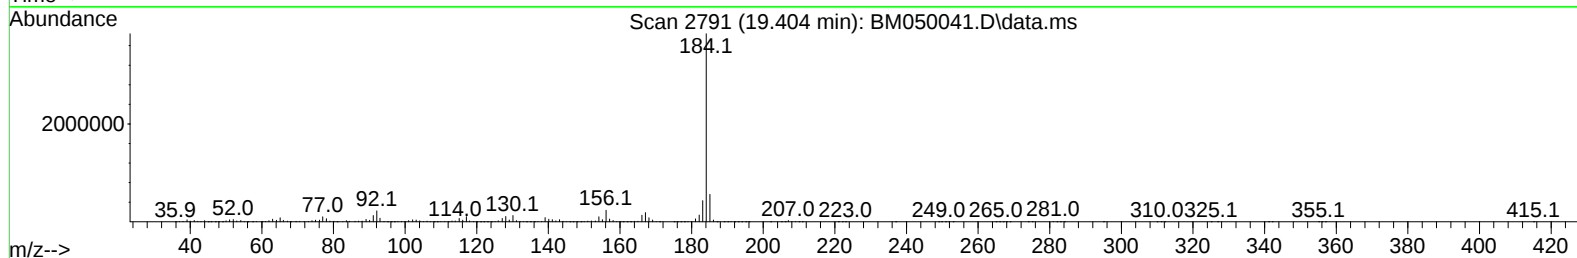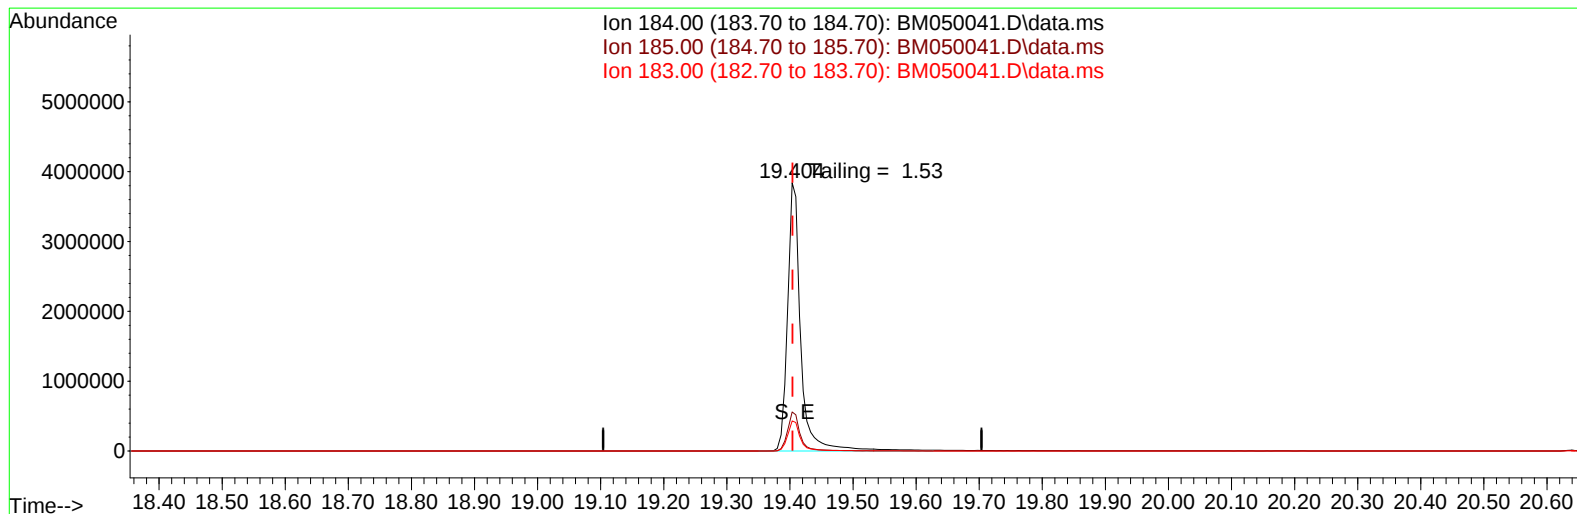

TIC: BM050041.D\data.ms

(77) Benzidine

19.404min (-0.000) 7947.43 ng

response **5627615**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.56
183.00	11.10	11.24
0.00	0.00	0.00