
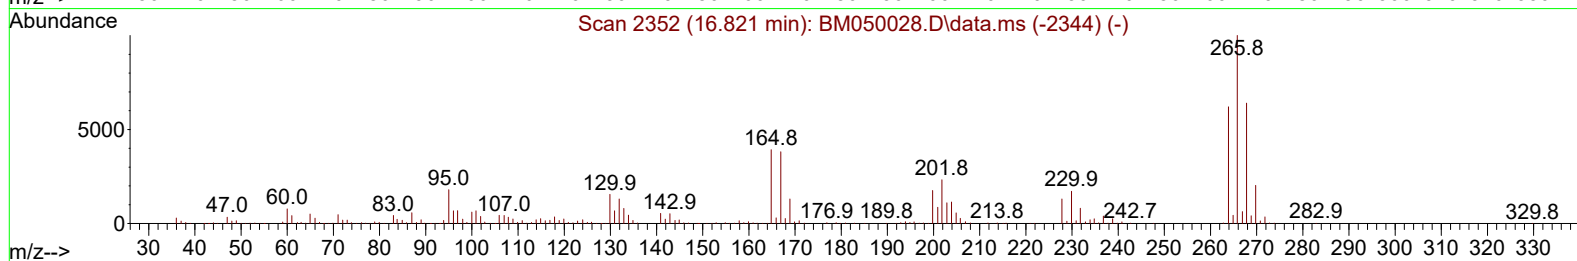
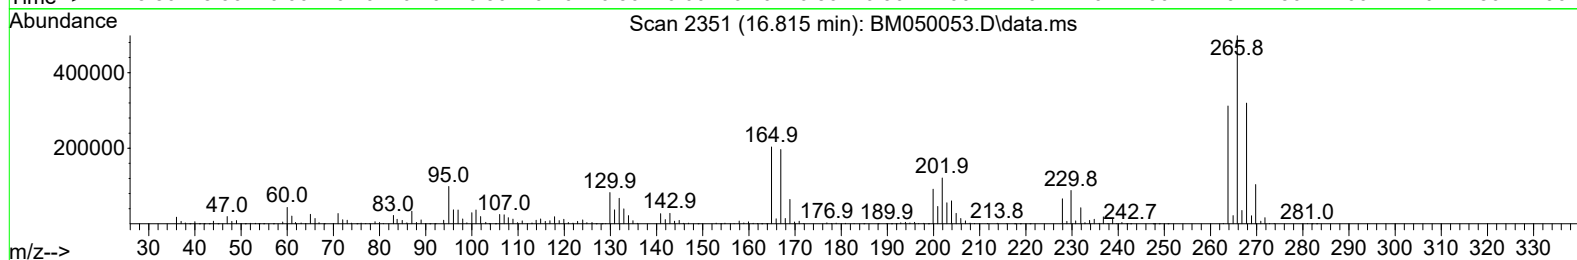


```
Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM043025\  
Data File : BM050053.D  
Acq On    : 30 Apr 2025   20:38  
Operator  : RC/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1   Sample Multiplier: 1
```

Quant Time: May 01 01:52:49 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 28 18:09:16 2025
Response via : Initial Calibration

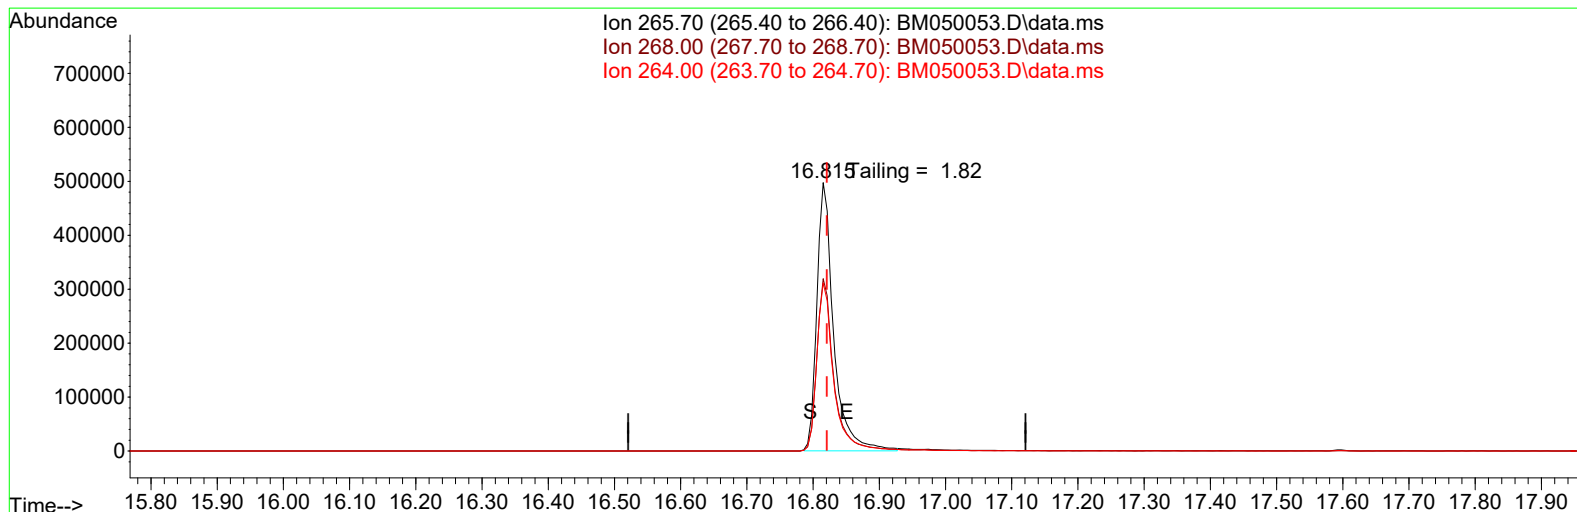

TIC: BM050053.D\data.ms

(70) Pentachlorophenol (C)




16.815min (-0.006) 998032.02 ng

response **884891**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.00	64.19
264.00	62.00	62.68
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM043025\
Data File : BM050053.D
Acq On : 30 Apr 2025 20:38
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 01 01:52:49 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 28 18:09:16 2025
Response via : Initial Calibration

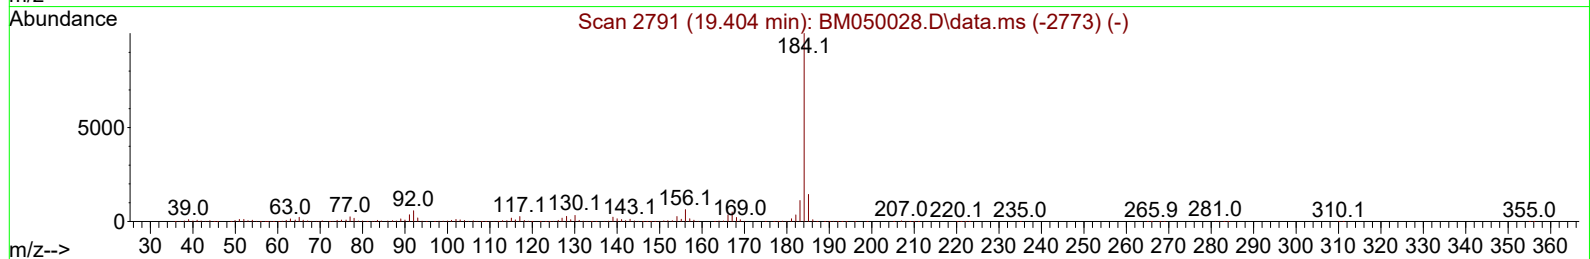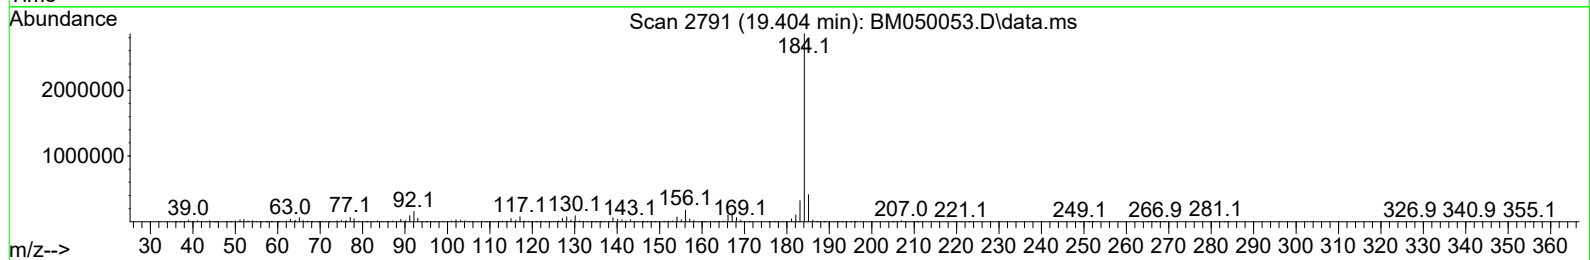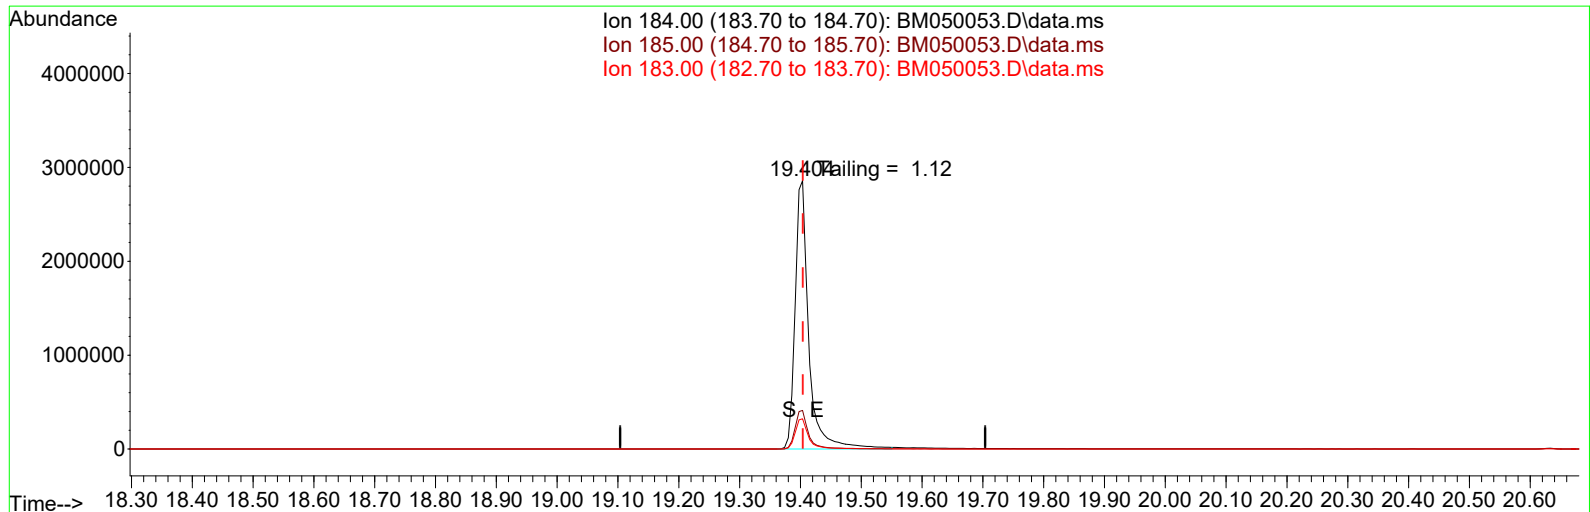

TIC: BM050053.D\data.ms

(77) Benzidine

19.404min (-0.000) 132996.89 ng m

response 4440691

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.39
183.00	11.10	11.28
0.00	0.00	0.00