

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM050119\
 Data File : BM020089.D
 Acq On : 01 May 2019 14:25
 Operator : JU/SJ
 Sample : PB119354BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB119354BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM043019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.369	398	405	415	rBV	2349966	3282612	47.66%	9.128%
2	6.951	666	674	685	rBV	2221895	3416820	49.61%	9.501%
3	7.322	729	737	749	rBV	2293159	3580110	51.98%	9.955%
4	7.793	810	817	823	rVB	375803	610386	8.86%	1.697%
5	8.110	863	871	879	rBV	1794098	2765789	40.16%	7.691%
6	8.957	1007	1015	1025	rBV	1285414	2111010	30.65%	5.870%
7	10.581	1284	1291	1299	rBV	434095	703054	10.21%	1.955%
8	13.051	1704	1711	1719	rBV	3351343	4704338	68.30%	13.081%
9	14.433	1938	1946	1953	rBV2	594511	891768	12.95%	2.480%
10	15.921	2192	2199	2217	rBV	2631781	3567562	51.80%	9.920%
11	17.174	2406	2412	2420	rVB2	767012	1073013	15.58%	2.984%
12	19.804	2854	2859	2865	rBV	6040665	6887371	100.00%	19.151%
13	21.362	3119	3124	3131	rBV	1017797	1200525	17.43%	3.338%
14	23.650	3507	3513	3521	rVB	634912	1168526	16.97%	3.249%


Sum of corrected areas: 35962884

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM050119\
Data File : BM020089.D
Acq On : 01 May 2019 14:25
Operator : JU/SJ
Sample : PB119354BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB119354BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM043019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

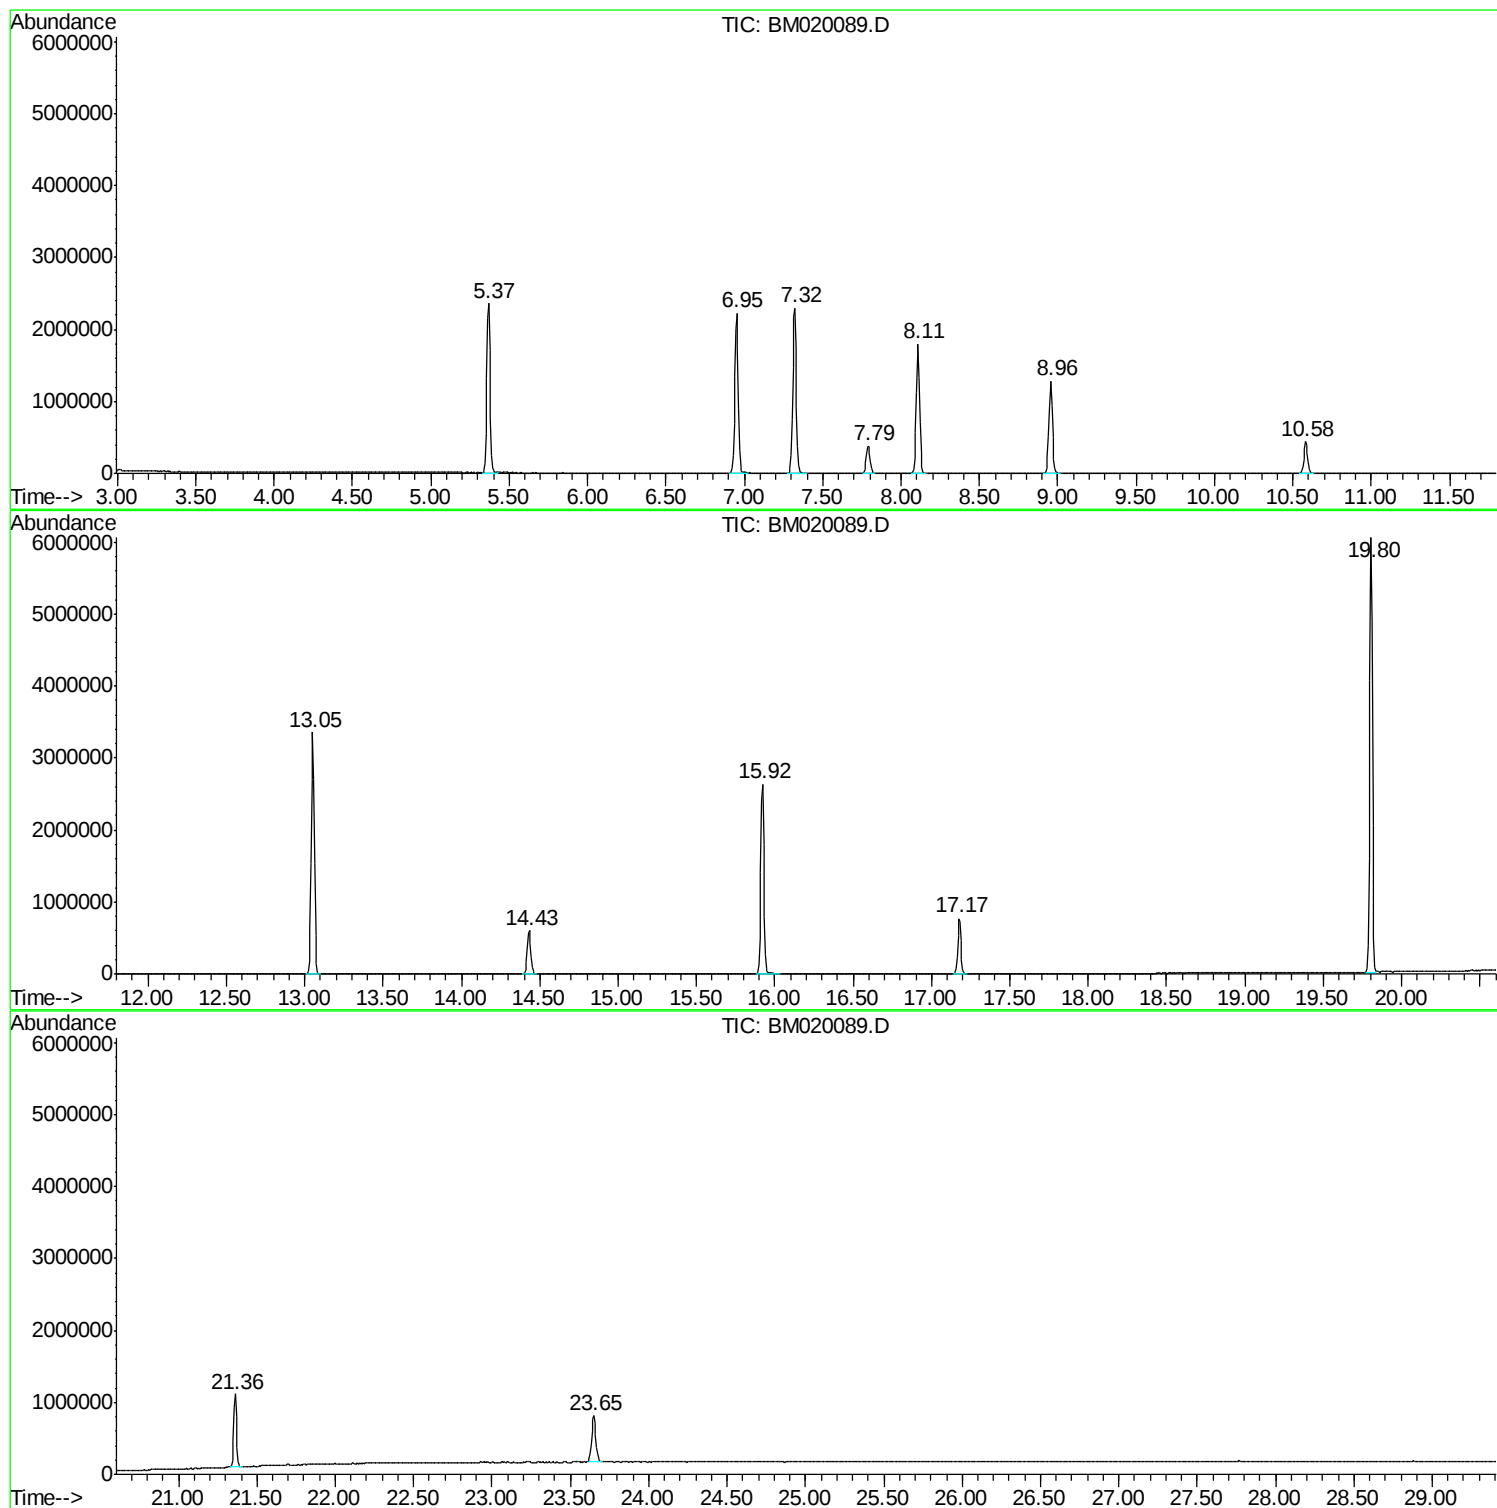

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM050119\
Data File : BM020089.D
Acq On : 01 May 2019 14:25
Operator : JU/SJ
Sample : PB119354BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB119354BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM043019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.32 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.32	117.31 ng	3580110	1,4-Dichlorobenzene-d4	7.79

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	14
2		4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	14
3		1,3,4-Thiadiazole-2(3H)-thione, ...	132	C3H4N2S2	029490-19-5	14
4		3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	14
5		3H-1,2-Dithiol-3-one, 5-methyl-	132	C4H4OS2	003620-08-4	10

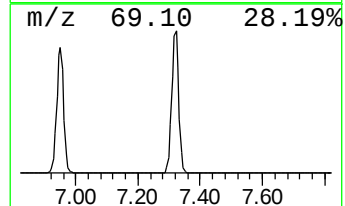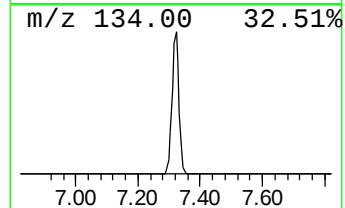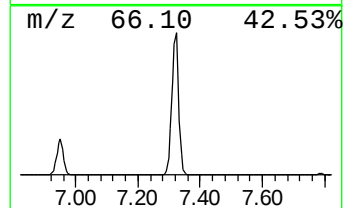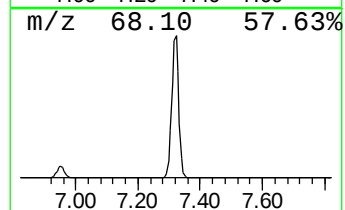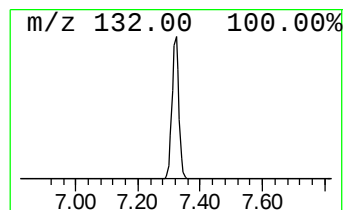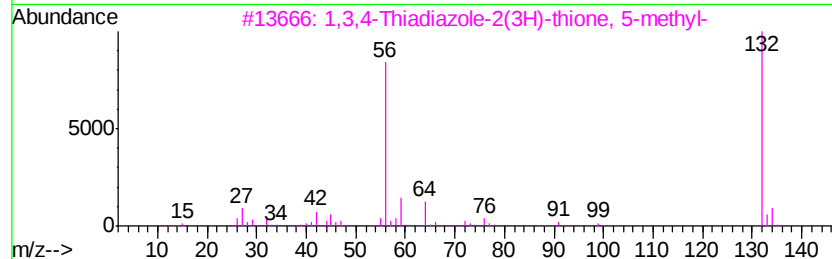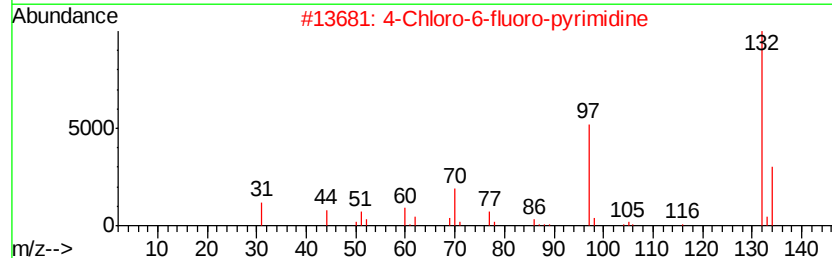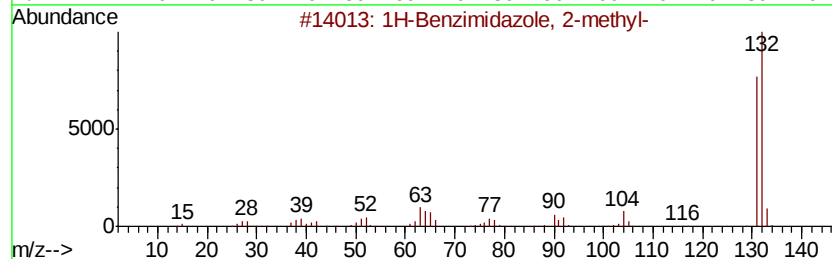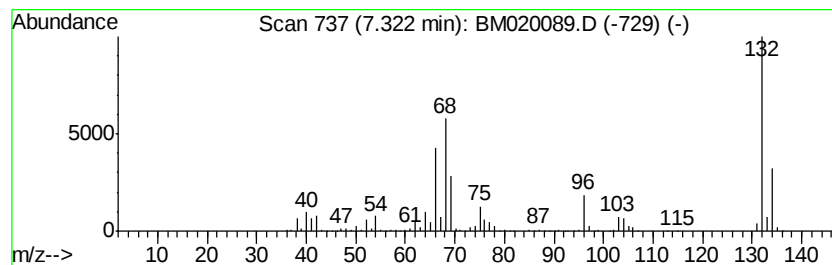

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM050119\
Data File : BM020089.D
Acq On : 01 May 2019 14:25
Operator : JU/SJ
Sample : PB119354BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB119354BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM043019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.32	7.32	117.3	ng	3580110	1	7.79	610386	20.0