


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM050119\
 Data File : BM020085.D
 Acq On : 01 May 2019 11:59
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM043019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 01 03:58:37 2019

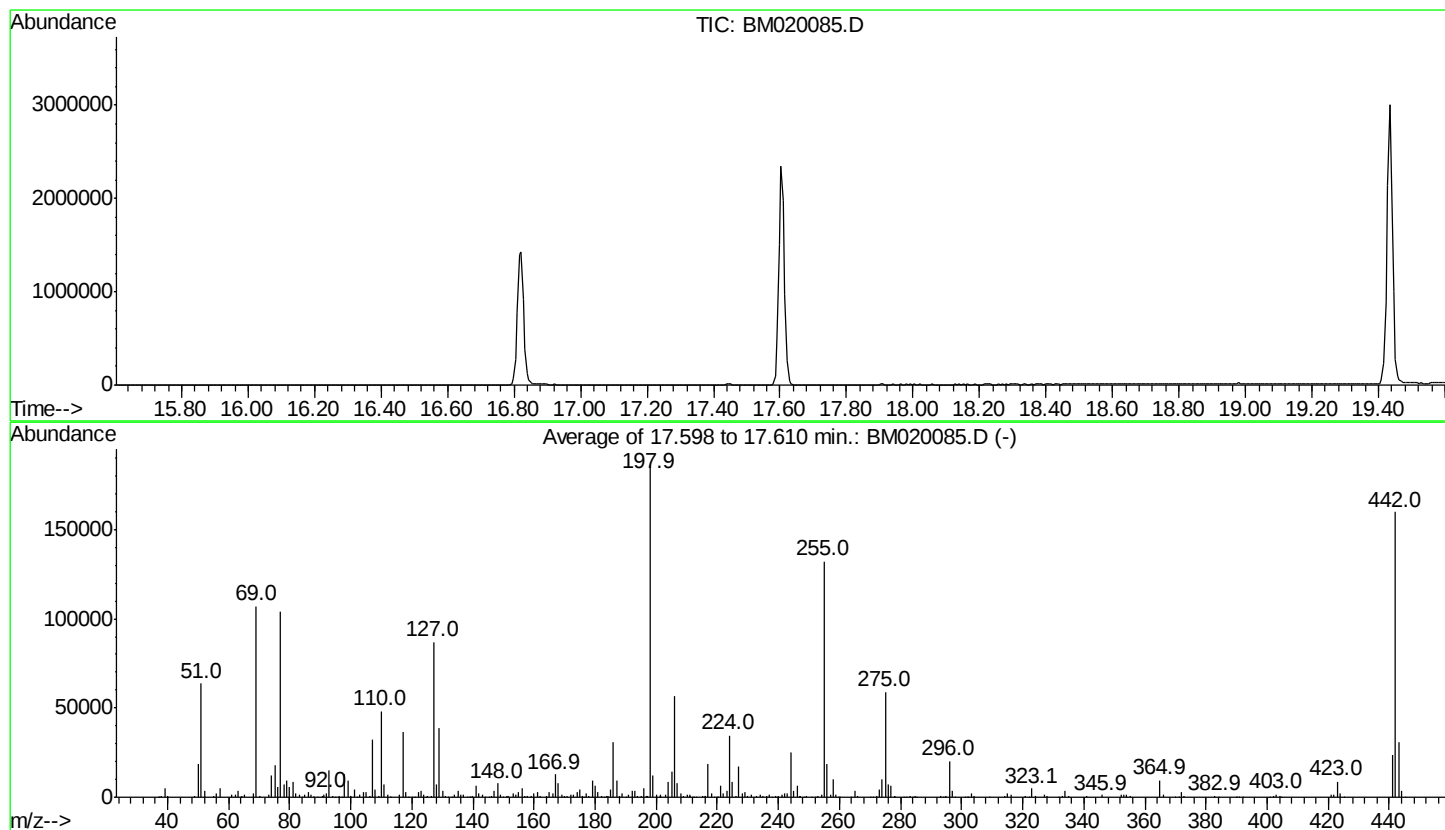

AutoFind: Scans 2484, 2485, 2486; Background Corrected with Scan 2478

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.2	63520	PASS
68	69	0.00	2	1.8	1890	PASS
69	198	0.00	100	57.6	106986	PASS
70	69	0.00	2	0.5	525	PASS
127	198	10	80	46.9	87120	PASS
197	198	0.00	2	0.6	1045	PASS
198	198	100	100	100.0	185770	PASS
199	198	5	9	6.7	12360	PASS
275	198	10	60	31.7	58914	PASS
365	198	1	100	5.1	9407	PASS
441	198	0.01	100	12.6	23418	PASS
442	198	50	100	86.0	159786	PASS
443	442	15	24	19.2	30693	PASS