

Quantitation Report (QT Reviewed)


```
Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM050121\  
Data File : BM029747.D  
Acq On    : 01 May 2021  14:36  
Operator  : CG/JU  
Sample    : SSTD08013  
Misc      :  
ALS Vial  : 6      Sample Multiplier: 1
```

Instrument :
BNA_M
ClientSampleId :
SSTD080013

Manual Integrations APPROVED

mohammad
5/3/2021 12:24:29 PM

Quant Time: May 01 15:08:35 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050121.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat May 01 14:02:00 2021
Response via : Initial Calibration

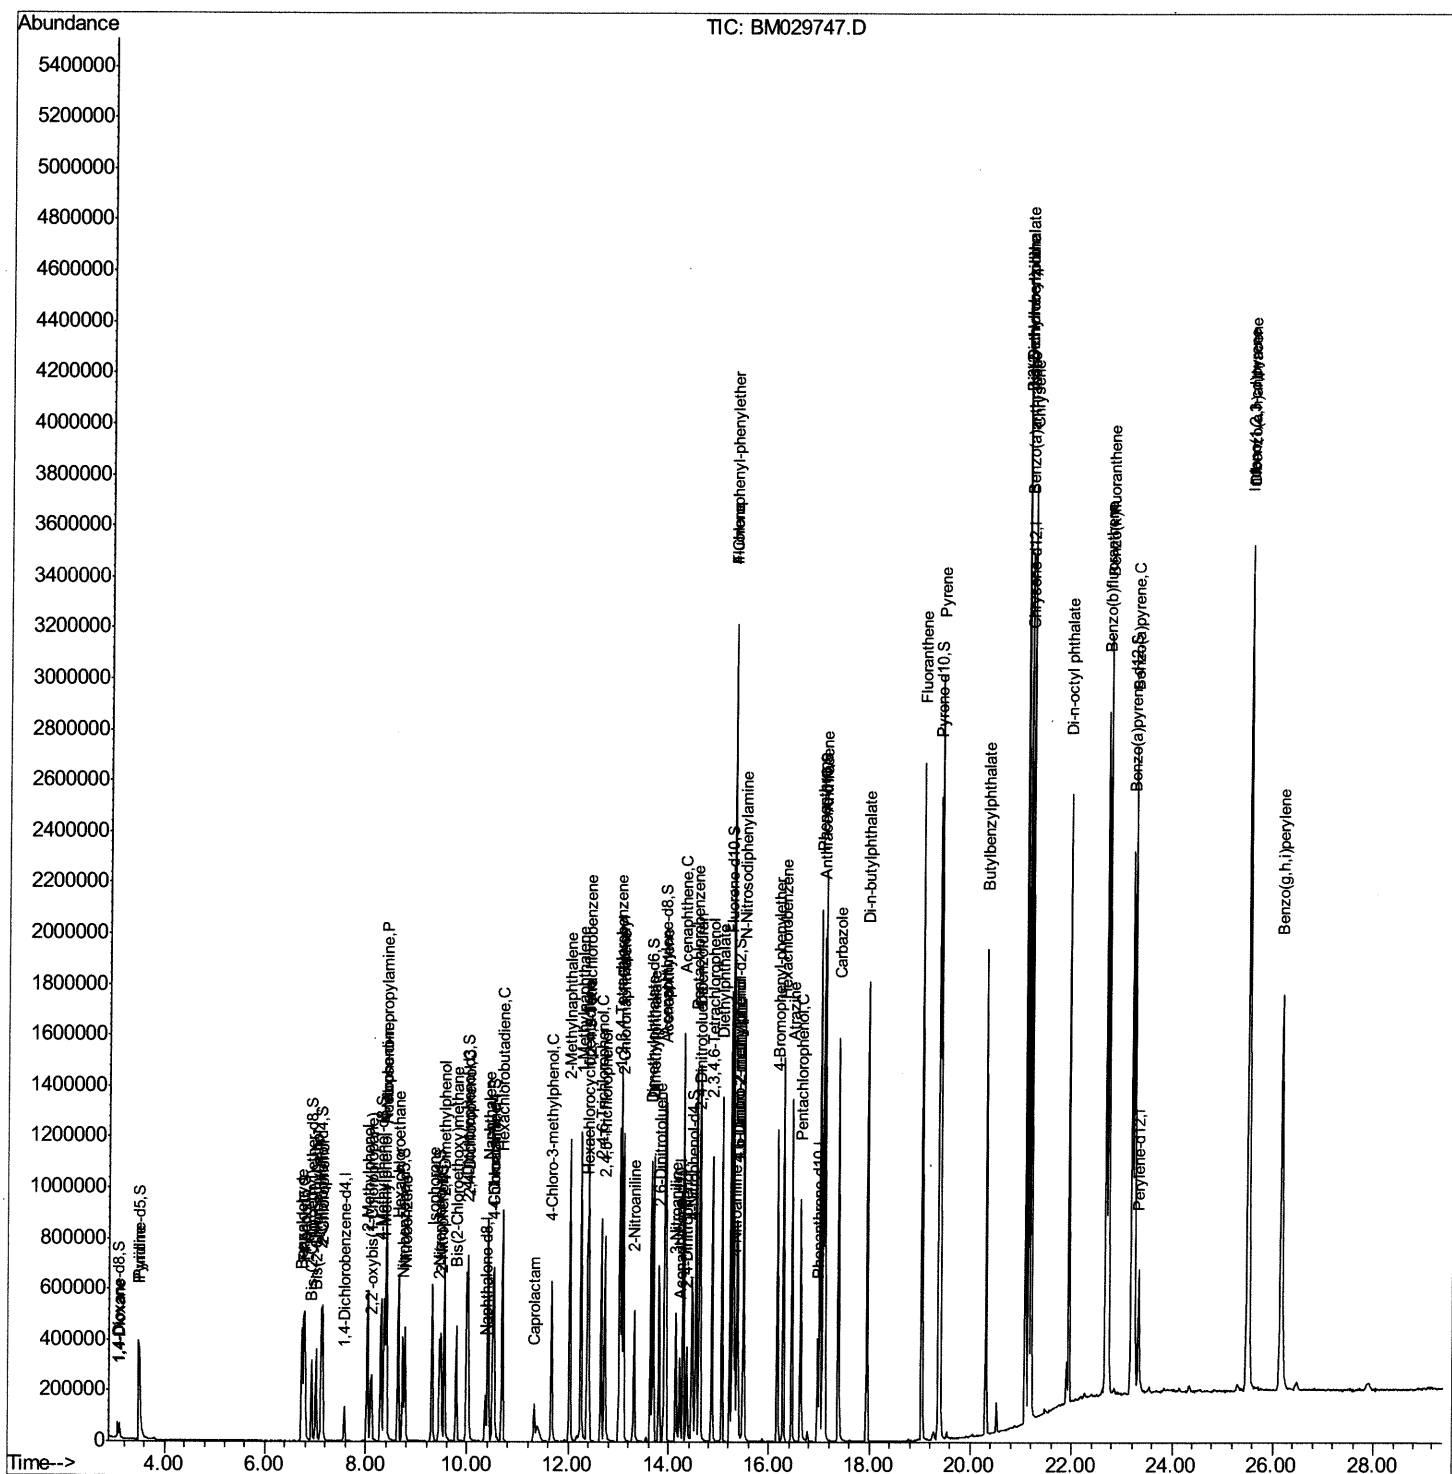

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM050121\
 Data File : BM029747.D
 Acq On : 01 May 2021 14:36
 Operator : CG/JU
 Sample : SSTD08013
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SSTD080013

Manual Integrations
 APPROVED

mohammad
 5/3/2021 12:24:29 PM

Quant Time: May 01 15:07:05 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050121.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat May 01 14:02:00 2021
 Response via : Initial Calibration

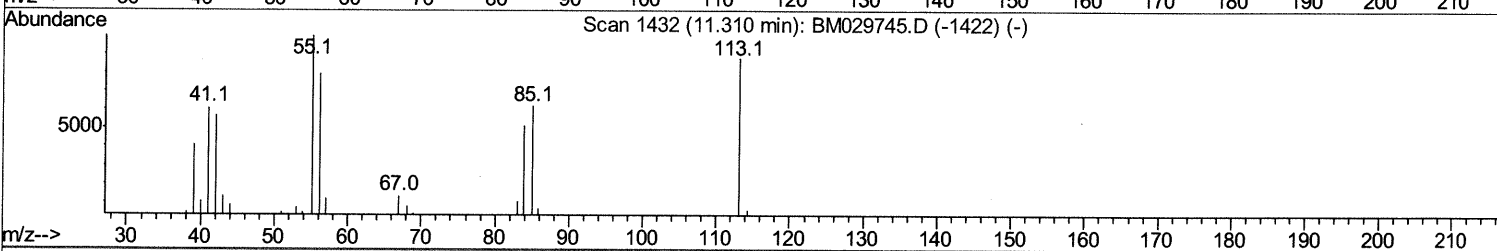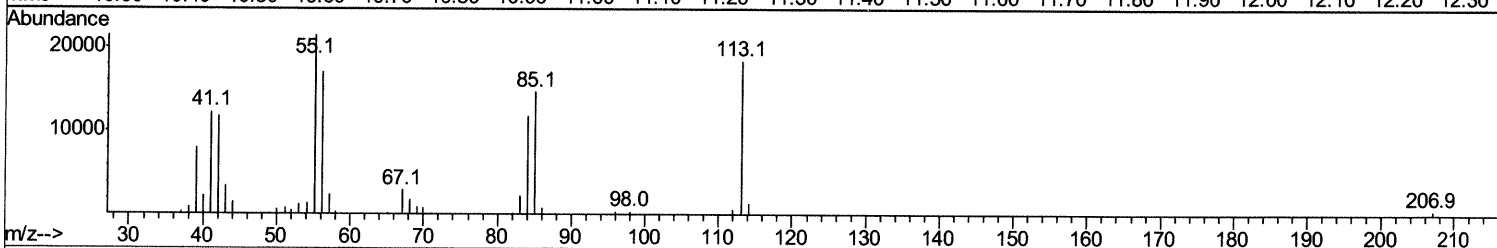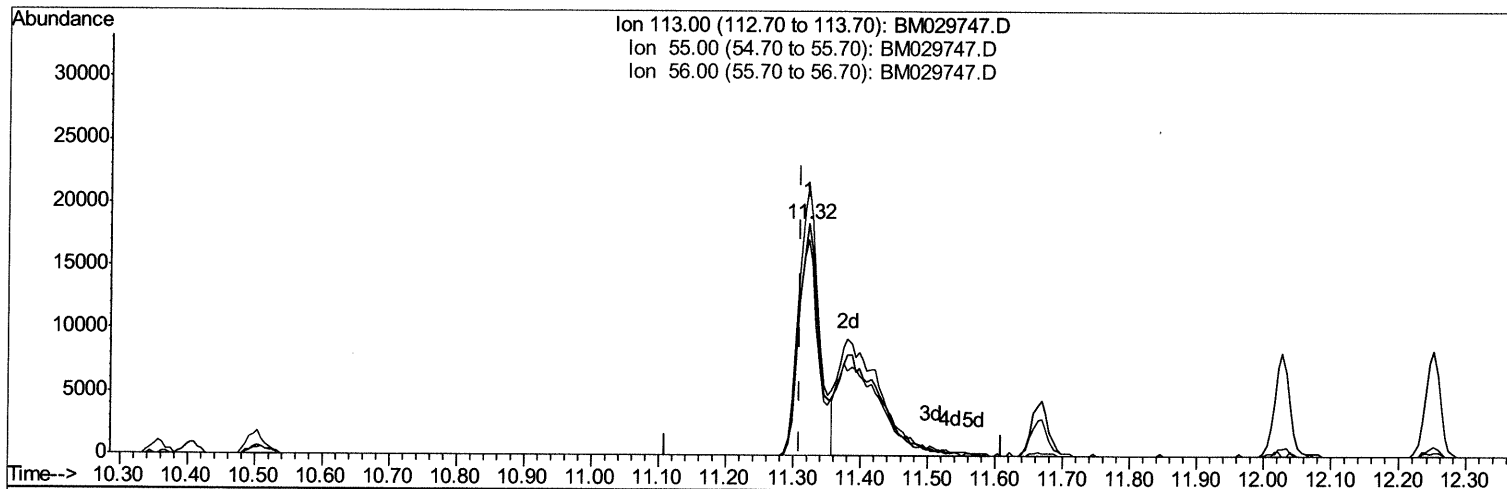

TIC: BM029747.D

(34) Caprolactam

11.322min (+0.012) 57.95ng/ul

response 37987

Ion	Exp%	Act%
113.00	100	100
55.00	113.50	116.52
56.00	90.40	93.09
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM050121\
Data File : BM029747.D
Acq On : 01 May 2021 14:36
Operator : CG/JU
Sample : SST080013
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SST080013

Manual Integrations
APPROVED

mohammad
5/3/2021 12:24:29 PM

Quant Time: May 01 15:07:05 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050121.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat May 01 14:02:00 2021
Response via : Initial Calibration

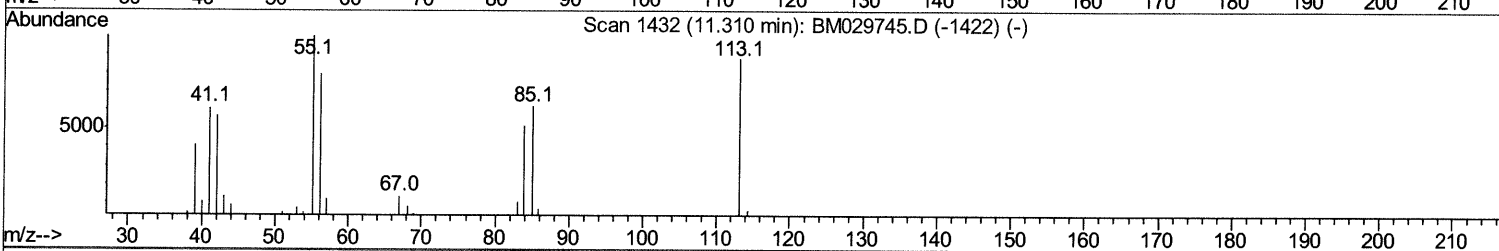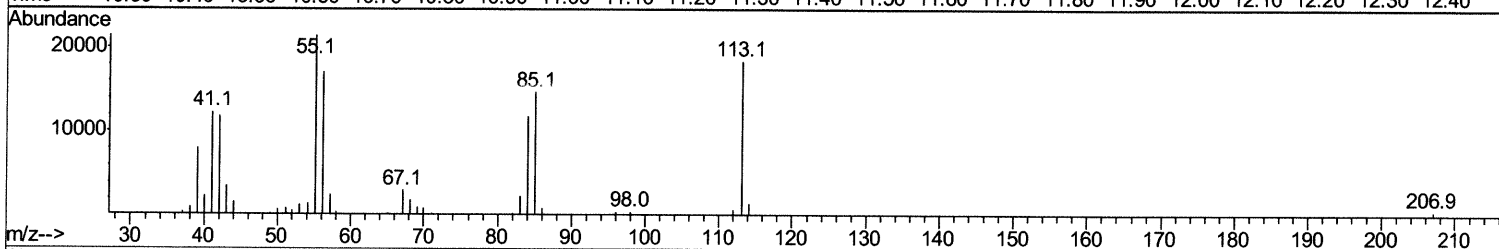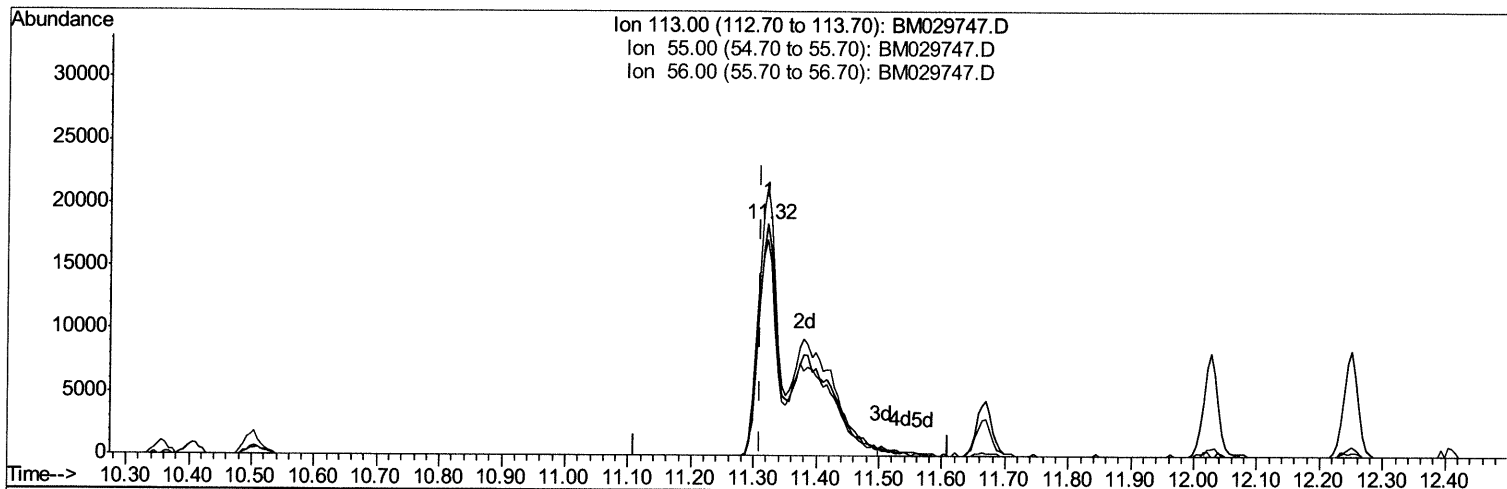

TIC: BM029747.D

(34) Caprolactam

11.322min (+0.012) 111.21ng/ul m 05/04/21 JU

response 72908

Ion	Exp%	Act%
113.00	100	100
55.00	113.50	116.52
56.00	90.40	93.09
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM050121\
Data File : BM029747.D
Acq On : 01 May 2021 14:36
Operator : CG/JU
Sample : SSTD08013
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SSTD080013

Manual Integrations
APPROVED

mohammad
5/3/2021 12:24:29 PM

Quant Time: May 01 15:07:05 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050121.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat May 01 14:02:00 2021
Response via : Initial Calibration

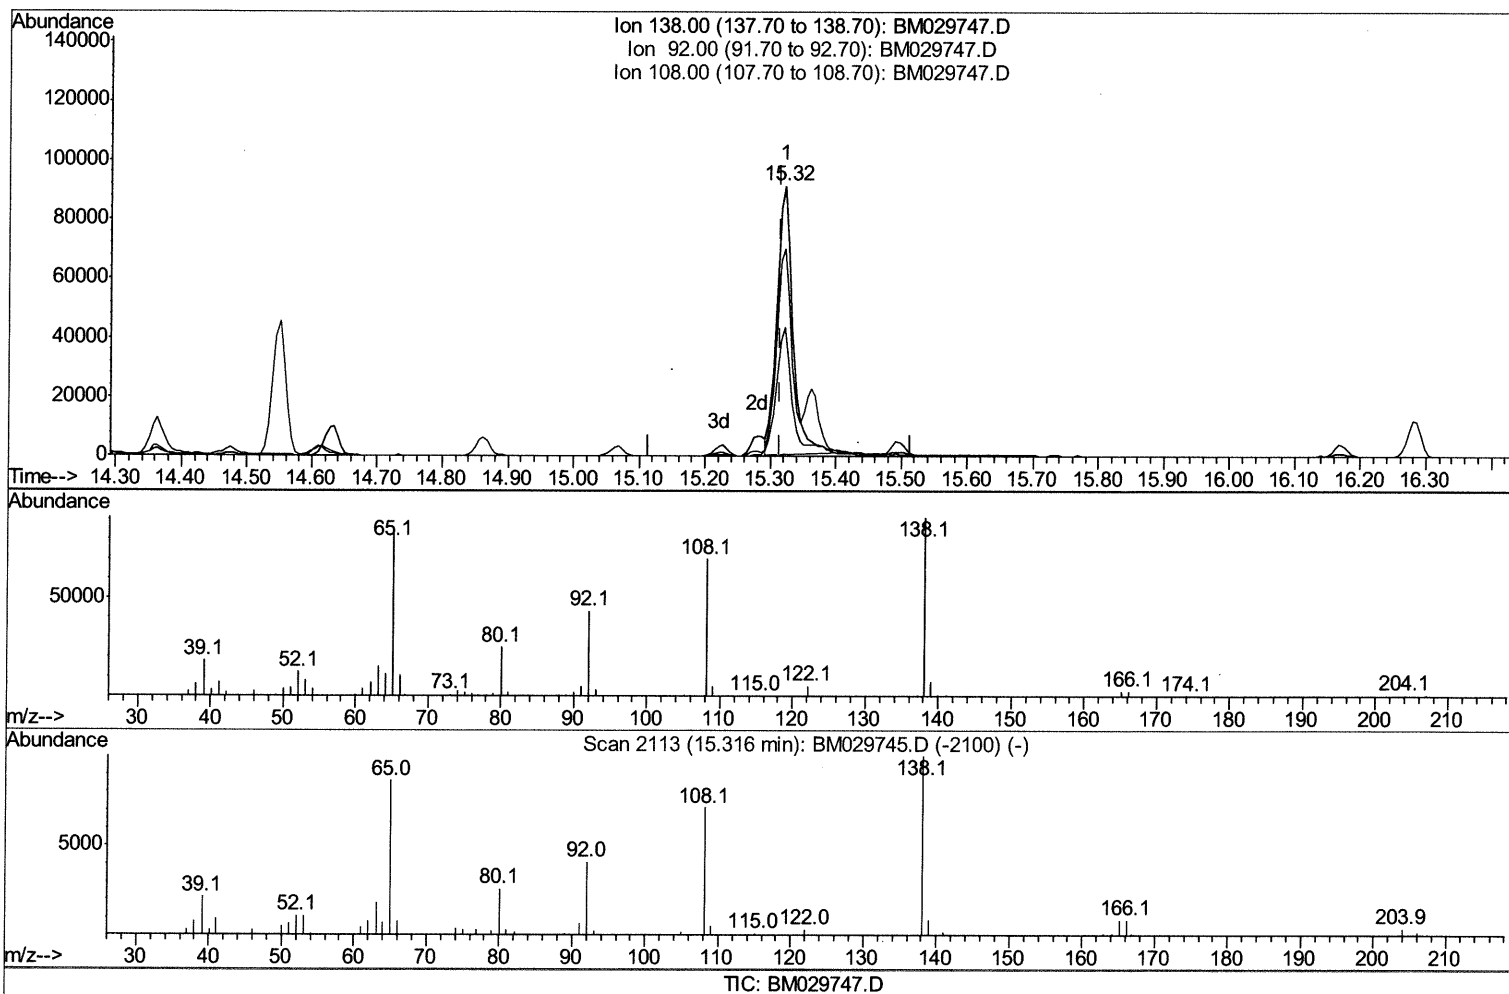

(63) 4-Nitroaniline

15.321min (+0.006) 95.91ng/ul

response 155649

Ion	Exp%	Act%
138.00	100	100
92.00	42.50	47.59
108.00	71.00	76.66
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM050121\
 Data File : BM029747.D
 Acq On : 01 May 2021 14:36
 Operator : CG/JU
 Sample : SST08013
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
ClientSampleId :
 SST080013

Manual Integrations
APPROVED

mohammad
 5/3/2021 12:24:29 PM

Quant Time: May 01 15:07:05 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050121.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat May 01 14:02:00 2021
 Response via : Initial Calibration

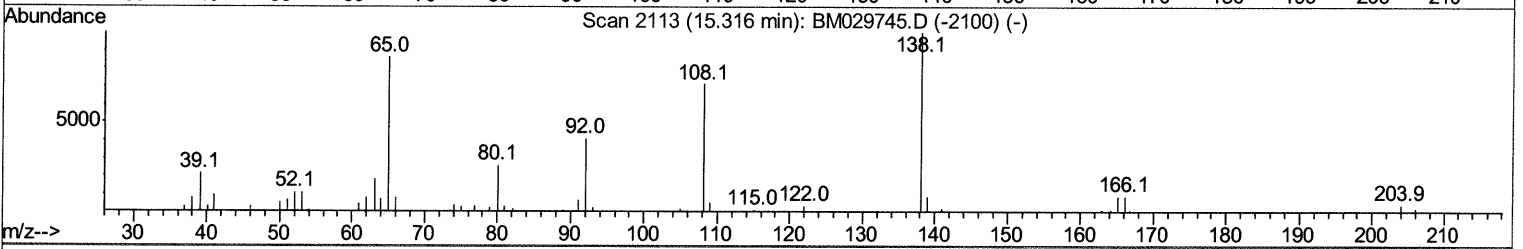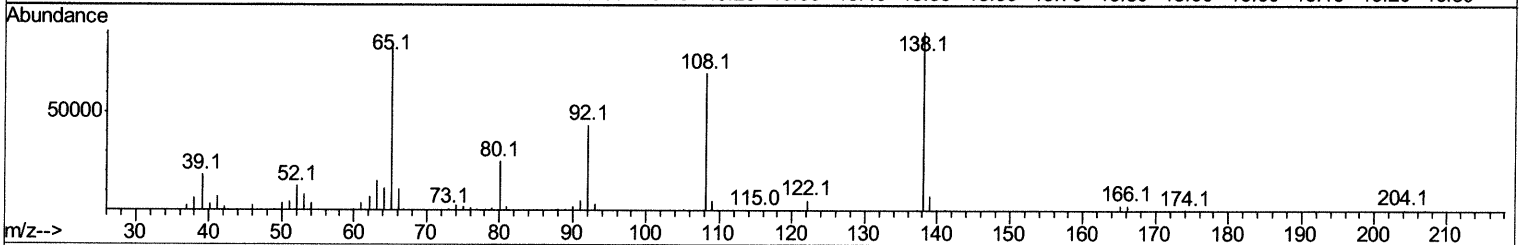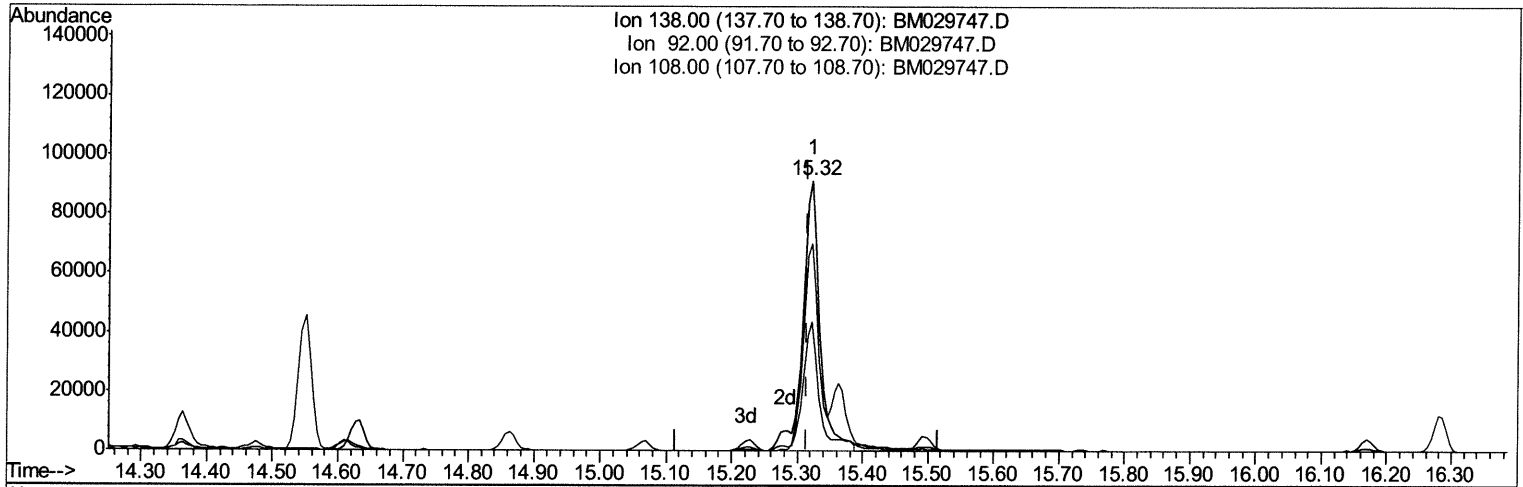

TIC: BM029747.D

(63) 4-Nitroaniline

15.321min (+0.006) 103.74ng/ul m 05/04/21 JU

response 168349

Ion	Exp%	Act%
138.00	100	100
92.00	42.50	47.59
108.00	71.00	76.66
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM050121\
 Data File : BM029747.D
 Acq On : 01 May 2021 14:36
 Operator : CG/JU
 Sample : SST080013
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SST080013

Manual Integrations
 APPROVED

mohammad
 5/3/2021 12:24:29 PM

Quant Time: May 01 15:08:35 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050121.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat May 01 14:02:00 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.58	152	43300	20.00	ng/ul	0.00
20) Naphthalene-d8	10.36	136	160387	20.00	ng/ul	0.00
38) Acenaphthene-d10	14.23	164	117045	20.00	ng/ul	0.00
64) Phenanthrene-d10	16.97	188	265461	20.00	ng/ul	0.00
79) Chrysene-d12	21.16	240	324095	20.00	ng/ul	0.00
88) Perylene-d12	23.33	264	346395	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.08	96	32842	29.81	ng/uL	0.00
4) Pyridine-d5	3.49	84	195528	67.91	ng/ul	-0.01
7) Phenol-d5	6.77	99	271049	79.26	ng/ul	0.00
9) Bis-(2-Chloroethyl)ether-d	6.92	67	136687	69.16	ng/ul	0.00
11) 2-Chlorophenol-d4	7.12	132	249281	93.66	ng/ul	0.00
15) 4-Methylphenol-d8	8.30	113	229743	86.56	ng/ul	0.01
21) Nitrobenzene-d5	8.73	128	116031	113.74	ng/ul	0.00
24) 2-Nitrophenol-d4	9.45	143	149837	154.07	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.99	165	303494	119.10	ng/ul	0.00
31) 4-Chloroaniline-d4	10.50	131	323211	89.65	ng/ul	0.00
46) Dimethylphthalate-d6	13.65	166	848316	96.10	ng/ul	0.00
49) Acenaphthylene-d8	13.92	160	1060617	101.63	ng/ul	0.00
54) 4-Nitrophenol-d4	14.46	143	130522	90.79	ng/ul	0.00
60) Fluorene-d10	15.23	176	745309	98.11	ng/ul	0.00
65) 4,6-Dinitro-2-methylphenol	15.36	200	186406	148.95	ng/ul	0.00
73) Anthracene-d10	17.07	188	1223431	96.51	ng/ul	0.00
81) Pyrene-d10	19.37	212	1507419	99.66	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.19	264	1789042	97.02	ng/ul	0.00

Target Compounds

					Ovalue
2) 1,4-Dioxane	3.11	88	33394	30.197	ng/uL 94
5) Pyridine	3.50	79	199963	67.600	ng/ul 94
6) Benzaldehyde	6.73	77	159333	86.827	ng/ul 97
8) Phenol	6.79	94	267814	74.518	ng/ul 97
10) Bis(2-Chloroethyl)ether	7.02	93	203355	76.575	ng/ul 97
12) 2-Chlorophenol	7.15	128	246970	86.976	ng/ul 99
13) 2-Methylphenol	8.03	108	212859	80.293	ng/ul 99
14) 2,2'-oxybis(1-Chloropropan	8.11	45	187531	53.877	ng/ul 98
16) Acetophenone	8.40	105	348073	80.241	ng/ul 98
17) N-Nitroso-di-n-propylamine	8.40	70	169096	81.952	ng/ul 97
18) 4-Methylphenol	8.37	108	231924	82.392	ng/ul 92
19) Hexachloroethane	8.65	117	104240	85.710	ng/ul 95
22) Nitrobenzene	8.78	77	246502	82.878	ng/ul 97
23) Isophorone	9.31	82	463492	87.222	ng/ul 100
25) 2-Nitrophenol	9.48	139	150410	134.240	ng/ul 99
26) 2,4-Dimethylphenol	9.55	107	260776	85.642	ng/ul 99
27) Bis(2-Chloroethoxy)methane	9.79	93	271502	85.527	ng/ul 98
29) 2,4-Dichlorophenol	10.02	162	287511	111.470	ng/ul 95
30) Naphthalene	10.40	128	763482	87.869	ng/ul 99
32) 4-Chloroaniline	10.53	127	324038	88.373	ng/ul 98
33) Hexachlorobutadiene	10.69	225	225145	121.560	ng/ul 99
34) Caprolactam	11.32	113	72908m	111.215	ng/ul > 05/04/21 04

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM050121\
 Data File : BM029747.D
 Acq On : 01 May 2021 14:36
 Operator : CG/JU
 Sample : SST080013
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SST080013

Manual Integrations
 APPROVED

mohammad
 5/3/2021 12:24:29 PM

Quant Time: May 01 15:08:35 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050121.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat May 01 14:02:00 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
35) 4-Chloro-3-methylphenol	11.67	107	236816	94.515	ng/ul	97
36) 2-Methylnaphthalene	12.03	142	591305	96.331	ng/ul	97
37) 1-Methylnaphthalene	12.25	142	581793	95.999	ng/ul	97
39) 1,2,4,5-Tetrachlorobenzene	12.40	216	426648	105.496	ng/ul	100
40) Hexachlorocyclopentadiene	12.38	237	236606	89.065	ng/ul	93
41) 2,4,6-Trichlorophenol	12.66	196	261136	117.429	ng/ul	94
42) 2,4,5-Trichlorophenol	12.73	196	274375	115.865	ng/ul	97
43) 1,1'-Biphenyl	13.06	154	807388	84.733	ng/ul	99
44) 2-Chloronaphthalene	13.10	162	653660	86.896	ng/ul	99
45) 2-Nitroaniline	13.31	65	142323	88.191	ng/ul	97
47) Dimethylphthalate	13.70	163	821557	90.929	ng/ul	100
48) 2,6-Dinitrotoluene	13.82	165	179923	127.955	ng/ul	93
50) Acenaphthylene	13.95	152	974344	90.279	ng/ul	99
51) 3-Nitroaniline	14.15	138	161954	104.150	ng/ul	92
52) Acenaphthene	14.29	153	675527	84.290	ng/ul	99
53) 2,4-Dinitrophenol	14.36	184	114726	152.046	ng/ul#	92
55) 4-Nitrophenol	14.47	109	92888	67.911	ng/ul	89
56) Dibenzofuran	14.63	168	1016028	91.226	ng/ul	99
57) 2,4-Dinitrotoluene	14.61	165	256104	127.637	ng/ul	97
58) 2,3,4,6-Tetrachlorophenol	14.86	232	260877	137.476	ng/ul	97
59) Diethylphthalate	15.07	149	774729	87.091	ng/ul	98
61) Fluorene	15.28	166	850199	91.237	ng/ul	100
62) 4-Chlorophenyl-phenylether	15.28	204	483471	103.364	ng/ul	95
63) 4-Nitroaniline	15.32	138	168349m	103.739	ng/ul>	05/04/21 JU
66) 4,6-Dinitro-2-methylphenol	15.38	198	177239	134.642	ng/ul#	98
67) N-Nitrosodiphenylamine	15.50	169	745913	87.962	ng/ul	99
68) 4-Bromophenyl-phenylether	16.17	248	299012	105.851	ng/ul	96
69) Hexachlorobenzene	16.29	284	341593	108.552	ng/ul	97
70) Atrazine	16.46	200	306026	94.203	ng/ul	100
71) Pentachlorophenol	16.63	266	199526	111.658	ng/ul	98
72) Phenanthrene	17.02	178	1364224	87.048	ng/ul	100
74) Anthracene	17.11	178	1430156	88.807	ng/ul	99
75) 1,2,3,4-Tetrachlorobenzene	13.02	216	447896	104.477	ng/uL	97
76) Pentachlorobenzene	14.55	250	415828	99.352	ng/uL	98
77) Carbazole	17.39	167	1228071	82.851	ng/ul	99
78) Di-n-butylphthalate	17.95	149	1349920	88.170	ng/ul	100
80) Fluoranthene	19.03	202	1777251	91.455	ng/ul	99
82) Pyrene	19.40	202	1856553	91.143	ng/ul	100
83) Butylbenzylphthalate	20.30	149	641081	89.562	ng/ul	98
84) 3,3'-Dichlorobenzidine	21.08	252	755842	112.617	ng/ul	99
85) Benzo(a)anthracene	21.14	228	1893038	90.541	ng/ul	99
86) Bis(2-ethylhexyl)phthalate	21.09	149	970222	82.489	ng/ul	97
87) Chrysene	21.20	228	1881593	92.046	ng/ul	100
89) Di-n-octyl phthalate	21.94	149	1703123	77.076	ng/ul	100
90) Benzo(b)fluoranthene	22.68	252	2035940	90.944	ng/ul	99
91) Benzo(k)fluoranthene	22.73	252	2014728	90.070	ng/ul	99
93) Benzo(a)pyrene	23.24	252	1843510	90.877	ng/ul	99
94) Indeno(1,2,3-cd)pyrene	25.51	276	2468045	90.476	ng/ul	99
95) Dibenzo(a,h)anthracene	25.52	278	2071590	90.007	ng/ul	99
96) Benzo(g,h,i)perylene	26.17	276	2013769	90.008	ng/ul	99

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM050121\
Data File : BM029747.D
Acq On : 01 May 2021 14:36
Operator : CG/JU
Sample : SSTD08013
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SSTD080013

Manual Integrations
APPROVED

mohammad
5/3/2021 12:24:29 PM

Quant Time: May 01 15:08:35 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050121.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat May 01 14:02:00 2021
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
--------------------	------	------	----------	------	-------	-----------

(#) = qualifier out of range (m) = manual integration (+) = signals summed