

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM050121\
 Data File : BM029764.D
 Acq On : 02 May 2021 02:04
 Operator : CG/JU
 Sample : M2065-12
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BG565

Manual Integrations
 APPROVED

mohammad
 5/3/2021 12:24:58 PM

Quant Time: May 02 08:21:35 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050121.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun May 02 01:03:03 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.57	152	43284	20.00	ng/ul	0.00
20) Naphthalene-d8	10.35	136	161088	20.00	ng/ul	0.00
38) Acenaphthene-d10	14.22	164	126216	20.00	ng/ul	0.00
64) Phenanthrene-d10	16.97	188	298826	20.00	ng/ul	0.00
79) Chrysene-d12	21.15	240	351892	20.00	ng/ul	0.00
88) Perylene-d12	23.31	264	377010	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.08	96	2621m	2.96	ng/uL	0.00
4) Pyridine-d5	3.56	84	4446m	2.32	ng/ul	0.06
7) Phenol-d5	6.76	99	39732	13.63	ng/ul	0.00
9) Bis-(2-Chloroethyl)ether-d	6.92	67	22443	14.70	ng/ul	0.00
11) 2-Chlorophenol-d4	7.12	132	39665	15.05	ng/ul	0.00
15) 4-Methylphenol-d8	8.30	113	29833	11.95	ng/ul	0.00
21) Nitrobenzene-d5	8.73	128	17746	15.13	ng/ul	0.00
24) 2-Nitrophenol-d4	9.45	143	21930	14.77	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.99	165	41733	13.45	ng/ul	0.00
31) 4-Chloroaniline-d4	10.51	131	39772	11.37	ng/ul	0.00
46) Dimethylphthalate-d6	13.64	166	177972	17.80	ng/ul	0.00
49) Acenaphthylene-d8	13.92	160	200724	16.28	ng/ul	0.00
54) 4-Nitrophenol-d4	14.48	143	8833m	6.68	ng/ul	0.02
60) Fluorene-d10	15.22	176	154987	17.92	ng/ul	0.00
65) 4,6-Dinitro-2-methylphenol	15.36	200	15040	6.92	ng/ul	0.00
73) Anthracene-d10	17.07	188	248746	16.51	ng/ul	0.00
81) Pyrene-d10	19.36	212	326551	18.17	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.18	264	365207	16.88	ng/ul	0.00
Target Compounds						
47) Dimethylphthalate	13.69	163	26624	2.746	ng/ul	Ovalue 99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM050121\
Data File : BM029764.D
Acq On : 02 May 2021 02:04
Operator : CG/JU
Sample : M2065-12
Misc :
ALS Vial : 14 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampled :
BG565

Manual Integrations
APPROVED

mohammad
5/3/2021 12:24:58 PM

Quant Time: May 02 08:21:35 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050121.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun May 02 01:03:03 2021
Response via : Initial Calibration

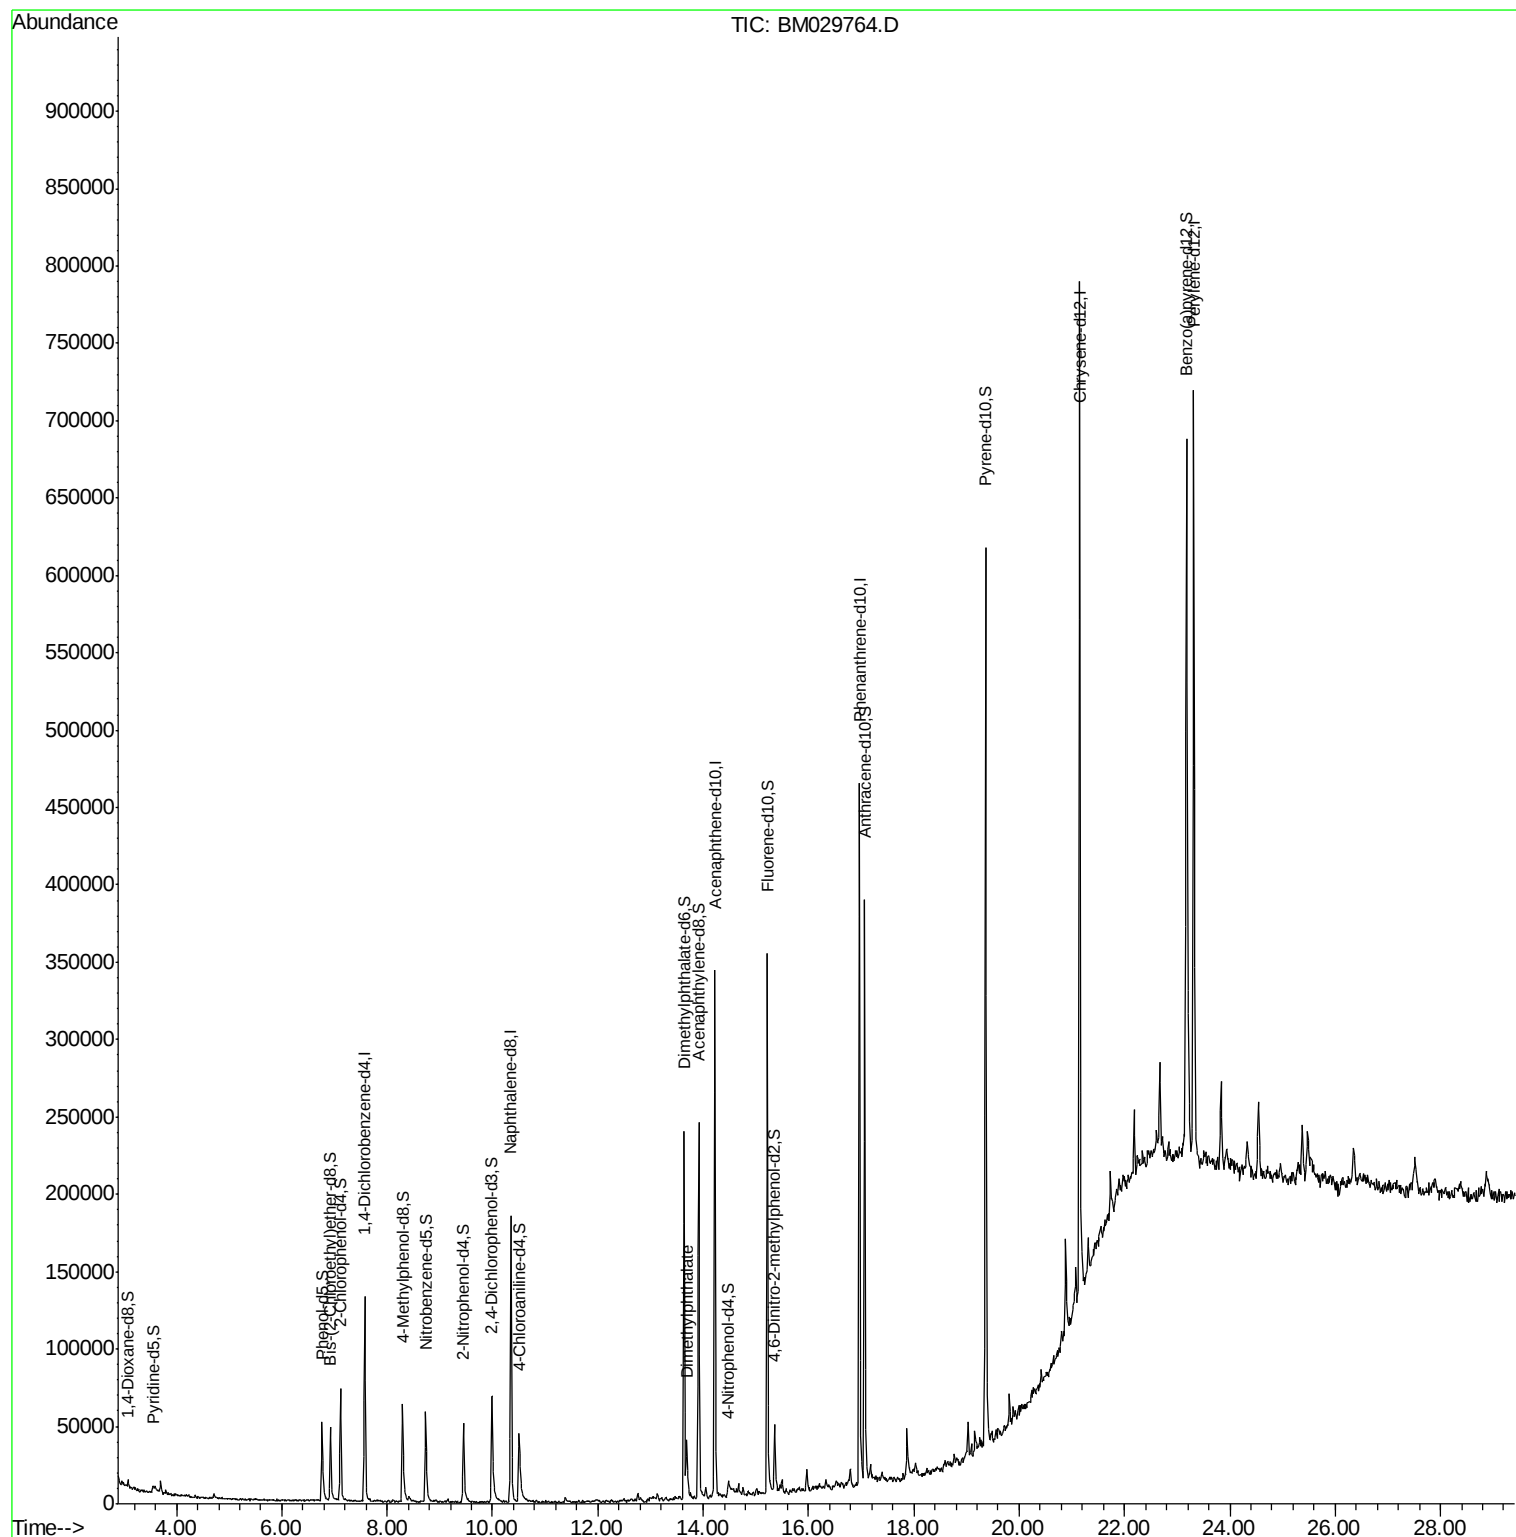

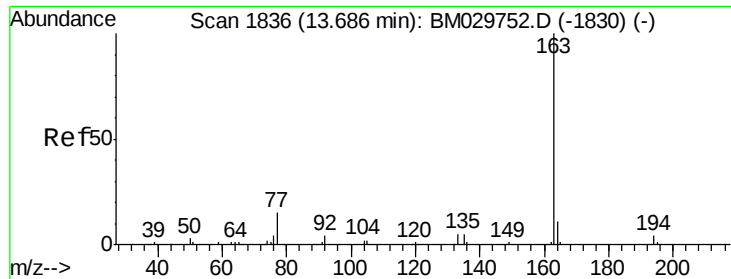

#47
 Dimethylphthalate
 Concen: 2.746 ng/ul
 RT: 13.69 min Scan# 1837
 Delta R.T. -0.00 min
 Lab File: BM029764.D
 Acq: 02 May 2021 02:04

Instrument :
 BNA_M
 ClientSampleId :
 BG565

Tot Ion	Ratio	Lower	Upper
163	100		
194	4.7	3.7	5.5
164	9.5	8.0	12.0

Manual Integrations
 APPROVED

mohammad
 5/3/2021 12:24:58 PM

