

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050121\
 Data File : BM029753.D
 Acq On : 01 May 2021 19:26
 Operator : CG/JU
 Sample : PB135972BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK972

Integration Parameters: LSCINT.P

Integrator: RTE

Smoother: OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050121.M
 Title : SVOA CALIBRATION

Signal : TIC: BM029753.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.081	29	33	44	rVB2	13268	24218	1.36%	0.176%
2	3.499	101	104	121	rBV	82181	181055	10.15%	1.313%
3	3.799	153	155	161	rVB2	3604	4369	0.24%	0.032%
4	6.763	653	659	674	rBV	144337	262809	14.74%	1.906%
5	6.922	680	686	698	rBV	114129	193925	10.87%	1.407%
6	7.110	712	718	732	rBV	176718	309543	17.36%	2.245%
7	7.575	790	797	808	rBV	156780	264811	14.85%	1.921%
8	8.292	913	919	935	rBV2	181932	341325	19.14%	2.476%
9	8.398	935	937	941	rVB4	1436	1934	0.11%	0.014%
10	8.734	987	994	1003	rBV	144029	257191	14.42%	1.866%
11	9.451	1110	1116	1131	rBV	128963	238804	13.39%	1.732%
12	9.986	1201	1207	1228	rBV	191314	384480	21.56%	2.789%
13	10.351	1261	1269	1280	rBV	205712	356196	19.97%	2.584%
14	10.504	1288	1295	1317	rBV	143542	347271	19.47%	2.519%
15	11.975	1541	1545	1551	rBV3	1806	3348	0.19%	0.024%
16	13.645	1822	1829	1844	rBV	426364	656592	36.81%	4.763%
17	13.916	1868	1875	1886	rBV	528618	811421	45.50%	5.886%
18	14.227	1921	1928	1942	rBV	358844	553478	31.03%	4.015%
19	14.463	1961	1968	1982	rBV2	46927	144749	8.12%	1.050%
20	15.221	2090	2097	2107	rBV	711473	1035104	58.04%	7.509%
21	15.357	2115	2120	2132	rBV	154928	245801	13.78%	1.783%
22	15.463	2134	2138	2144	rVB	8078	11796	0.66%	0.086%
23	16.010	2228	2231	2235	rVB3	2943	3892	0.22%	0.028%
24	16.762	2355	2359	2362	rVB2	1266	1830	0.10%	0.013%
25	16.968	2388	2394	2405	rBV	493515	692002	38.80%	5.020%
26	17.068	2405	2411	2429	rVV	758644	1151776	64.58%	8.355%
27	19.004	2736	2740	2743	rBV2	6677	8842	0.50%	0.064%
28	19.251	2779	2782	2787	rVB	5793	7542	0.42%	0.055%
29	19.362	2795	2801	2815	rBV	1060064	1536271	86.14%	11.144%
30	21.156	3101	3106	3117	rBV	618566	922250	51.71%	6.690%
31	23.186	3444	3451	3465	rBV	954924	1783525	100.00%	12.938%
32	23.321	3468	3474	3486	rVB	533892	1047189	58.71%	7.596%




Sum of corrected areas: 13785339

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050121\
Data File : BM029753.D
Acq On : 01 May 2021 19:26
Operator : CG/JU
Sample : PB135972BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK972

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050121.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

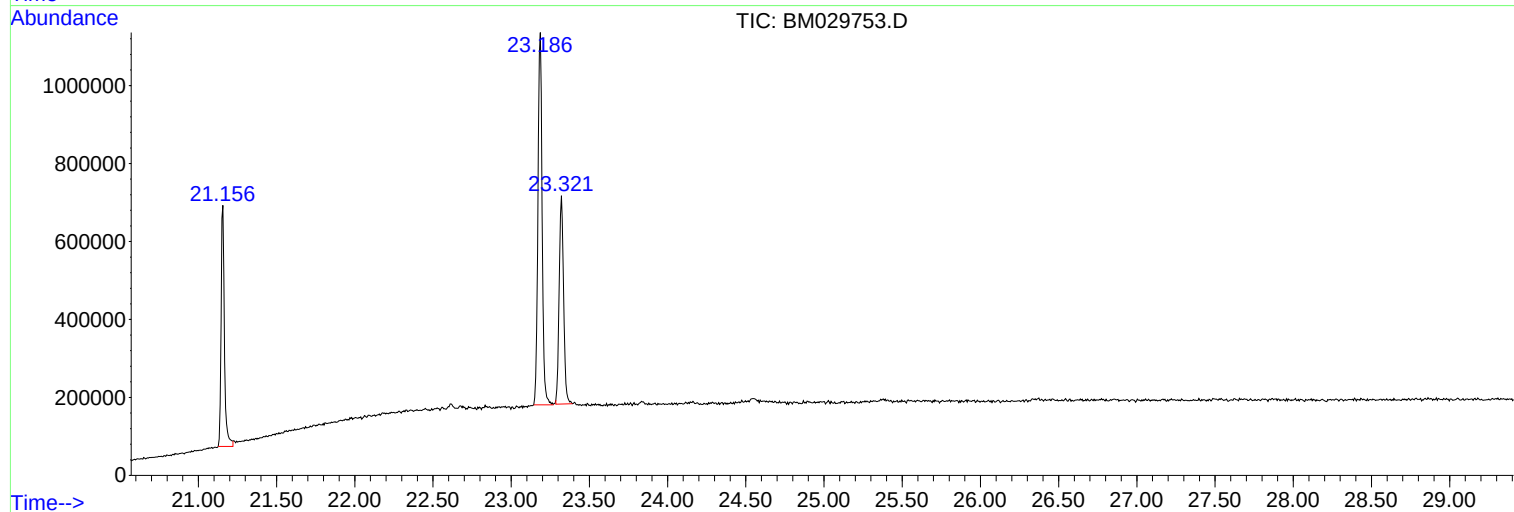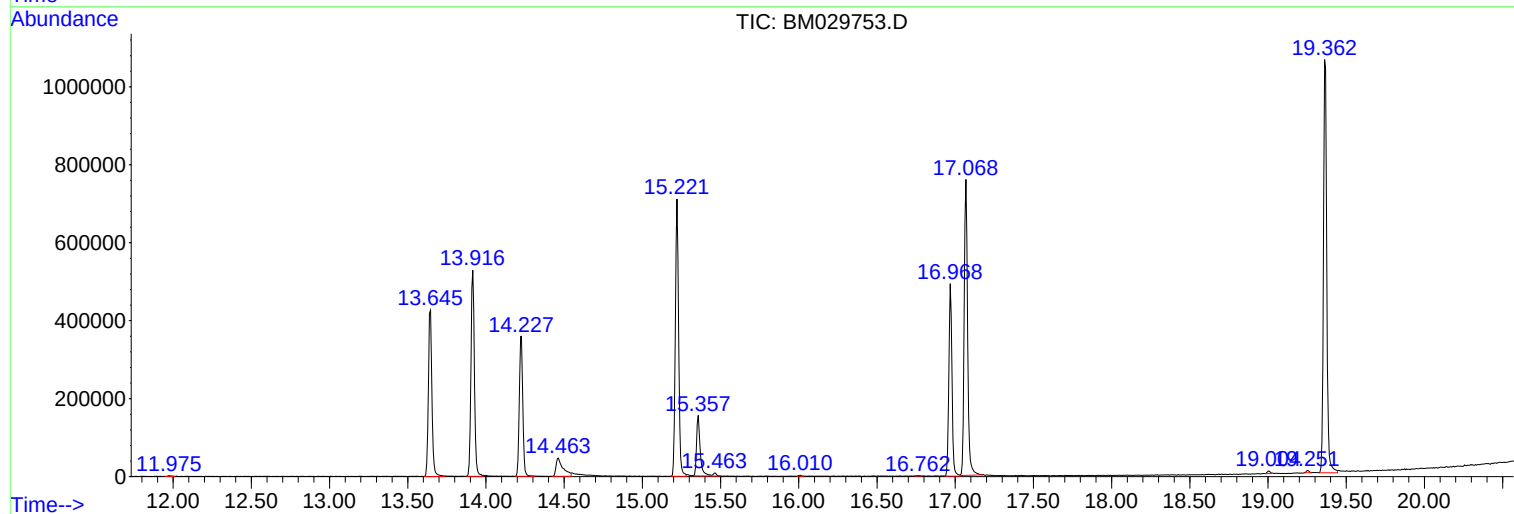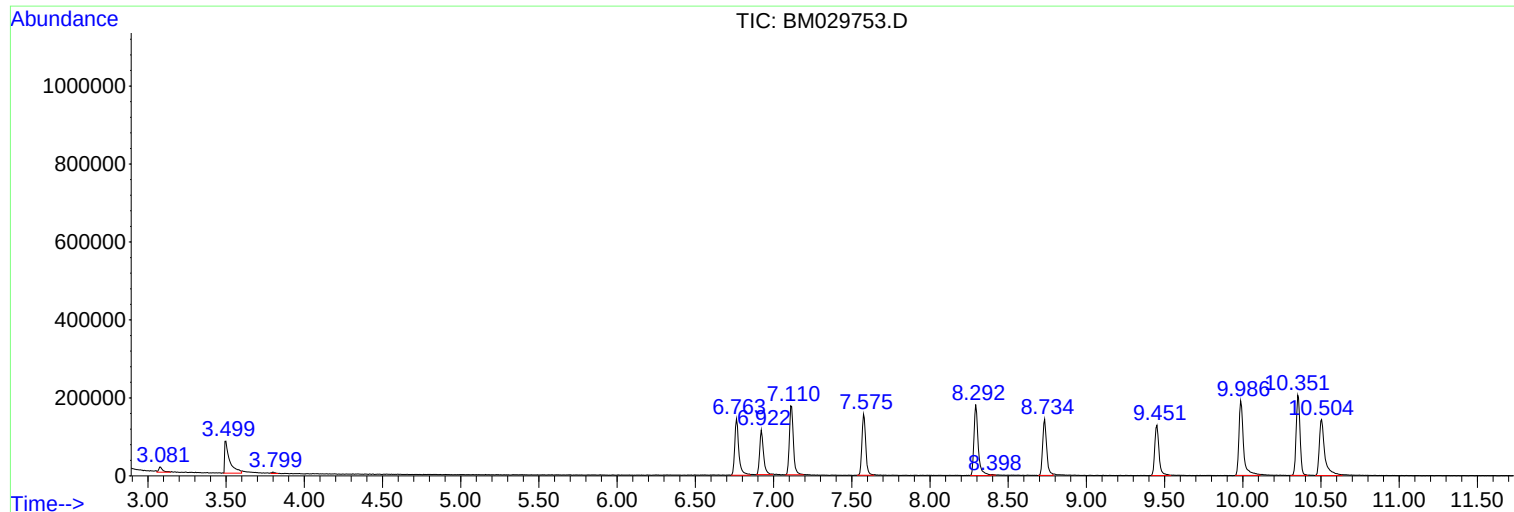

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050121\
Data File : BM029753.D
Acq On : 01 May 2021 19:26
Operator : CG/JU
Sample : PB135972BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK972

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050121.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050121\
Data File : BM029753.D
Acq On : 01 May 2021 19:26
Operator : CG/JU
Sample : PB135972BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK972

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050121.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
