

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM050121\
 Data File : BM029758.D
 Acq On : 01 May 2021 22:26
 Operator : CG/JU
 Sample : PB135930BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK930

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050121.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.075	29	32	40	rVB	12602	15975	0.79%	0.100%
2	3.493	100	103	123	rBV	89787	199622	9.90%	1.255%
3	3.793	152	154	158	rVB3	2562	2825	0.14%	0.018%
4	6.763	652	659	672	rBV	155190	284037	14.09%	1.786%
5	6.922	680	686	699	rBV	126663	220016	10.91%	1.383%
6	7.110	712	718	733	rBV	200258	341512	16.94%	2.147%
7	7.304	749	751	758	rBV5	1111	2097	0.10%	0.013%
8	7.575	791	797	813	rBV	180788	295854	14.67%	1.860%
9	8.293	912	919	936	rBV	205932	382592	18.98%	2.406%
10	8.734	987	994	1016	rBV	161391	299874	14.87%	1.886%
11	9.445	1109	1115	1130	rBV	147831	271640	13.47%	1.708%
12	9.986	1201	1207	1227	rBV	230294	448968	22.27%	2.823%
13	10.351	1262	1269	1280	rBV	243659	406646	20.17%	2.557%
14	10.498	1288	1294	1315	rBV	176415	393427	19.51%	2.474%
15	11.975	1539	1545	1550	rBV2	2317	4305	0.21%	0.027%
16	13.645	1822	1829	1842	rBV	511444	783892	38.88%	4.929%
17	13.916	1868	1875	1885	rBV	636883	939524	46.60%	5.908%
18	14.222	1921	1927	1940	rBV	439361	648701	32.17%	4.079%
19	14.457	1961	1967	1981	rBV2	61619	172923	8.58%	1.087%
20	15.221	2088	2097	2114	rBV	828496	1231281	61.07%	7.742%
21	15.357	2114	2120	2133	rVV	187161	304729	15.11%	1.916%
22	15.463	2133	2138	2143	rVB4	8543	14487	0.72%	0.091%
23	15.998	2227	2229	2234	rVB3	2365	3039	0.15%	0.019%
24	16.763	2355	2359	2363	rBV2	1727	2551	0.13%	0.016%
25	16.968	2388	2394	2405	rBV	580994	814177	40.38%	5.120%
26	17.068	2405	2411	2425	rVV	930695	1354004	67.16%	8.514%
27	19.004	2736	2740	2747	rVB	9800	11875	0.59%	0.075%
28	19.251	2778	2782	2788	rBV	7652	11968	0.59%	0.075%
29	19.362	2795	2801	2815	rBV	1249000	1789863	88.78%	11.255%
30	21.156	3100	3106	3117	rBV	704415	1077862	53.46%	6.778%
31	23.186	3444	3451	3464	rVV	1066773	2016174	100.00%	12.678%
32	23.321	3468	3474	3485	rVB2	592036	1156491	57.36%	7.272%

LSC Area Percent Report

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM050121\
Data File : BM029758.D
Acq On : 01 May 2021 22:26
Operator : CG/JU
Sample : PB135930BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK930

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050121.M
Title : SVOA CALIBRATION


Sum of corrected areas: 15902931

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM050121\
Data File : BM029758.D
Acq On : 01 May 2021 22:26
Operator : CG/JU
Sample : PB135930BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK930

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050121.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

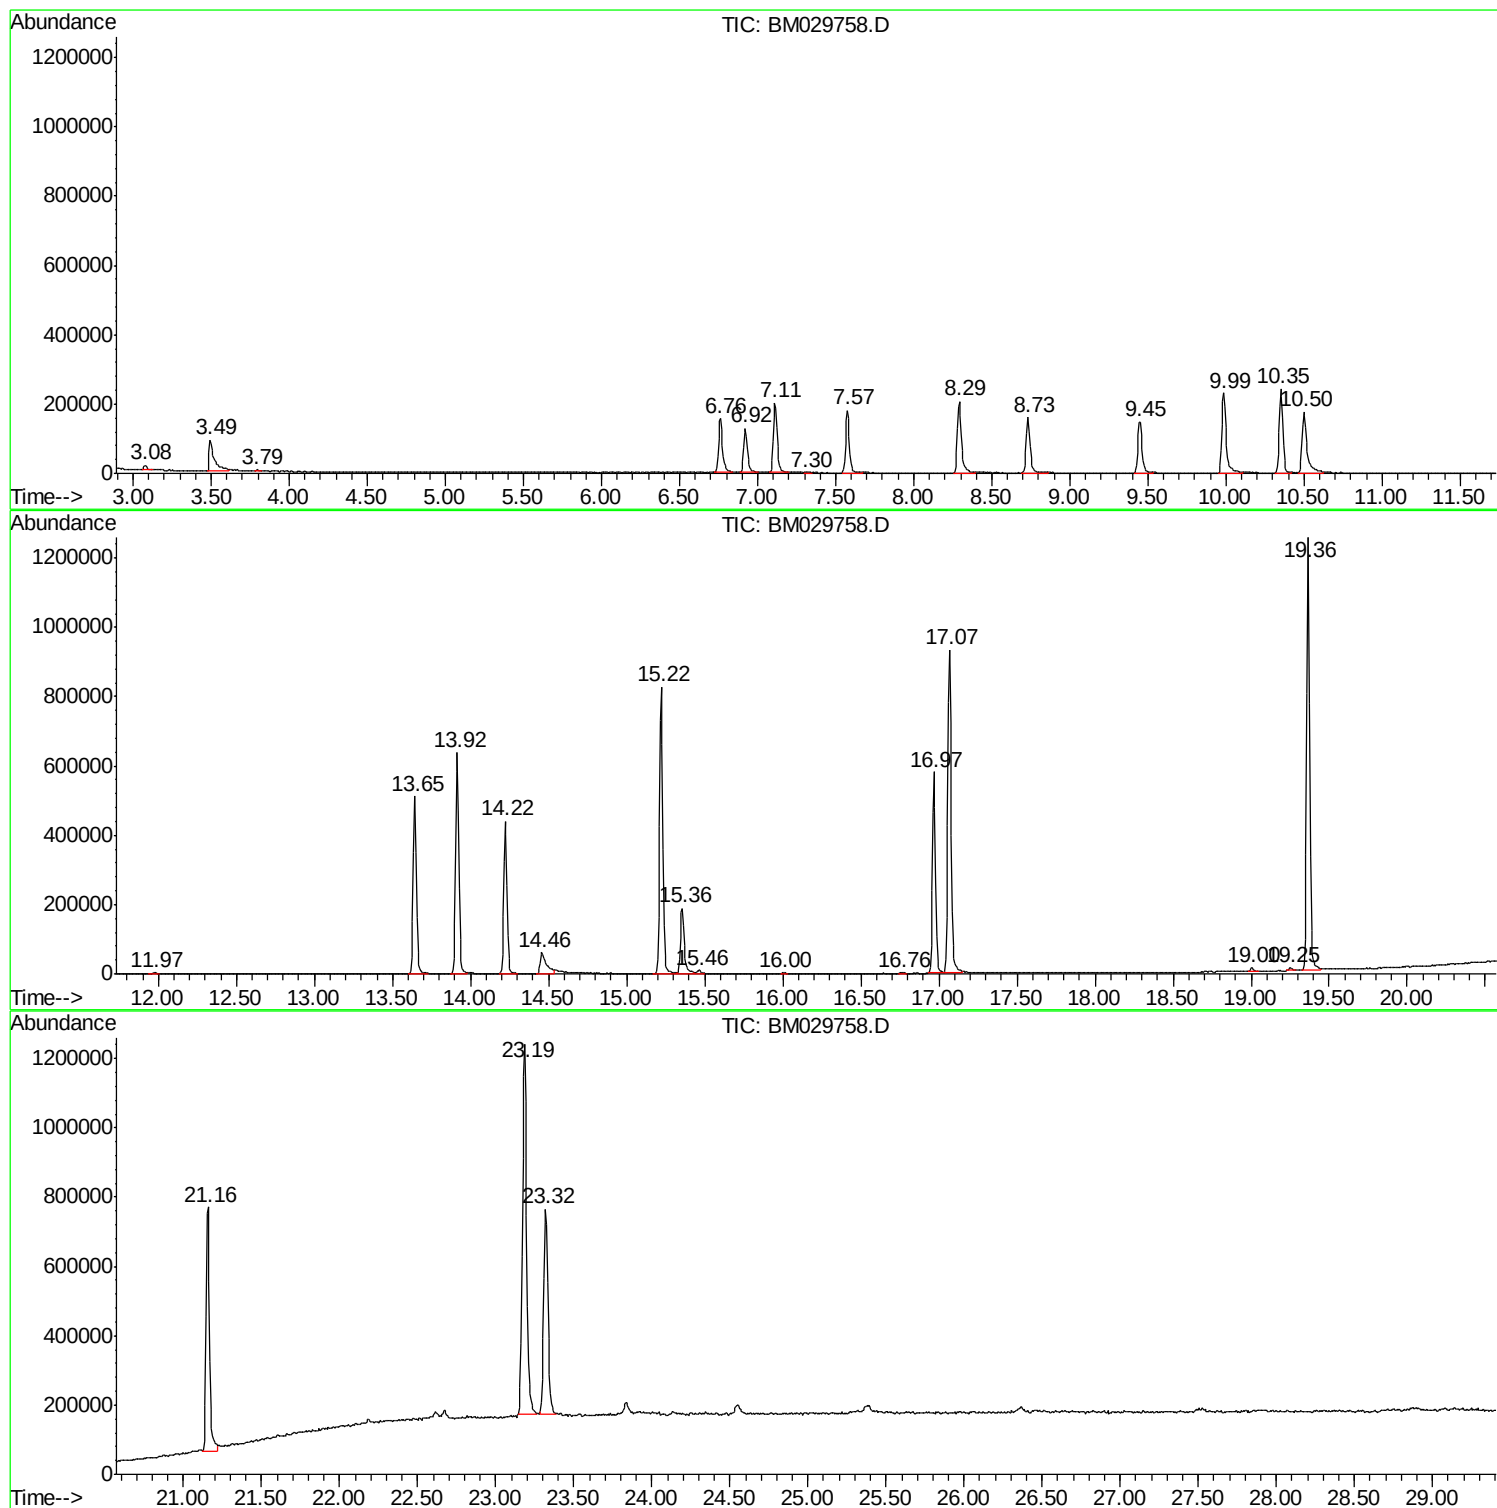

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM050121\\\

Data_File : BM029758.D

Acq_On : 01_May, 2021 22:266

Operator : CG/JUU

Sample : PB135930BLL

Misc :

ALS_Vial : 8 Sample_Multiplier: 11

Instrument :
BNA_M
ClientSampleId :
SBLK930

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SEAM-EPA-BM050121.MM

Quant_Title : SVOA_CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL

TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
