

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050121\
 Data File : BM029760.D
 Acq On : 01 May 2021 23:39
 Operator : CG/JU
 Sample : PB135931BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK931

Integration Parameters: LSCINT.P

Integrator: RTE

Soothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050121.M
 Title : SVOA CALIBRATION

Signal : TIC: BM029760.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.081	30	33	38	rVB	11083	14886	0.76%	0.098%
2	3.493	100	103	119	rBV	91021	189430	9.68%	1.246%
3	3.793	152	154	161	rBV4	2894	4166	0.21%	0.027%
4	6.763	653	659	671	rBV	153821	277248	14.17%	1.823%
5	6.922	679	686	697	rBV	122329	215373	11.01%	1.416%
6	7.110	712	718	729	rBV	199420	337197	17.23%	2.217%
7	7.575	791	797	809	rBV	176684	289342	14.79%	1.902%
8	8.292	913	919	937	rBV2	202633	372406	19.03%	2.449%
9	8.733	987	994	1006	rBV	152304	281872	14.41%	1.853%
10	9.451	1109	1116	1127	rBV	141189	259164	13.25%	1.704%
11	9.986	1200	1207	1225	rBV	218723	429962	21.98%	2.827%
12	10.104	1225	1227	1235	rVB4	2529	4513	0.23%	0.030%
13	10.351	1263	1269	1280	rBV	233857	392638	20.07%	2.582%
14	10.498	1287	1294	1308	rBV	162550	371314	18.98%	2.441%
15	11.974	1540	1545	1550	rBV3	2154	4533	0.23%	0.030%
16	13.639	1822	1828	1840	rBV	481875	732390	37.43%	4.815%
17	13.915	1868	1875	1889	rBV	613467	902768	46.14%	5.936%
18	14.221	1921	1927	1939	rBV	418014	618761	31.62%	4.068%
19	14.457	1961	1967	1991	rBV2	53849	187080	9.56%	1.230%
20	15.221	2089	2097	2114	rBV	805920	1164839	59.53%	7.659%
21	15.357	2114	2120	2133	rVV	179705	289439	14.79%	1.903%
22	15.457	2135	2137	2143	rVB2	7861	11047	0.56%	0.073%
23	16.004	2227	2230	2235	rBV4	2779	3322	0.17%	0.022%
24	16.756	2356	2358	2363	rVB2	1901	2338	0.12%	0.015%
25	16.968	2388	2394	2405	rBV	534808	765280	39.11%	5.032%
26	17.068	2405	2411	2431	rVV	871998	1289103	65.89%	8.476%
27	19.003	2736	2740	2744	rBV	9368	11976	0.61%	0.079%
28	19.250	2779	2782	2788	rBV	7771	9449	0.48%	0.062%
29	19.368	2795	2802	2820	rBV	1150797	1714108	87.61%	11.270%
30	21.156	3100	3106	3118	rBV	684658	1004069	51.32%	6.602%
31	23.185	3444	3451	3462	rBV	1041658	1956590	100.00%	12.865%
32	23.321	3468	3474	3483	rVB2	592905	1102426	56.34%	7.248%




Sum of corrected areas: 15209029

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050121\
Data File : BM029760.D
Acq On : 01 May 2021 23:39
Operator : CG/JU
Sample : PB135931BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK931

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050121.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

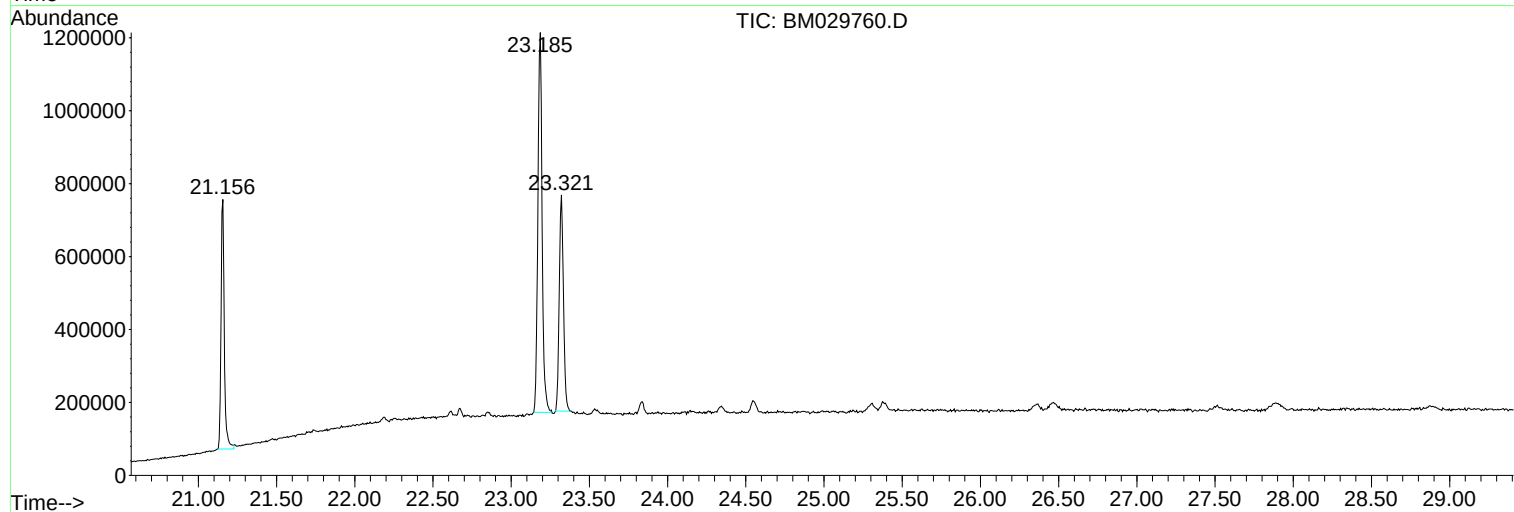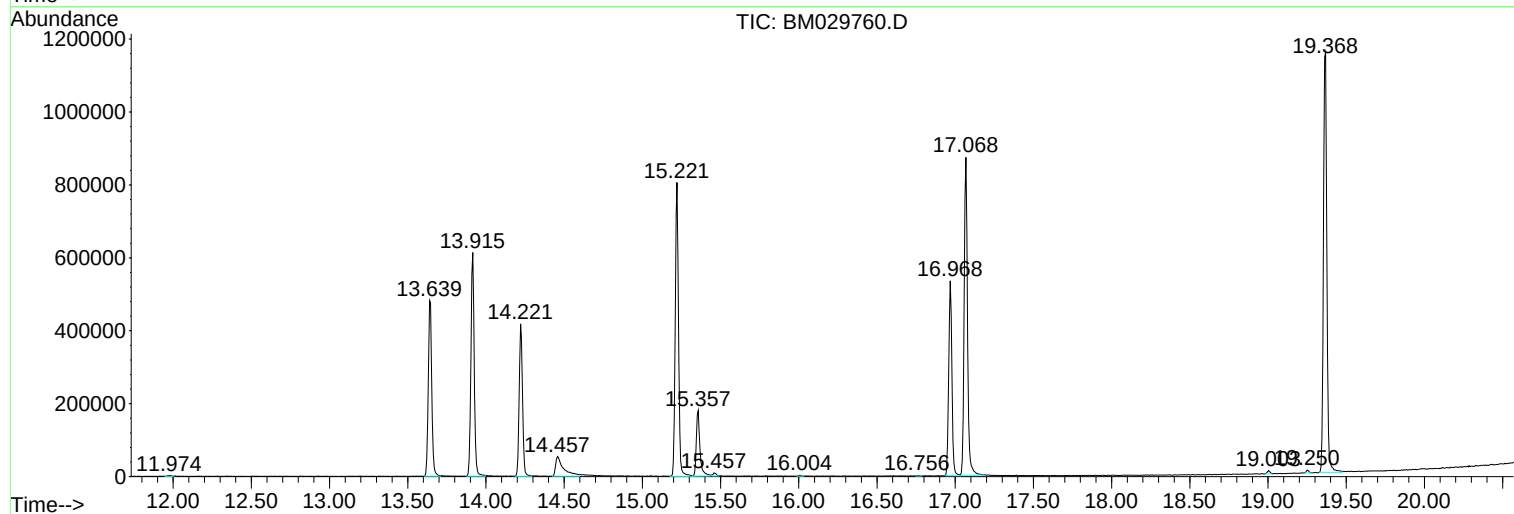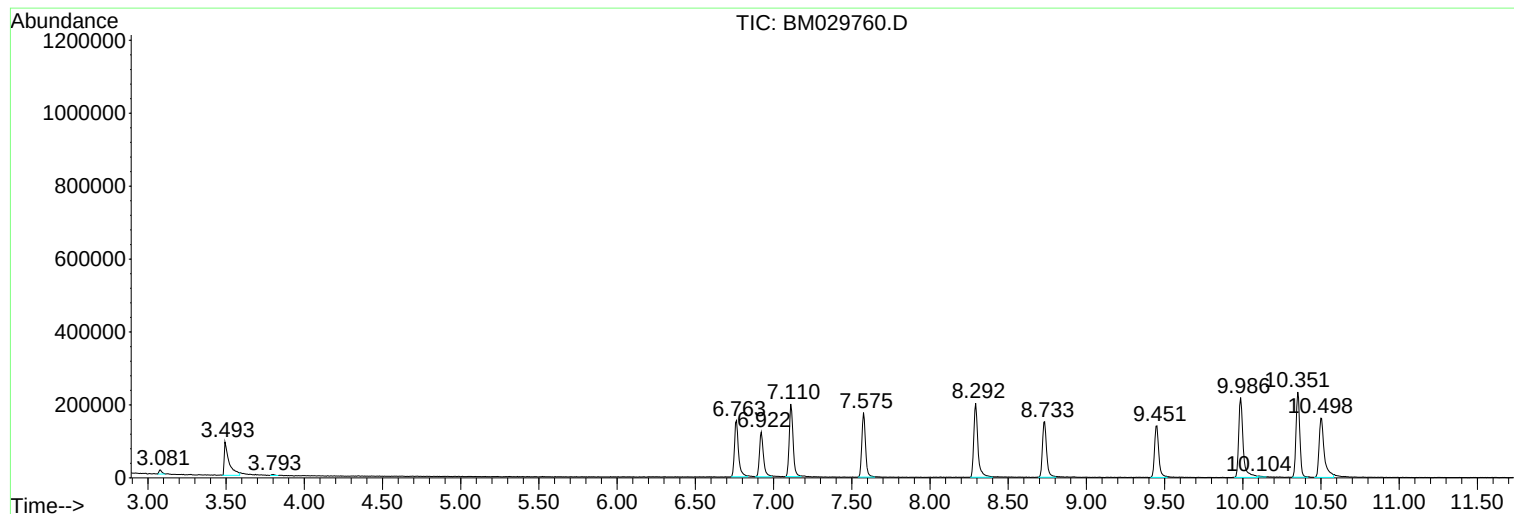

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050121\
Data File : BM029760.D
Acq On : 01 May 2021 23:39
Operator : CG/JU
Sample : PB135931BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK931

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050121.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050121\
Data File : BM029760.D
Acq On : 01 May 2021 23:39
Operator : CG/JU
Sample : PB135931BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK931

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050121.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
