

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050121\
 Data File : BM029767.D
 Acq On : 02 May 2021 04:29
 Operator : CG/JU
 Sample : PB135971BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK971

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050121.M
 Title : SVOA CALIBRATION

Signal : TIC: BM029767.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.075	29	32	38	rBV	11274	14262	0.68%	0.086%
2	3.340	75	77	80	rVB3	2102	2113	0.10%	0.013%
3	3.493	101	103	127	rBV	93087	207500	9.83%	1.253%
4	6.757	652	658	676	rBV	158896	292615	13.86%	1.767%
5	6.922	679	686	699	rBV	128611	223952	10.60%	1.352%
6	7.110	712	718	733	rBV	210437	352731	16.70%	2.130%
7	7.575	790	797	808	rBV	185932	302605	14.33%	1.827%
8	8.292	912	919	931	rBV	204717	386580	18.30%	2.334%
9	8.728	987	993	1013	rBV	163667	310629	14.71%	1.876%
10	9.445	1109	1115	1127	rBV	149920	269777	12.77%	1.629%
11	9.986	1200	1207	1221	rBV	231182	449072	21.26%	2.712%
12	10.351	1262	1269	1278	rBV	250867	413261	19.57%	2.496%
13	10.498	1287	1294	1311	rBV	181026	392738	18.60%	2.372%
14	11.980	1538	1546	1549	rBV4	2590	5463	0.26%	0.033%
15	13.639	1822	1828	1841	rBV	546636	809246	38.32%	4.887%
16	13.916	1868	1875	1894	rBV	626192	979764	46.39%	5.916%
17	14.221	1921	1927	1938	rBV	460580	666320	31.55%	4.024%
18	14.457	1961	1967	1983	rBV	68451	200117	9.48%	1.208%
19	15.221	2090	2097	2109	rBV	857586	1272270	60.24%	7.683%
20	15.351	2114	2119	2134	rVV	199137	322968	15.29%	1.950%
21	15.462	2134	2138	2142	rVB	9252	12440	0.59%	0.075%
22	16.004	2224	2230	2233	rBV4	3149	4391	0.21%	0.027%
23	16.757	2353	2358	2364	rBV3	1585	3281	0.16%	0.020%
24	16.968	2388	2394	2404	rBV	602039	854903	40.48%	5.162%
25	17.068	2404	2411	2430	rVV	964309	1432818	67.84%	8.652%
26	18.998	2736	2739	2747	rVB	8403	12932	0.61%	0.078%
27	19.250	2778	2782	2788	rBV	8520	11184	0.53%	0.068%
28	19.362	2795	2801	2813	rBV	1411944	1891268	89.55%	11.421%
29	19.615	2842	2844	2846	rBV3	2393	2493	0.12%	0.015%
30	21.150	3100	3105	3121	rBV	804251	1137801	53.88%	6.871%
31	23.180	3444	3450	3462	rVB	1138030	2111913	100.00%	12.753%
32	23.315	3467	3473	3484	rVB2	617996	1210756	57.33%	7.311%




Sum of corrected areas: 16560163

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050121\
Data File : BM029767.D
Acq On : 02 May 2021 04:29
Operator : CG/JU
Sample : PB135971BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK971

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050121.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

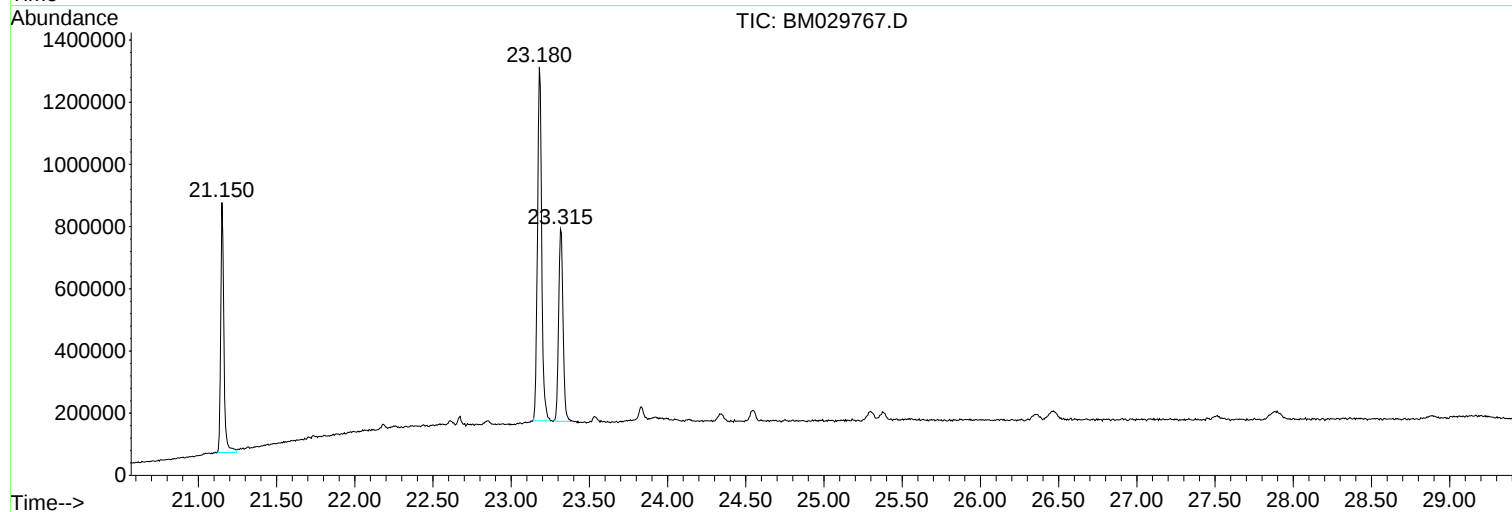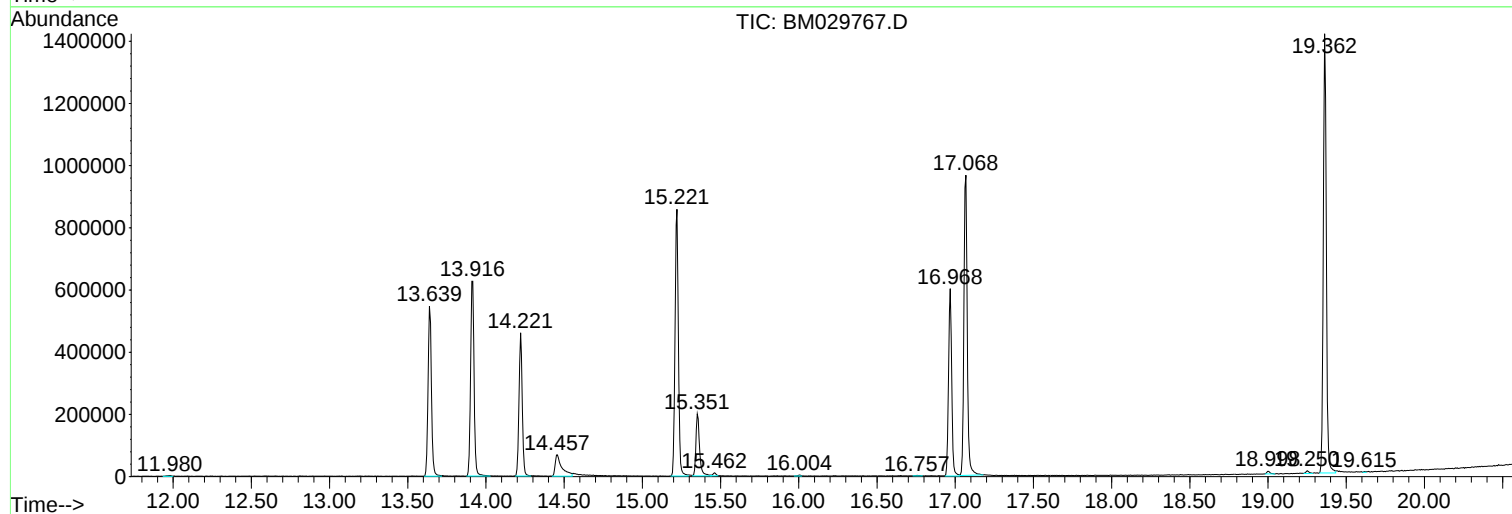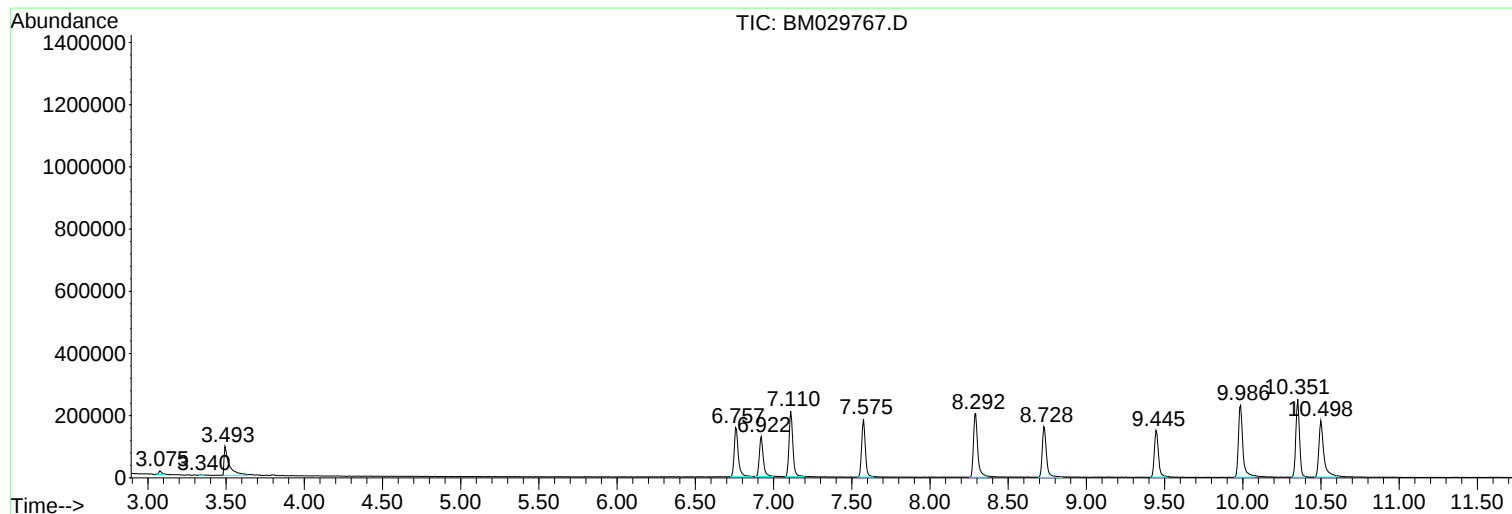

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050121\
Data File : BM029767.D
Acq On : 02 May 2021 04:29
Operator : CG/JU
Sample : PB135971BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK971

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050121.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050121\
Data File : BM029767.D
Acq On : 02 May 2021 04:29
Operator : CG/JU
Sample : PB135971BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK971

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050121.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc