

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050121\
 Data File : BM029774.D
 Acq On : 02 May 2021 08:41
 Operator : CG/JU
 Sample : M2144-02
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0GH2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050121.M
 Title : SVOA CALIBRATION

Signal : TIC: BM029774.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.263	62	64	68	rBV5	1927	2398	0.11%	0.017%
2	3.710	136	140	145	rVB3	3243	5217	0.24%	0.037%
3	3.799	151	155	158	rBV4	2523	3753	0.17%	0.027%
4	4.910	338	344	349	rBV5	5117	9093	0.42%	0.065%
5	6.722	647	652	654	rBV2	2326	2964	0.14%	0.021%
6	6.763	654	659	672	rVV2	26781	63581	2.94%	0.453%
7	6.916	679	685	700	rBV	99636	186116	8.62%	1.327%
8	7.110	711	718	732	rBV	138481	243111	11.26%	1.734%
9	7.575	791	797	808	rBV	156029	264736	12.26%	1.888%
10	7.922	849	856	864	rVB2	8492	15634	0.72%	0.112%
11	8.287	912	918	935	rBV	80258	164827	7.63%	1.176%
12	8.728	987	993	1009	rBV	130378	254086	11.76%	1.812%
13	9.145	1059	1064	1068	rBV3	7143	10029	0.46%	0.072%
14	9.445	1108	1115	1130	rBV	124643	225632	10.45%	1.609%
15	9.981	1200	1206	1221	rBV	149130	337140	15.61%	2.404%
16	10.081	1221	1223	1232	rVB3	4726	8268	0.38%	0.059%
17	10.186	1237	1241	1244	rVV4	1813	2946	0.14%	0.021%
18	10.351	1261	1269	1281	rBV	202305	352708	16.33%	2.516%
19	10.539	1296	1301	1305	rBV3	2217	3720	0.17%	0.027%
20	11.639	1480	1488	1492	rBV5	3220	5457	0.25%	0.039%
21	11.957	1539	1542	1544	rBV3	1779	2280	0.11%	0.016%
22	13.039	1722	1726	1732	rBV5	2648	4659	0.22%	0.033%
23	13.639	1821	1828	1834	rBV	464664	669523	31.00%	4.775%
24	13.686	1834	1836	1842	rVB	15160	19932	0.92%	0.142%
25	13.910	1867	1874	1891	rBV	559681	829827	38.42%	5.918%
26	14.221	1919	1927	1938	rBV	366208	561599	26.00%	4.005%
27	14.480	1967	1971	1972	rBV3	2947	3830	0.18%	0.027%
28	14.863	2031	2036	2040	rVB	2130	3038	0.14%	0.022%
29	14.980	2052	2056	2062	rBV3	2774	4154	0.19%	0.030%
30	15.216	2089	2096	2112	rBV	733446	1117089	51.72%	7.967%
31	15.351	2114	2119	2134	rVV	196656	299911	13.89%	2.139%
32	15.463	2134	2138	2144	rVB2	8882	13087	0.61%	0.093%
33	15.951	2216	2221	2224	rVV3	1636	2219	0.10%	0.016%
34	16.004	2226	2230	2235	rVB4	2659	4372	0.20%	0.031%
35	16.210	2261	2265	2268	rBV3	2431	2397	0.11%	0.017%
36	16.751	2352	2357	2358	rBV4	2241	2719	0.13%	0.019%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050121\
 Data File : BM029774.D
 Acq On : 02 May 2021 08:41
 Operator : CG/JU
 Sample : M2144-02
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0GH2

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050121.M
 Title : SVOA CALIBRATION

37	16.962	2387	2393	2404	rBV	481416	717603	33.23%	5.118%
38	17.062	2404	2410	2429	rVV	936255	1393669	64.53%	9.940%
39	17.874	2544	2548	2554	rBV3	12628	20240	0.94%	0.144%
40	18.633	2673	2677	2680	rVB	8423	10243	0.47%	0.073%
41	18.998	2736	2739	2744	rVB	9269	12485	0.58%	0.089%
42	19.168	2764	2768	2773	rBV6	5313	8056	0.37%	0.057%
43	19.251	2778	2782	2790	rVV2	7996	12456	0.58%	0.089%
44	19.362	2795	2801	2817	rBV	1396552	1876377	86.88%	13.382%
45	20.880	3056	3059	3065	rBV3	44042	73685	3.41%	0.526%
46	21.150	3100	3105	3118	rBV	690795	971322	44.97%	6.927%
47	23.180	3443	3450	3466	rBV	1137632	2159728	100.00%	15.403%
48	23.315	3467	3473	3483	rVB2	570863	1063440	49.24%	7.584%




Sum of corrected areas: 14021356

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050121\
Data File : BM029774.D
Acq On : 02 May 2021 08:41
Operator : CG/JU
Sample : M2144-02
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0GH2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050121.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

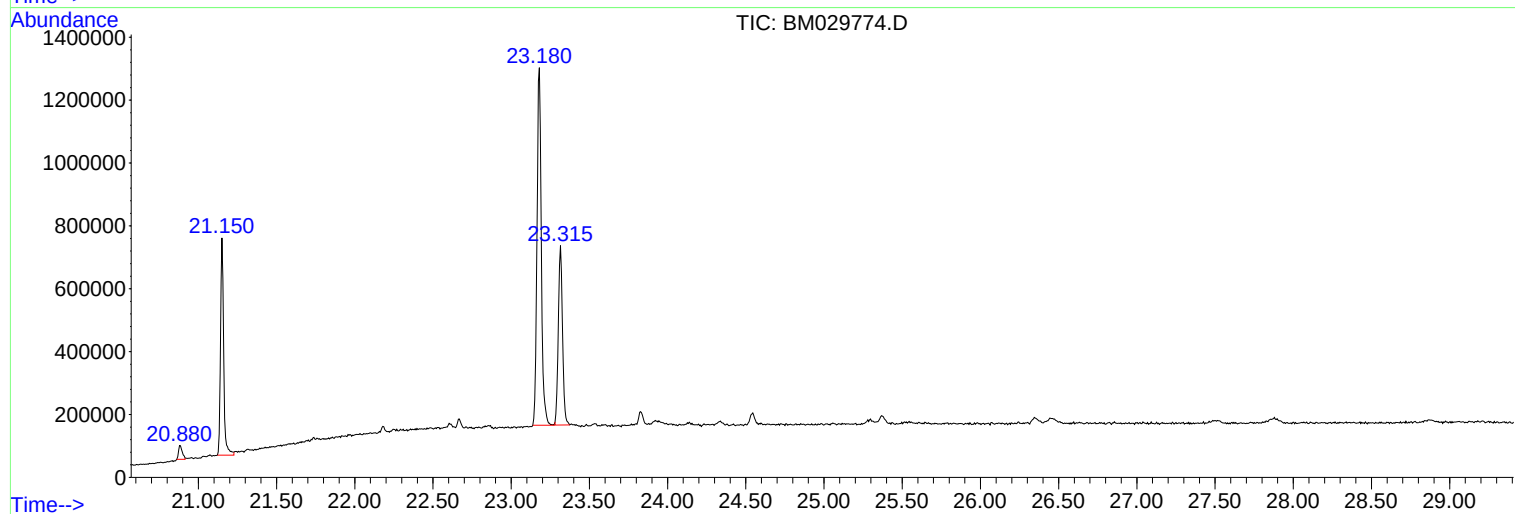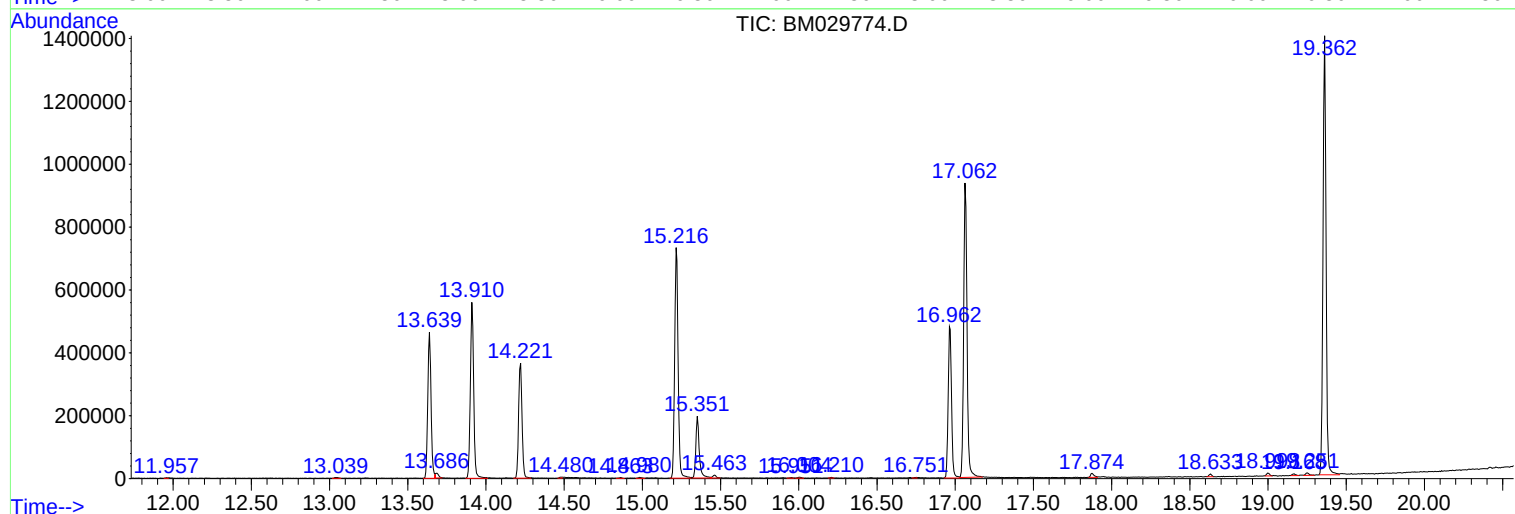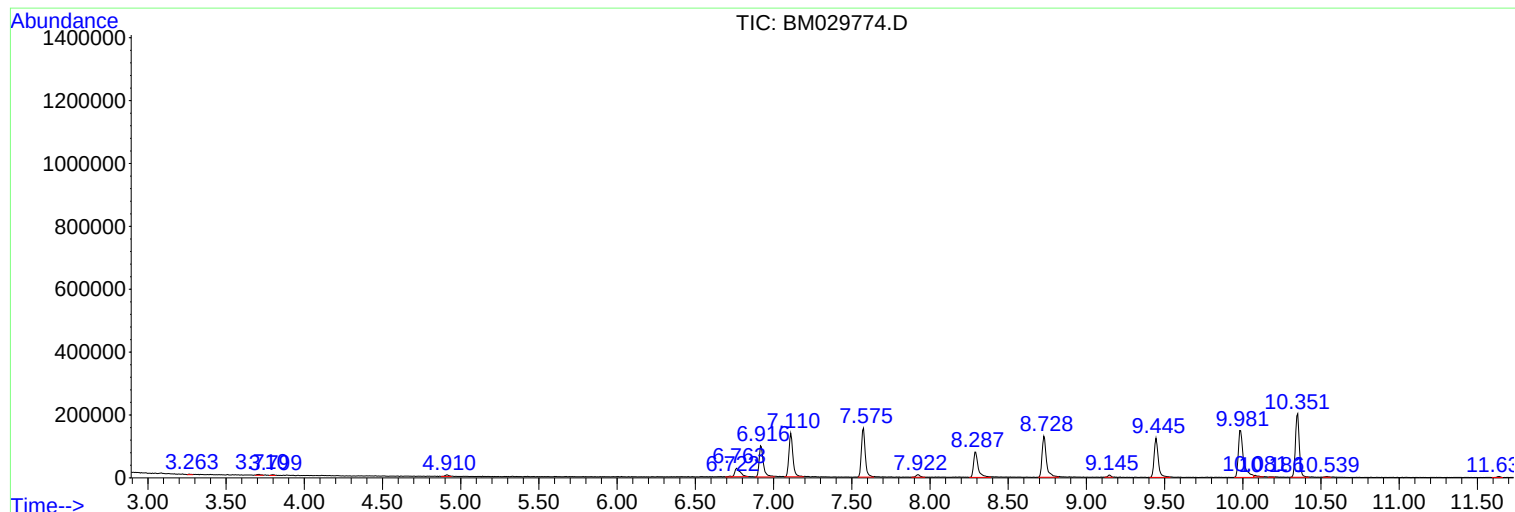

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050121\
Data File : BM029774.D
Acq On : 02 May 2021 08:41
Operator : CG/JU
Sample : M2144-02
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0GH2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050121.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050121\
Data File : BM029774.D
Acq On : 02 May 2021 08:41
Operator : CG/JU
Sample : M2144-02
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0GH2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050121.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------