

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050121\
 Data File : BM029775.D
 Acq On : 02 May 2021 09:17
 Operator : CG/JU
 Sample : M2144-03
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0GH3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050121.M
 Title : SVOA CALIBRATION

Signal : TIC: BM029775.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.087	33	34	38	rVB3	4007	3421	0.17%	0.026%
2	3.799	151	155	158	rBV4	3716	4438	0.22%	0.034%
3	6.646	635	639	643	rVB5	1425	2158	0.11%	0.017%
4	6.763	654	659	671	rBV2	22692	59909	2.95%	0.463%
5	6.922	680	686	698	rBV	92702	170003	8.37%	1.314%
6	7.110	712	718	731	rBV	134254	236241	11.63%	1.826%
7	7.575	790	797	810	rBV	156119	262524	12.92%	2.030%
8	8.292	913	919	928	rBV	74549	143106	7.04%	1.106%
9	8.728	986	993	1008	rBV	123989	231137	11.38%	1.787%
10	9.151	1059	1065	1071	rVB2	4990	8242	0.41%	0.064%
11	9.445	1108	1115	1128	rBV	114556	208875	10.28%	1.615%
12	9.987	1200	1207	1224	rBV	137268	319090	15.71%	2.467%
13	10.351	1260	1269	1277	rBV	200005	343572	16.91%	2.656%
14	10.534	1295	1300	1301	rBV3	1654	2751	0.14%	0.021%
15	11.633	1484	1487	1496	rBV4	2147	4156	0.20%	0.032%
16	11.969	1538	1544	1549	rVB4	1816	3443	0.17%	0.027%
17	13.639	1821	1828	1834	rBV	401942	588344	28.96%	4.549%
18	13.910	1867	1874	1885	rBV	505243	750459	36.94%	5.802%
19	14.222	1920	1927	1939	rBV	352006	525756	25.88%	4.065%
20	14.498	1967	1974	1976	rBV4	2046	4092	0.20%	0.032%
21	15.216	2090	2096	2113	rBV	669827	1012229	49.83%	7.826%
22	15.351	2113	2119	2129	rBV	161270	242055	11.92%	1.871%
23	15.463	2134	2138	2143	rVB4	6363	10046	0.49%	0.078%
24	15.645	2166	2169	2174	rBV5	1521	2315	0.11%	0.018%
25	15.904	2211	2213	2218	rVB2	2075	2709	0.13%	0.021%
26	15.951	2218	2221	2224	rBV4	3586	5577	0.27%	0.043%
27	16.004	2228	2230	2234	rVB3	3740	3685	0.18%	0.028%
28	16.116	2244	2249	2253	rVB4	1399	2835	0.14%	0.022%
29	16.210	2260	2265	2268	rVB3	3139	4471	0.22%	0.035%
30	16.321	2279	2284	2287	rBV5	1549	2458	0.12%	0.019%
31	16.757	2353	2358	2361	rBV5	2546	4349	0.21%	0.034%
32	16.963	2387	2393	2404	rBV	448207	668239	32.90%	5.166%
33	17.063	2404	2410	2428	rVV	835089	1223551	60.23%	9.460%
34	17.333	2450	2456	2457	rBV5	1345	2234	0.11%	0.017%
35	17.433	2471	2473	2478	rVB4	1610	2447	0.12%	0.019%
36	17.874	2544	2548	2558	rBV9	12980	23612	1.16%	0.183%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050121\
 Data File : BM029775.D
 Acq On : 02 May 2021 09:17
 Operator : CG/JU
 Sample : M2144-03
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0GH3

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050121.M
 Title : SVOA CALIBRATION

37	18.021	2571	2573	2578	rBV6	1901	2033	0.10%	0.016%
38	18.627	2673	2676	2681	rBV4	8509	12485	0.61%	0.097%
39	18.998	2735	2739	2744	rBV2	10237	15502	0.76%	0.120%
40	19.039	2744	2746	2751	rVB6	3637	3420	0.17%	0.026%
41	19.162	2764	2767	2770	rBV5	4792	6766	0.33%	0.052%
42	19.251	2779	2782	2787	rBV2	7422	9184	0.45%	0.071%
43	19.362	2794	2801	2810	rBV	1237889	1682064	82.80%	13.005%
44	20.880	3055	3059	3068	rBV4	44945	93529	4.60%	0.723%
45	21.150	3100	3105	3116	rBV	675491	936518	46.10%	7.241%
46	23.180	3443	3450	3463	rBV	1091217	2031367	100.00%	15.705%
47	23.315	3467	3473	3483	rVB2	554157	1056788	52.02%	8.171%




Sum of corrected areas: 12934185

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050121\
Data File : BM029775.D
Acq On : 02 May 2021 09:17
Operator : CG/JU
Sample : M2144-03
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0GH3

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050121.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

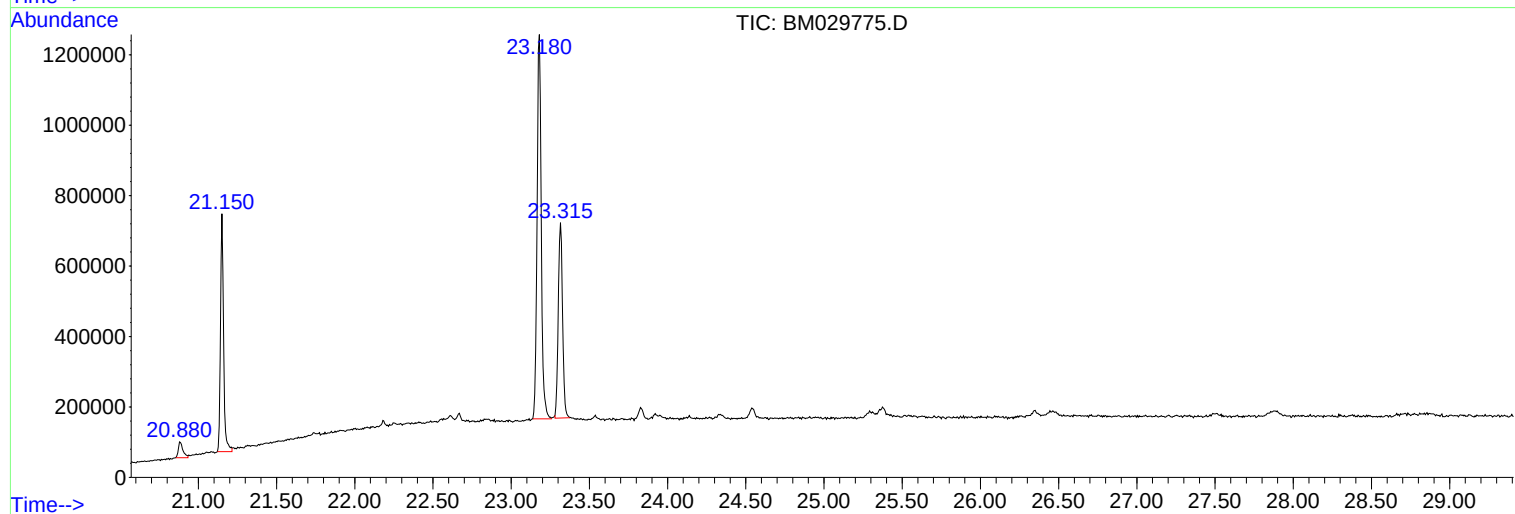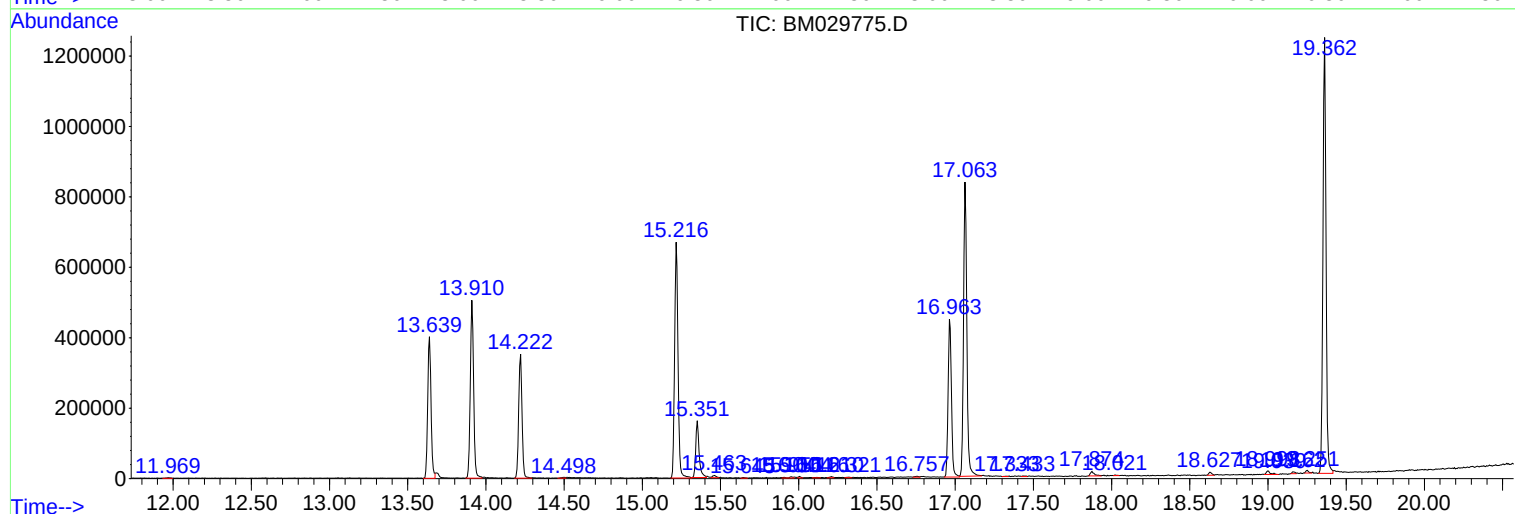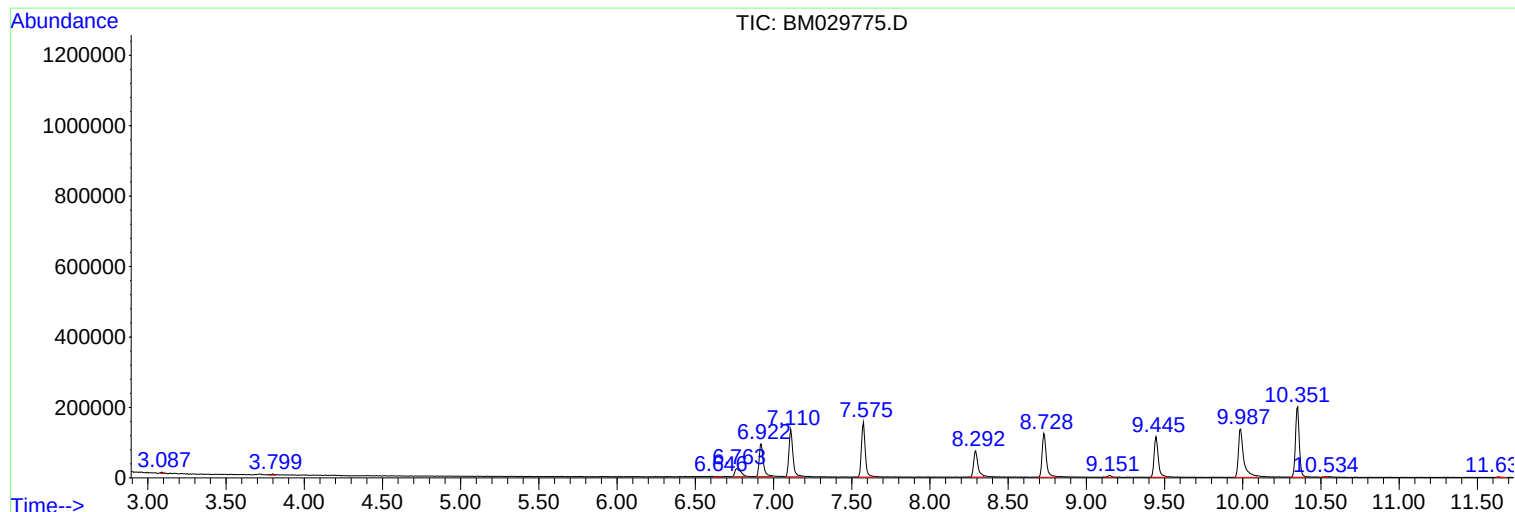

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050121\
Data File : BM029775.D
Acq On : 02 May 2021 09:17
Operator : CG/JU
Sample : M2144-03
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0GH3

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050121.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050121\
Data File : BM029775.D
Acq On : 02 May 2021 09:17
Operator : CG/JU
Sample : M2144-03
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0GH3

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050121.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
