

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM050319\
 Data File : BM020110.D
 Acq On : 03 May 2019 14:04
 Operator : JU/SJ
 Sample : PB119431BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB119431BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM043019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.363	398	404	414	rBV	3011576	4151065	52.94%	9.192%
2	6.945	664	673	684	rBV	2789233	4359981	55.60%	9.654%
3	7.316	728	736	745	rBV	2964322	4532154	57.80%	10.036%
4	7.787	809	816	824	rBV	542347	838885	10.70%	1.858%
5	8.104	863	870	877	rBV	2179155	3449681	43.99%	7.639%
6	8.951	1006	1014	1026	rBV	1683618	2683994	34.23%	5.943%
7	10.580	1283	1291	1302	rVB	613995	1023100	13.05%	2.265%
8	13.045	1703	1710	1717	rBV	4093877	6019395	76.76%	13.329%
9	14.427	1937	1945	1953	rBV2	902116	1320422	16.84%	2.924%
10	15.915	2192	2198	2212	rBV	3178256	4366496	55.69%	9.669%
11	17.174	2405	2412	2420	rBV2	1085385	1556907	19.85%	3.447%
12	19.797	2853	2858	2864	rBV	6549128	7841416	100.00%	17.363%
13	21.356	3118	3123	3130	rBV	1266100	1545013	19.70%	3.421%
14	23.638	3505	3511	3522	rVB	750284	1472419	18.78%	3.260%


Sum of corrected areas: 45160928

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM050319\
Data File : BM020110.D
Acq On : 03 May 2019 14:04
Operator : JU/SJ
Sample : PB119431BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB119431BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM043019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

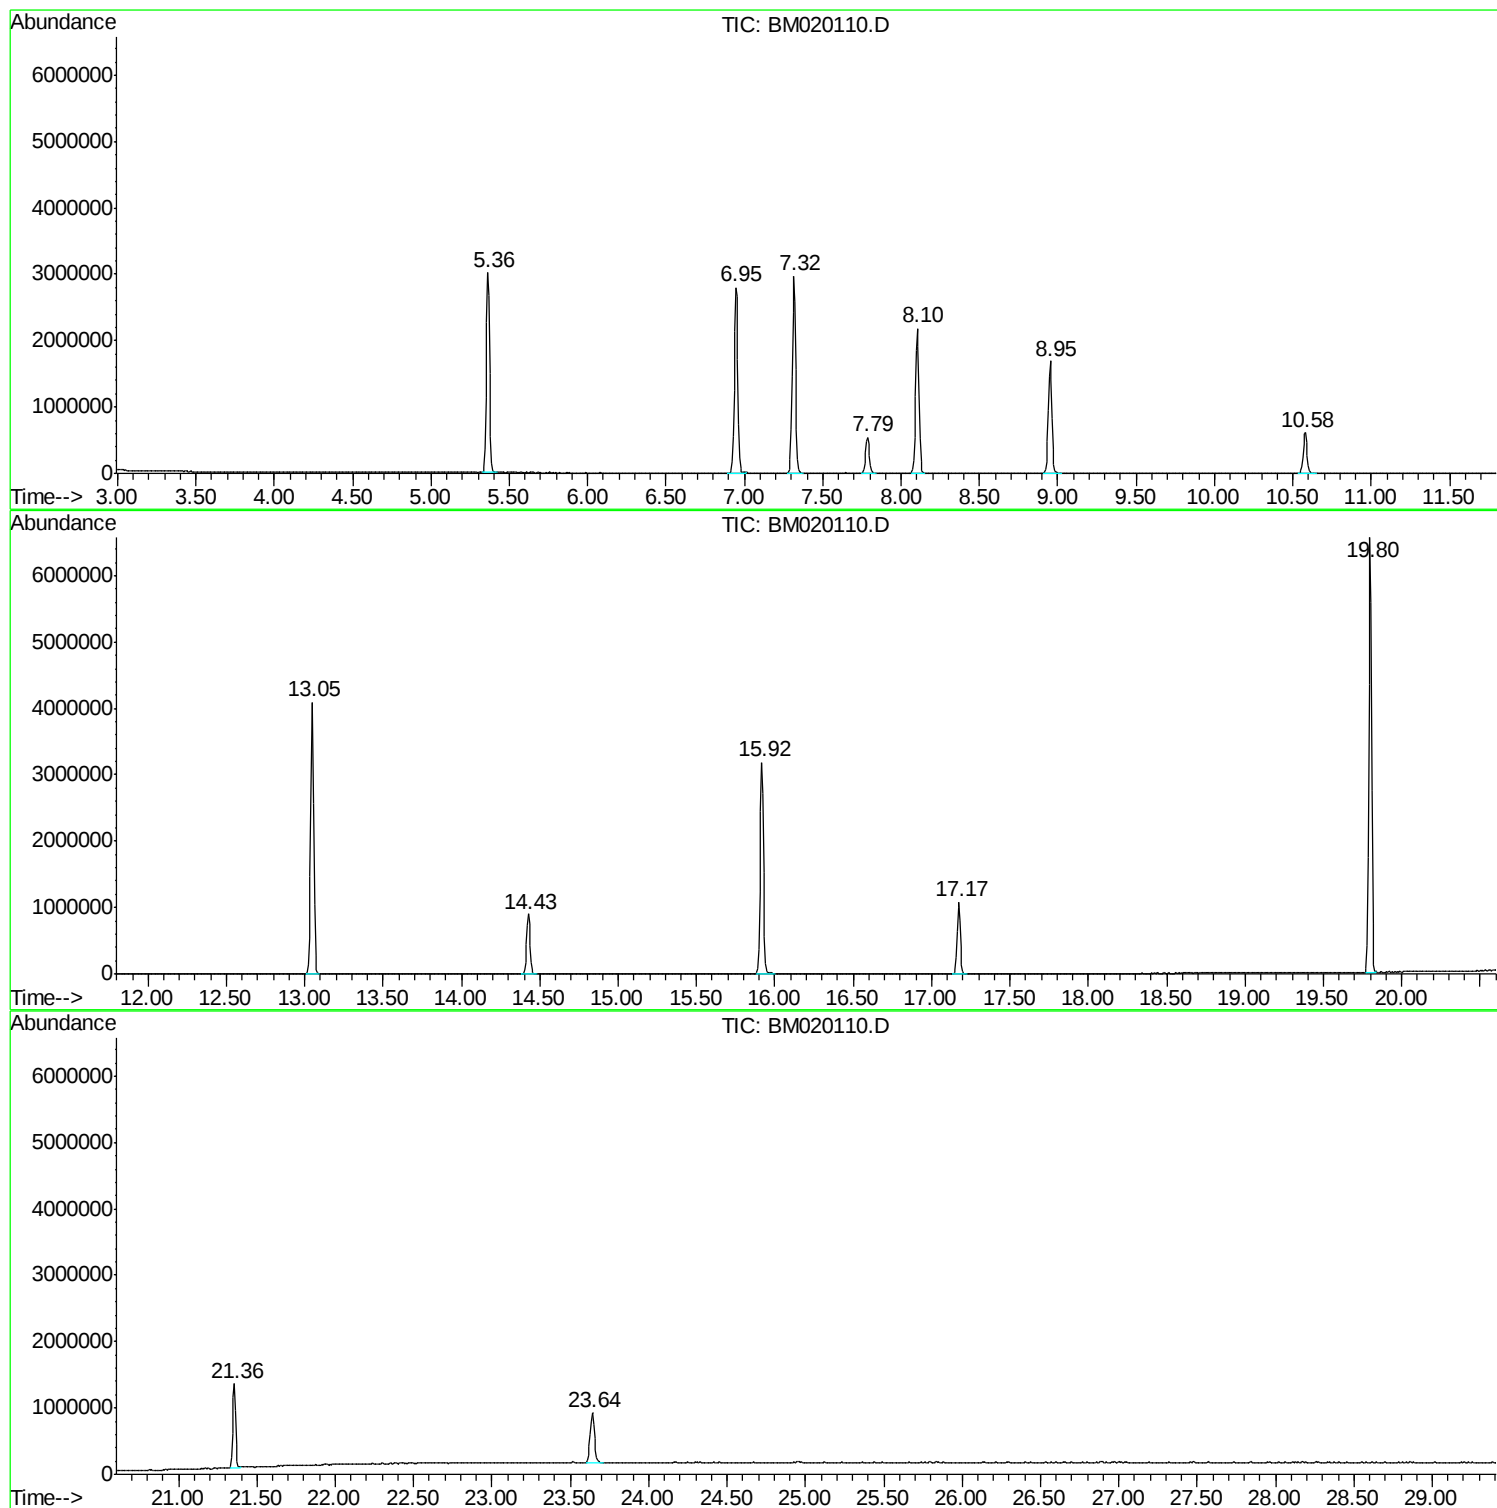

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM050319\
Data File : BM020110.D
Acq On : 03 May 2019 14:04
Operator : JU/SJ
Sample : PB119431BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB119431BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM043019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.32 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.32	108.05 ng	4532150	1,4-Dichlorobenzene-d4	7.79

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	14
2		4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	14
3		2H-Cyclopenta[d]pyridazine, 2-me...	132	C8H8N2	022291-85-6	10
4		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	9
5		1,2,3-Trifluorobenzene	132	C6H3F3	001489-53-8	9

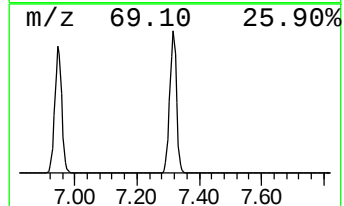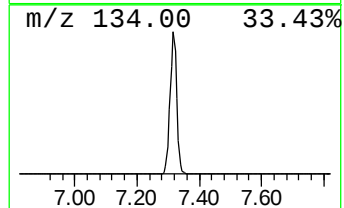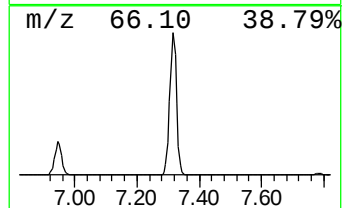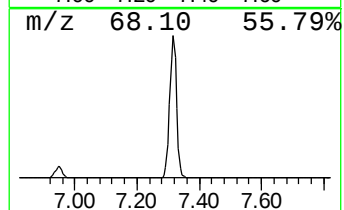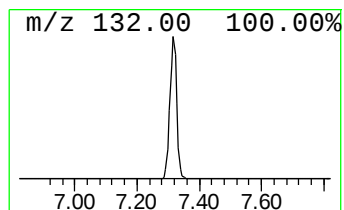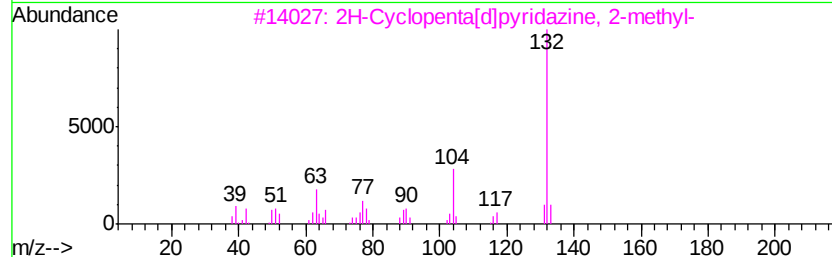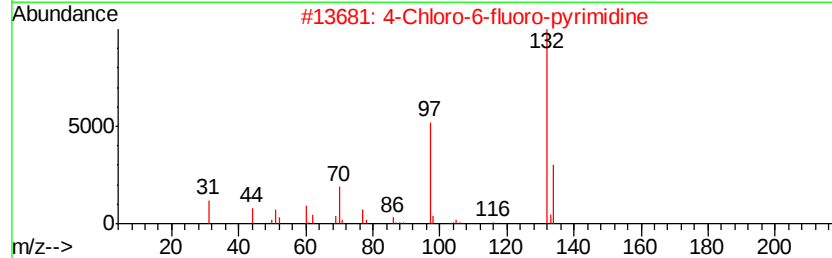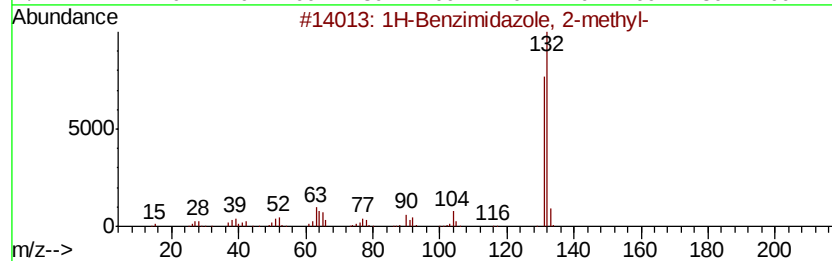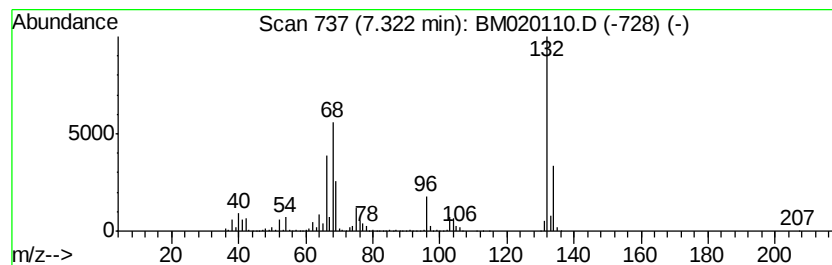

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM050319\
Data File : BM020110.D
Acq On : 03 May 2019 14:04
Operator : JU/SJ
Sample : PB119431BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB119431BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM043019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.32	7.32	108.1	ng	4532150	1	7.79	838885	20.0