


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM050319\
 Data File : BM020107.D
 Acq On : 03 May 2019 11:38
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM043019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 01 03:58:37 2019

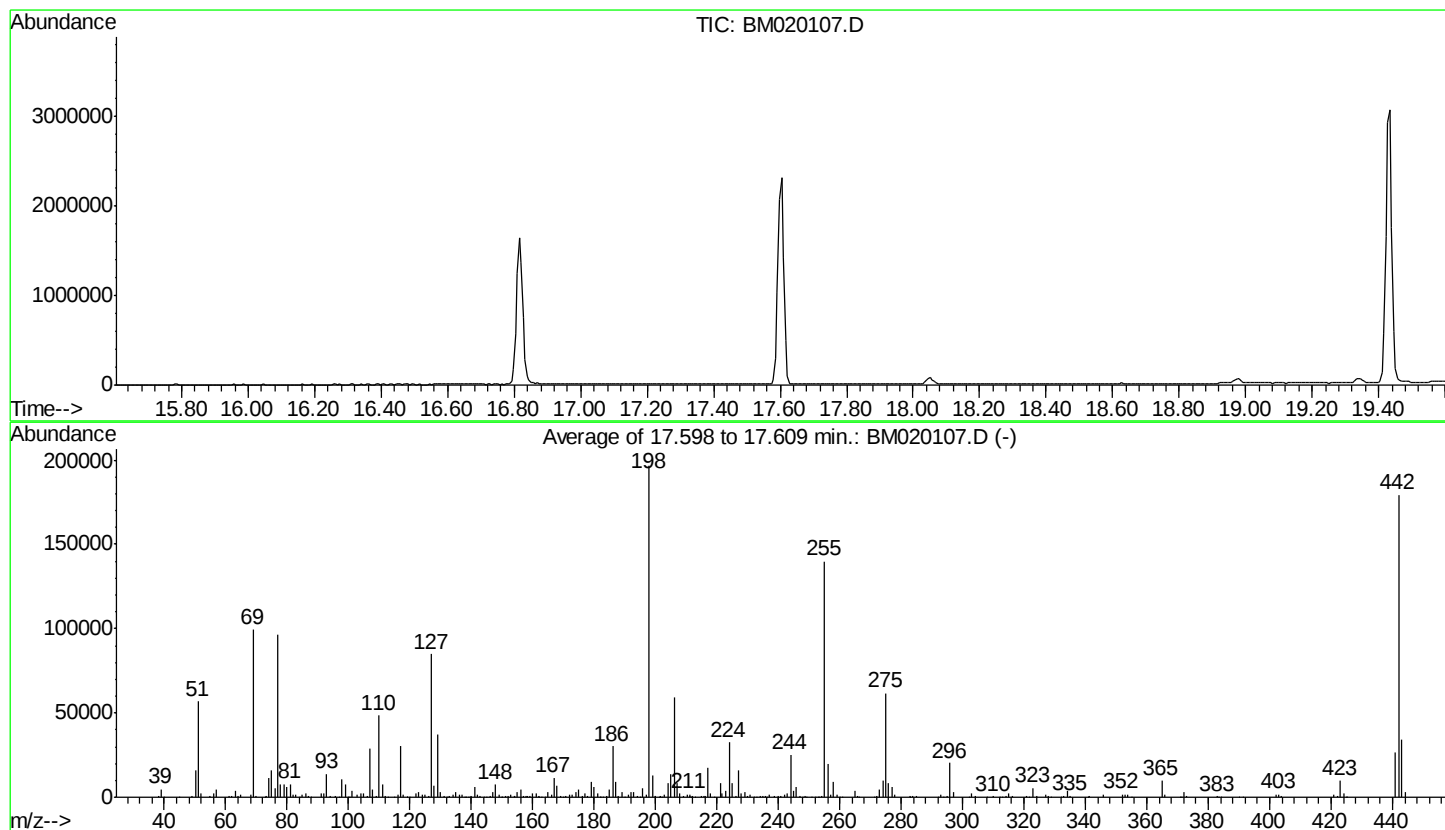

AutoFind: Scans 2484, 2485, 2486; Background Corrected with Scan 2477

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.8	56733	PASS
68	69	0.00	2	1.9	1875	PASS
69	198	0.00	100	50.4	99210	PASS
70	69	0.00	2	0.7	650	PASS
127	198	10	80	43.1	84778	PASS
197	198	0.00	2	1.0	1880	PASS
198	198	100	100	100.0	196714	PASS
199	198	5	9	6.7	13183	PASS
275	198	10	60	31.3	61653	PASS
365	198	1	100	4.9	9622	PASS
441	198	0.01	100	13.6	26762	PASS
442	198	50	100	91.3	179605	PASS
443	442	15	24	18.9	33997	PASS