


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050324\
Data File : BM045670.D
Acq On : 02 May 2024 16:16
Operator : MA/JU
Sample : DFTPP023
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP023

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM050324.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri May 03 03:27:04 2024

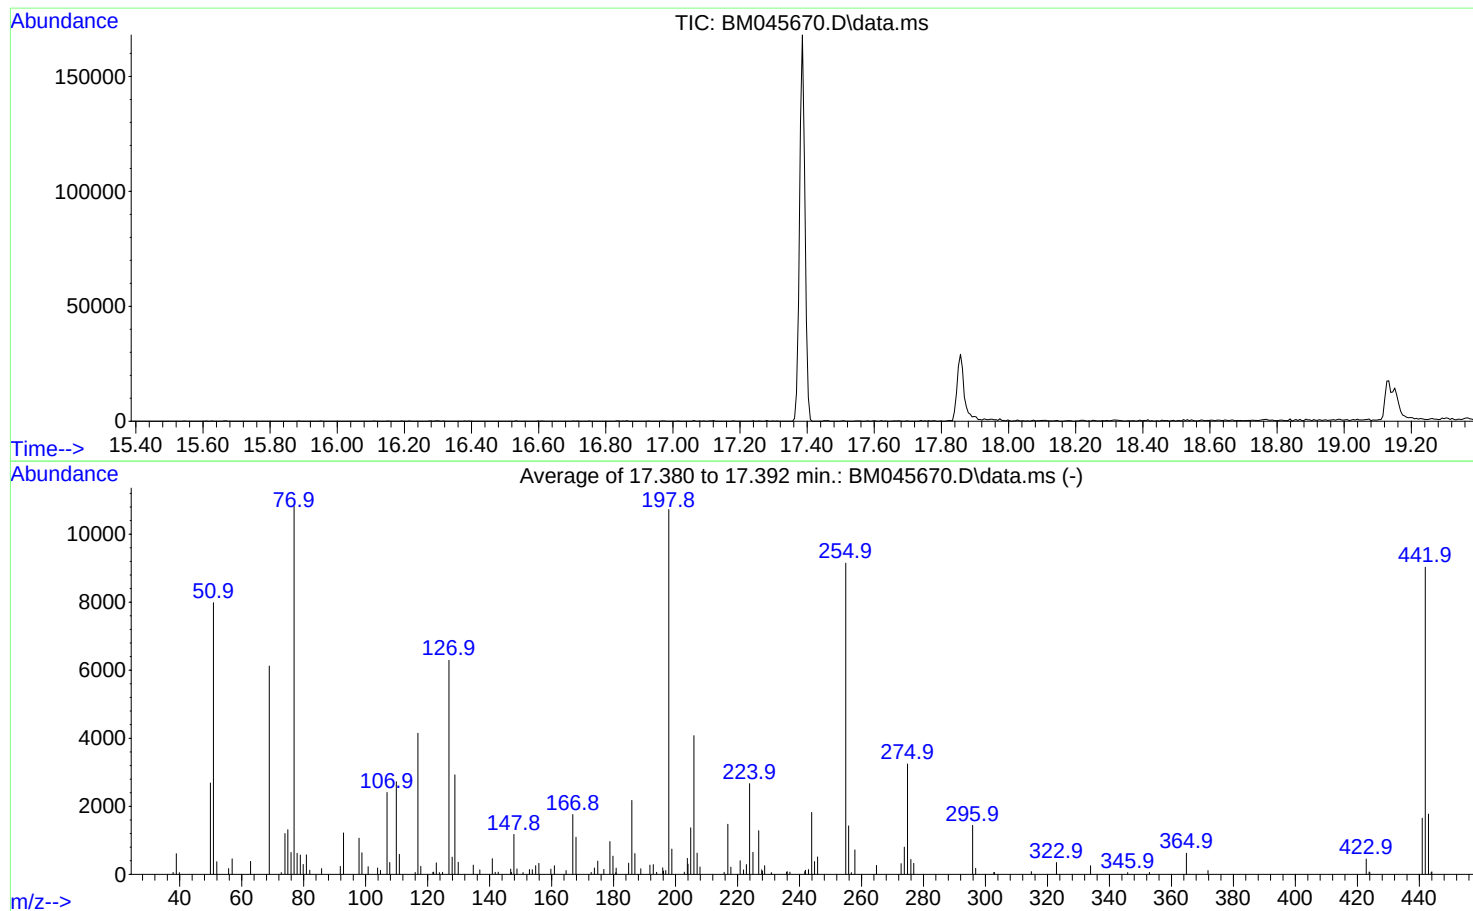

AutoFind: Scans 2430, 2431, 2432; Background Corrected with Scan 2424

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	74.5	7987	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	57.1	6123	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	58.7	6295	PASS
197	198	0.00	2	1.1	115	PASS
198	198	100	100	100.0	10725	PASS
199	198	5	9	6.9	741	PASS
275	198	10	60	30.3	3245	PASS
365	198	1	100	5.8	620	PASS
441	198	0.01	100	15.4	1650	PASS
442	198	50	100	84.2	9029	PASS
443	442	15	24	19.6	1772	PASS

Instrument :

BNA_M

ClientSampleId :

DFTPP023

m/z	Abundance
38.90	754.0
49.90	3123.0
50.90	9087.0
51.90	342.0
55.80	303.0
56.90	786.0
62.90	472.0
68.90	6581.0
74.00	1306.0
74.90	1395.0
75.90	491.0
76.90	11049.0
77.90	788.0
78.90	626.0
79.90	453.0
80.90	567.0
81.90	153.0
85.80	157.0
91.90	162.0
92.90	982.0
97.80	1117.0
98.80	733.0
100.90	183.0
104.00	225.0
106.90	2679.0
107.80	375.0
109.90	2315.0
110.80	556.0
116.80	4315.0
117.80	152.0
121.70	178.0
122.80	289.0
124.80	185.0
126.90	6075.0
127.90	514.0
128.80	2946.0
129.90	464.0
134.80	256.0
140.90	576.0
141.80	183.0
146.80	207.0
147.90	1346.0
148.80	192.0
152.90	155.0
153.80	221.0
154.90	370.0
155.90	191.0
159.80	190.0
160.80	166.0
164.70	162.0
166.90	1732.0
167.90	1014.0
173.80	247.0
174.80	360.0
176.80	183.0
178.80	852.0
179.80	545.0
180.70	156.0
184.90	323.0
185.90	2216.0
186.90	528.0
188.90	226.0
191.70	173.0
192.80	325.0
195.80	305.0
197.80	10001.0
198.80	733.0
203.80	671.0
204.90	1211.0
205.90	3807.0
207.00	568.0
208.00	269.0
215.70	185.0
216.90	1595.0
217.90	212.0
220.80	301.0
222.90	350.0
223.90	2507.0
224.90	744.0
226.90	1209.0
227.80	176.0
228.70	164.0
235.80	201.0
241.70	237.0
243.90	1465.0
244.80	321.0
245.80	412.0
254.90	7306.0
255.90	1311.0
256.70	162.0
257.90	736.0
272.90	271.0

Instrument :
BNA_M
ClientSampleId :
DFTPP023

273.80	834.0
274.80	2568.0
275.80	414.0
276.80	276.0
295.90	1216.0
296.90	192.0
322.90	264.0
333.90	179.0
352.90	172.0
364.80	500.0
371.80	166.0
423.00	318.0
441.00	1078.0
441.90	6454.0
443.00	1473.0

Instrument :
BNA_M
ClientSampleId :
DFTPP023

m/z	Abundance
37.90	173.0
38.90	702.0
39.90	155.0
49.90	3022.0
50.90	9778.0
52.00	499.0
55.80	209.0
57.00	340.0
62.90	300.0
68.90	7091.0
72.80	159.0
73.90	1467.0
74.90	1422.0
75.90	993.0
76.90	13278.0
77.90	648.0
78.90	730.0
79.80	419.0
80.90	714.0
82.00	219.0
85.80	356.0
91.70	237.0
92.80	1469.0
97.90	1368.0
98.80	633.0
100.70	345.0
103.80	183.0
104.80	182.0
106.90	2866.0
107.80	455.0
109.90	3627.0
110.80	654.0
116.00	173.0
116.90	5460.0
117.90	263.0
121.90	203.0
122.80	500.0
126.90	7781.0
128.00	496.0
128.80	3695.0
129.80	348.0
134.80	352.0
136.80	236.0
140.80	566.0
142.80	205.0
147.00	174.0
147.80	1424.0
148.80	290.0
150.80	150.0
152.80	268.0
153.80	190.0
154.80	385.0
156.00	467.0
159.70	271.0
160.90	413.0
164.60	170.0
166.90	2131.0
167.90	1421.0
172.80	175.0
173.80	167.0
174.90	506.0
176.90	249.0
178.80	1346.0
179.80	536.0
180.90	333.0
184.90	368.0
185.90	2622.0
186.80	775.0
188.70	266.0
191.70	263.0
192.80	368.0
193.90	187.0
195.90	279.0
196.80	192.0
197.80	13031.0
198.80	993.0
202.80	193.0
204.00	910.0
204.90	1794.0
205.90	5100.0
206.90	710.0
207.80	213.0
216.80	1467.0
217.80	184.0
220.80	492.0
221.90	174.0
222.80	329.0
223.90	3290.0
224.90	710.0
226.80	1485.0
228.00	282.0
228.80	380.0

Instrument :
BNA_M
ClientSampleId :
DFTPP023

230.90	151.0
236.00	240.0
236.90	192.0
241.90	169.0
242.90	262.0
243.90	2079.0
244.90	415.0
245.80	534.0
254.90	11611.0
255.80	1777.0
257.90	810.0
264.90	461.0
272.70	263.0
273.80	1007.0
274.90	4575.0
275.90	559.0
276.90	392.0
295.80	1887.0
296.90	159.0
302.70	168.0
322.80	372.0
334.00	385.0
345.90	153.0
364.90	687.0
422.80	625.0
423.80	206.0
441.00	2095.0
441.90	10318.0
442.90	2160.0
443.80	171.0

Instrument :
BNA_M
ClientSampleId :
DFTPP023

m/z	Abundance
38.90	370.0
49.90	1910.0
50.90	5096.0
51.90	270.0
56.80	237.0
62.80	365.0
68.90	4697.0
73.90	827.0
74.90	1123.0
75.80	451.0
76.90	8110.0
78.00	424.0
78.90	353.0
80.90	439.0
91.80	313.0
92.90	1204.0
97.90	705.0
98.80	535.0
100.90	157.0
103.80	158.0
104.80	172.0
106.90	1674.0
107.90	209.0
109.90	2223.0
110.90	550.0
116.90	2676.0
117.70	293.0
122.80	235.0
123.80	152.0
126.90	5028.0
127.80	521.0
128.80	2139.0
129.80	263.0
134.70	206.0
136.90	156.0
140.80	248.0
146.80	252.0
147.80	753.0
155.80	312.0
161.00	182.0
166.80	1408.0
167.80	836.0
173.80	151.0
175.00	301.0
178.80	688.0
179.80	532.0
180.80	221.0
184.80	302.0
185.90	1685.0
186.80	535.0
191.70	390.0
192.80	167.0
196.10	301.0
196.90	152.0
197.80	9143.0
198.70	496.0
203.80	743.0
204.90	1099.0
205.90	3329.0
206.90	604.0
207.90	173.0
216.90	1359.0
217.80	243.0
220.90	412.0
221.90	216.0
222.80	189.0
223.90	2202.0
225.00	497.0
226.80	1157.0
227.80	234.0
228.80	212.0
241.90	199.0
242.90	154.0
243.90	1921.0
244.90	395.0
245.90	598.0
254.90	8530.0
255.80	1190.0
257.80	619.0
264.80	324.0
272.80	408.0
273.80	564.0
274.90	2592.0
276.00	338.0
276.90	313.0
295.90	1212.0
296.80	179.0
302.90	165.0
314.80	246.0
323.00	414.0
333.80	192.0
364.90	674.0

Instrument :
BNA_M
ClientSampleId :
DFTPP023

371.80	176.0
422.90	414.0
424.00	182.0
440.90	1778.0
441.90	10315.0
442.90	1684.0
444.00	231.0

Instrument :
BNA_M
ClientSampleId :
DFTPP023