

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM050719\
 Data File : BM020176.D
 Acq On : 07 May 2019 21:54
 Operator : JU/SJ
 Sample : K2697-07
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 MW-4-20190502-A

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM043019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.369	399	405	413	rBV	1364535	1957932	20.05%	4.647%
2	6.951	667	674	683	rBV	865267	1354794	13.87%	3.215%
3	7.316	728	736	745	rBV	2317774	3795024	38.85%	9.007%
4	7.787	808	816	823	rBV	483443	769636	7.88%	1.827%
5	8.104	863	870	878	rBV	2065952	3287249	33.66%	7.801%
6	8.951	1007	1014	1024	rBV	1677511	2847858	29.16%	6.759%
7	10.581	1284	1291	1300	rBV	525385	919673	9.42%	2.183%
8	13.051	1703	1711	1723	rBV	4162957	6015090	61.58%	14.275%
9	14.292	1912	1922	1930	rBV2	43189	111331	1.14%	0.264%
10	14.433	1939	1946	1952	rBV2	787143	1209383	12.38%	2.870%
11	15.921	2192	2199	2215	rBV	3260542	4768549	48.82%	11.317%
12	17.180	2406	2413	2423	rBV	1023593	1481538	15.17%	3.516%
13	18.057	2557	2562	2569	rBV3	77818	135510	1.39%	0.322%
14	19.803	2853	2859	2869	rBV	8038395	9767335	100.00%	23.180%
15	21.362	3119	3124	3132	rBV	1443992	1842584	18.86%	4.373%
16	23.650	3507	3513	3521	rVB	939783	1872644	19.17%	4.444%


Sum of corrected areas: 42136130

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM050719\
Data File : BM020176.D
Acq On : 07 May 2019 21:54
Operator : JU/SJ
Sample : K2697-07
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
MW-4-20190502-A

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM043019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

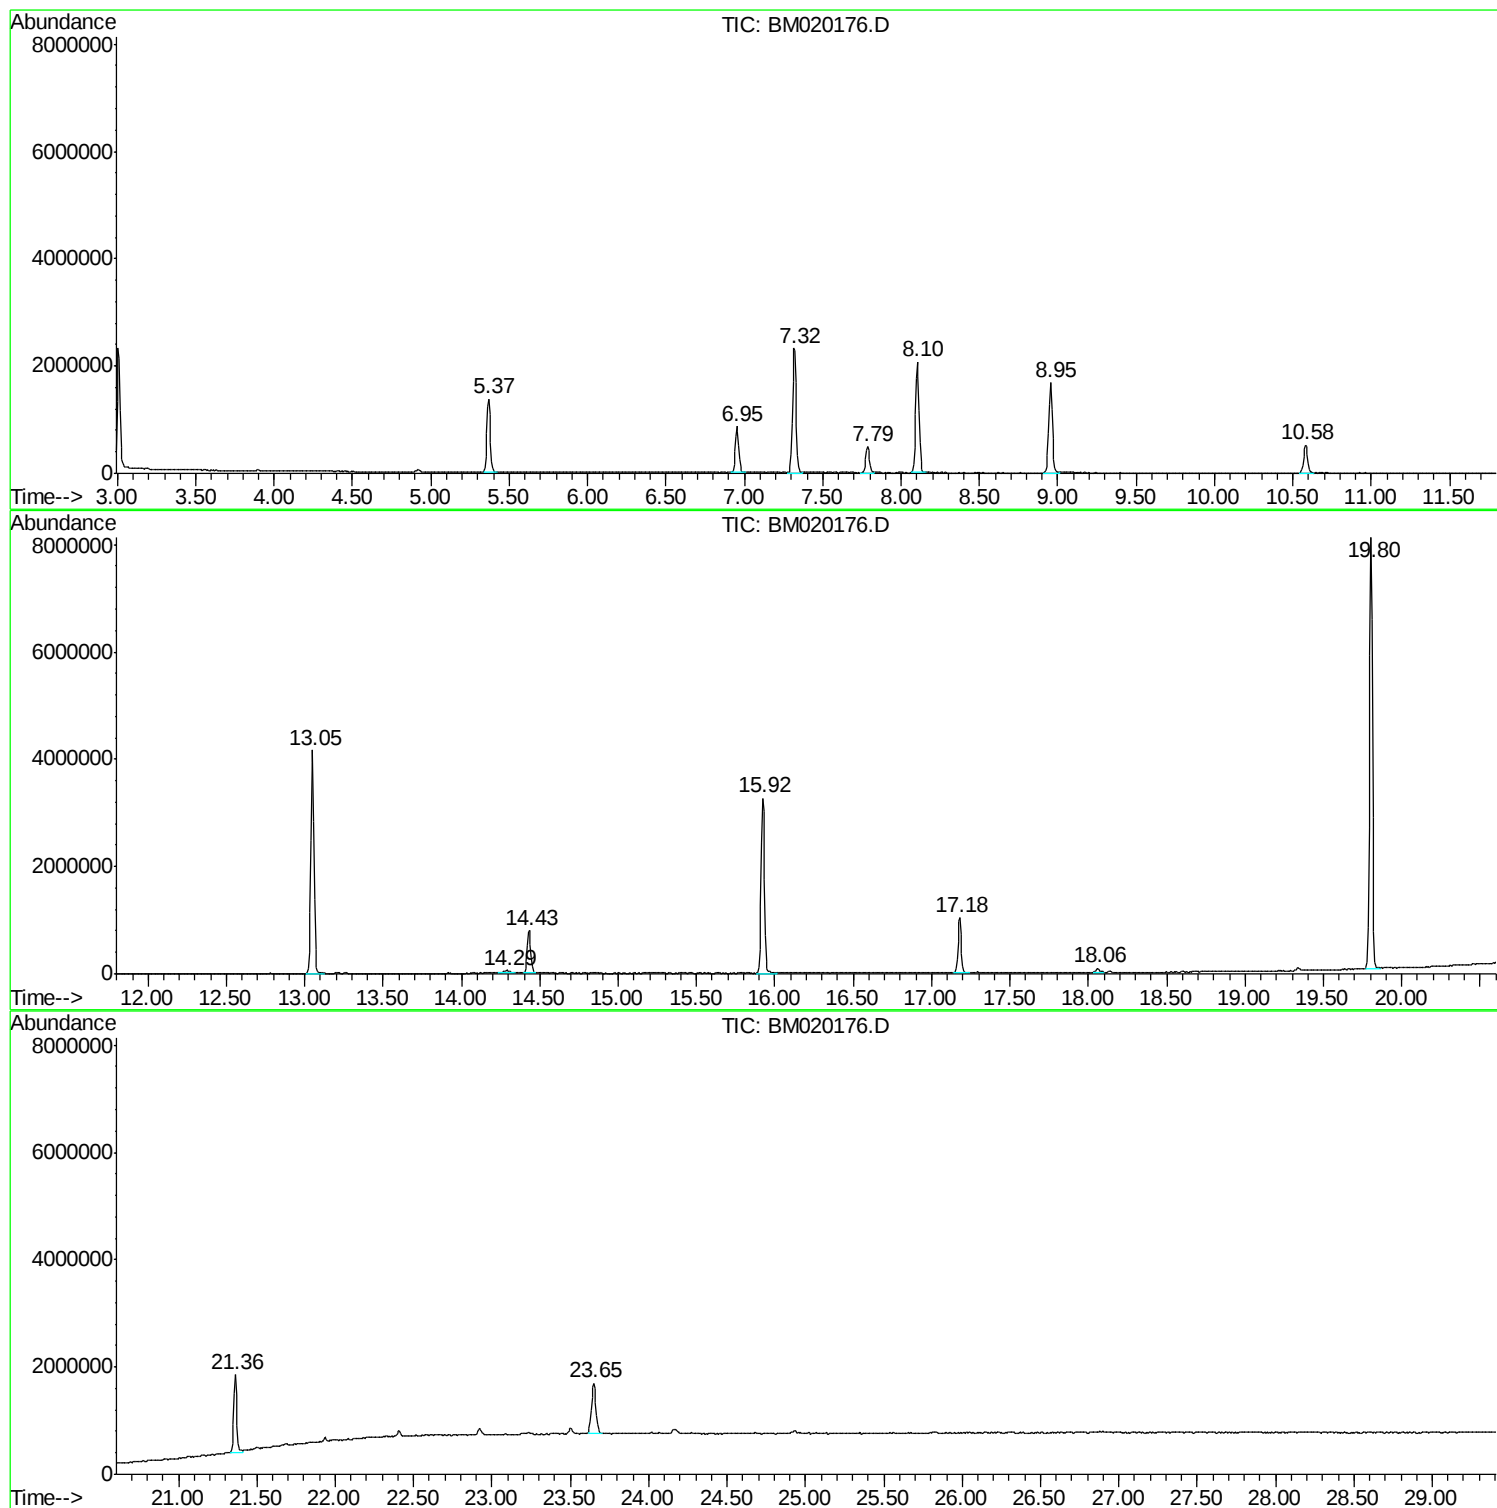

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM050719\
Data File : BM020176.D
Acq On : 07 May 2019 21:54
Operator : JU/SJ
Sample : K2697-07
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
MW-4-20190502-A










Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM043019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.32 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.32	98.62 ng	3795020	1,4-Dichlorobenzene-d4	7.79

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	1,3-Cyclopentanedione, 2-chloro-	132	C5H5ClO2	014203-19-1	25
2		3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	14
3		4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	14
4		1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	10
5		1,3,4-Thiadiazole-2(3H)-thione, ...	132	C3H4N2S2	029490-19-5	10

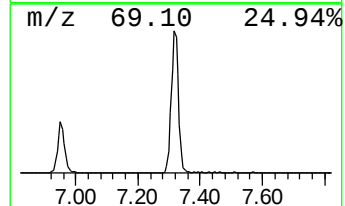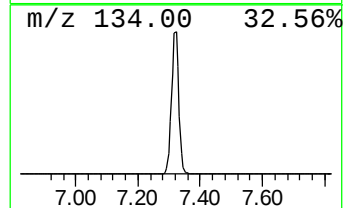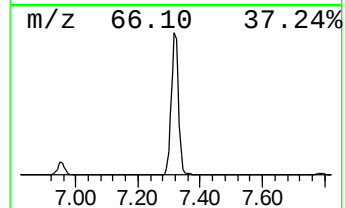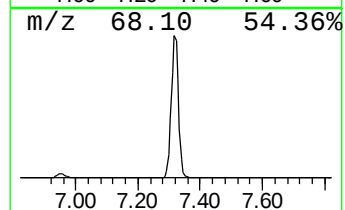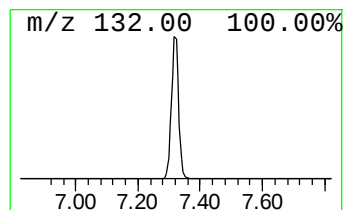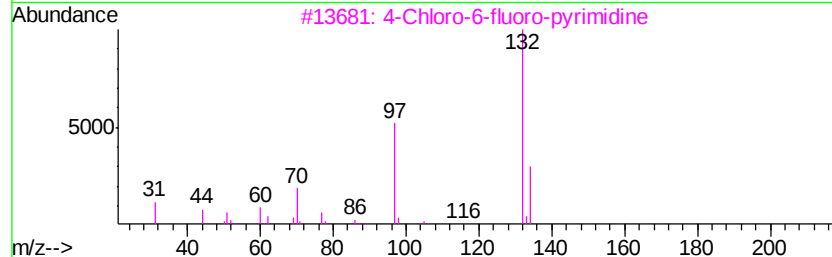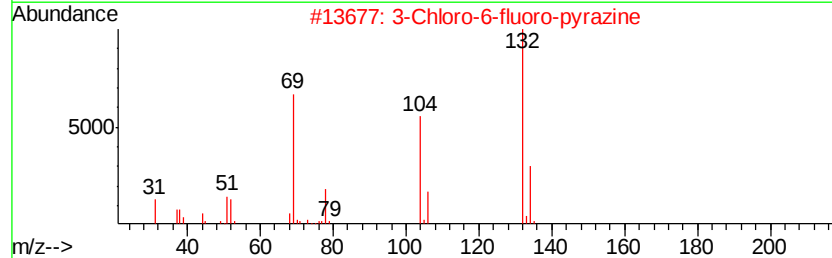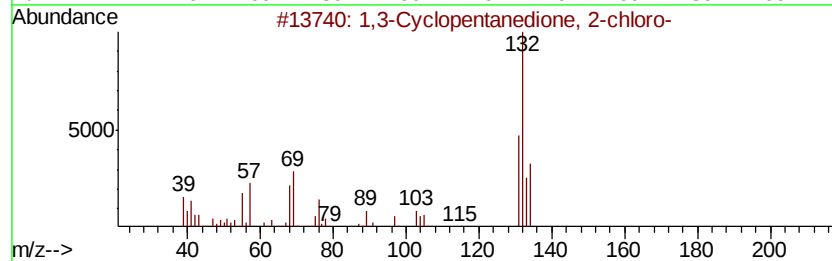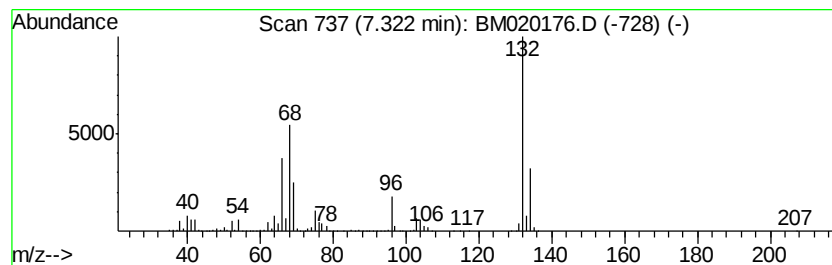

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM050719\
Data File : BM020176.D
Acq On : 07 May 2019 21:54
Operator : JU/SJ
Sample : K2697-07
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
MW-4-20190502-A

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM043019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---			
					#	RT	Resp	Conc
unknown7.32	7.32	98.6	ng	3795020	1	7.79	769636	20.0