


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM050719\
 Data File : BM020167.D
 Acq On : 07 May 2019 16:25
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM043019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 01 03:58:37 2019

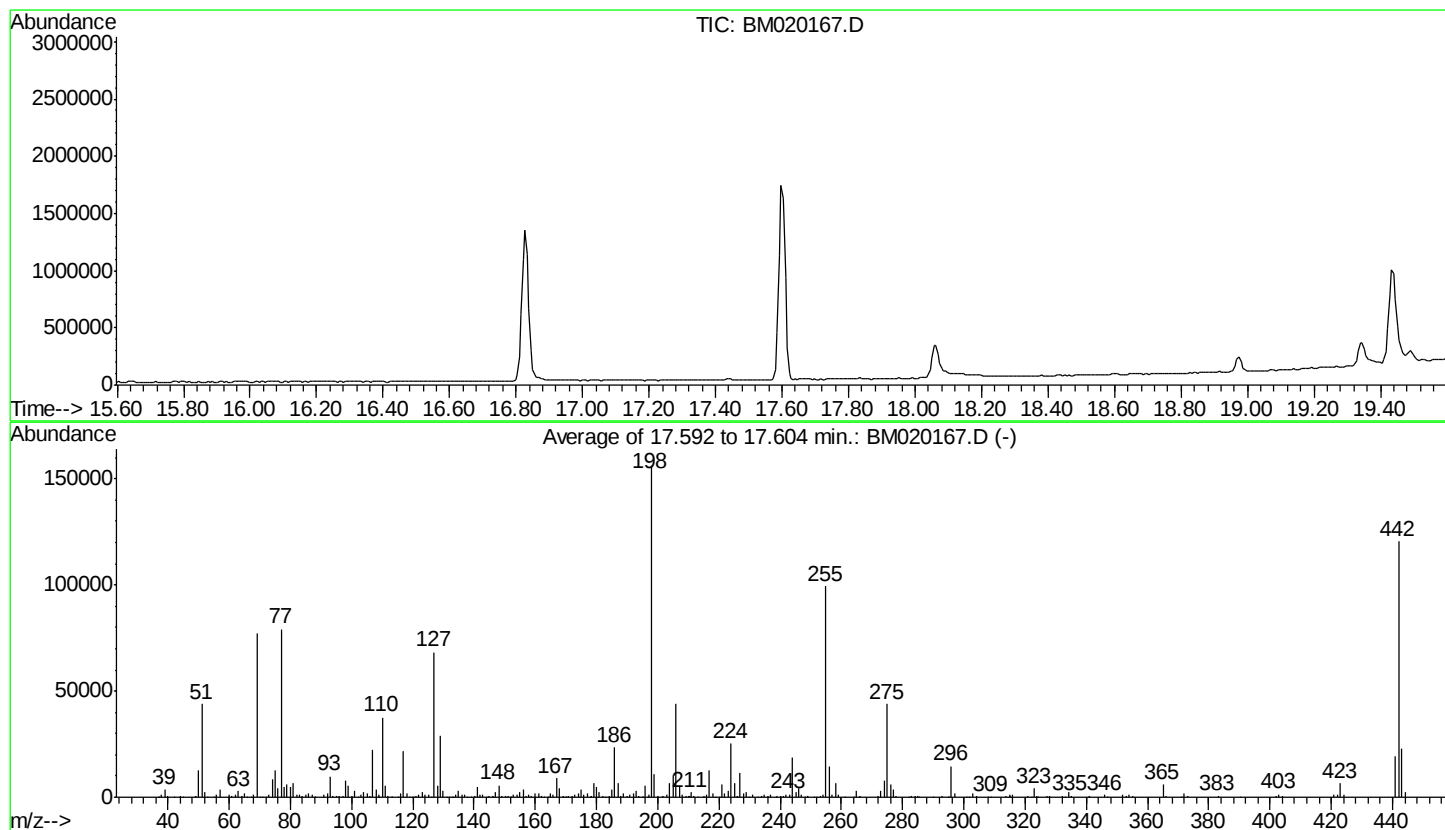

AutoFind: Scans 2483, 2484, 2485; Background Corrected with Scan 2477

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.1	43845	PASS
68	69	0.00	2	1.7	1325	PASS
69	198	0.00	100	49.2	76910	PASS
70	69	0.00	2	0.4	300	PASS
127	198	10	80	43.8	68389	PASS
197	198	0.00	2	0.6	986	PASS
198	198	100	100	100.0	156208	PASS
199	198	5	9	6.9	10749	PASS
275	198	10	60	28.1	43936	PASS
365	198	1	100	3.7	5837	PASS
441	198	0.01	100	12.3	19202	PASS
442	198	50	100	77.1	120408	PASS
443	442	15	24	19.3	23208	PASS