


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM050719\  
 Data File : BM020187.D  
 Acq On : 08 May 2019 05:13  
 Operator : JU/SJ  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\8270-BM043019.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Wed May 01 03:58:37 2019

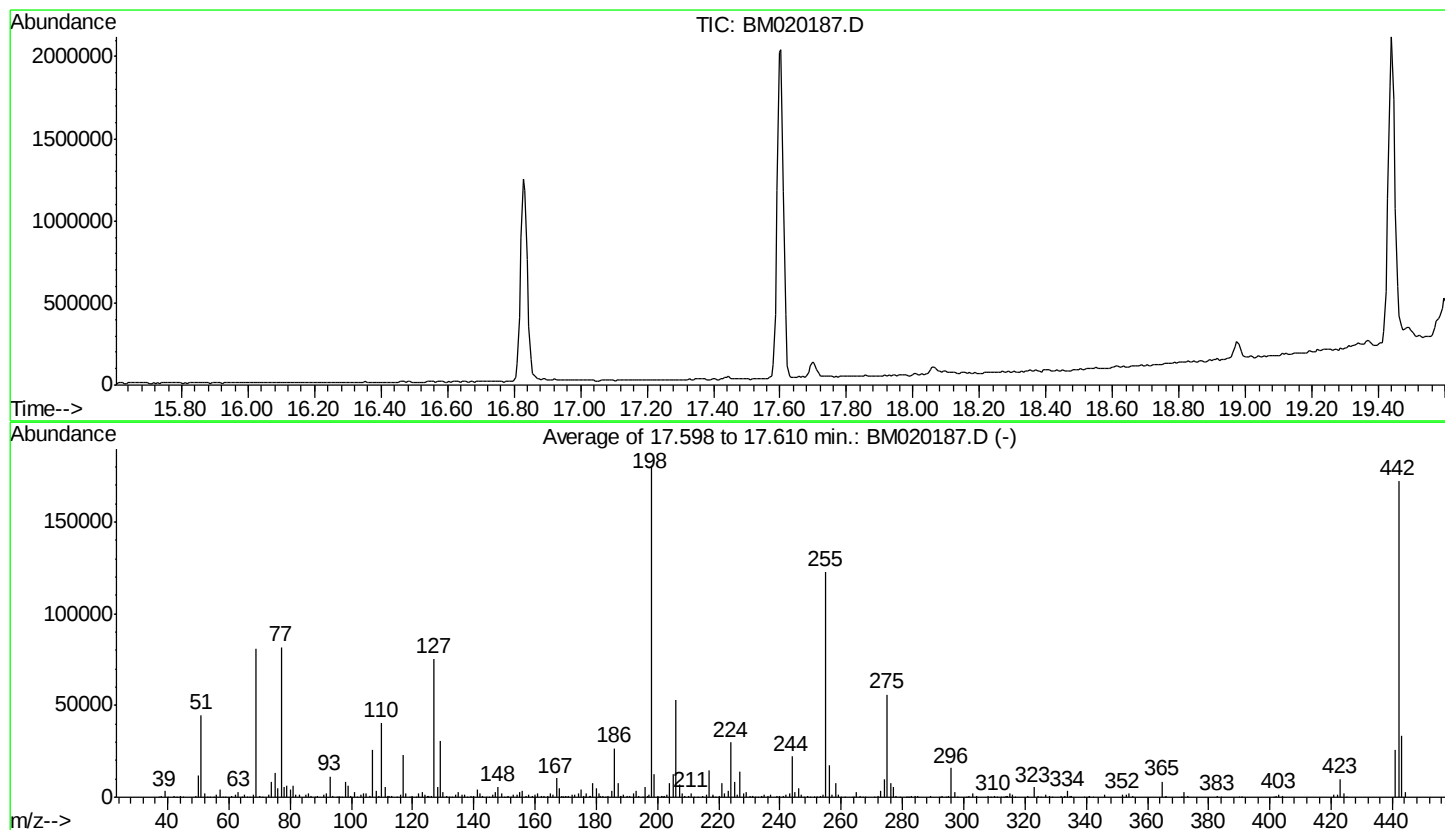

AutoFind: Scans 2484, 2485, 2486; Background Corrected with Scan 2477

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 24.7      | 44634   | PASS             |
| 68          | 69           | 0.00         | 2            | 1.5       | 1244    | PASS             |
| 69          | 198          | 0.00         | 100          | 44.8      | 80959   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.8       | 627     | PASS             |
| 127         | 198          | 10           | 80           | 41.9      | 75613   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.8       | 1395    | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 180624  | PASS             |
| 199         | 198          | 5            | 9            | 6.8       | 12224   | PASS             |
| 275         | 198          | 10           | 60           | 31.0      | 56053   | PASS             |
| 365         | 198          | 1            | 100          | 4.6       | 8373    | PASS             |
| 441         | 198          | 0.01         | 100          | 14.2      | 25680   | PASS             |
| 442         | 198          | 50           | 100          | 95.5      | 172501  | PASS             |
| 443         | 442          | 15           | 24           | 19.6      | 33837   | PASS             |