
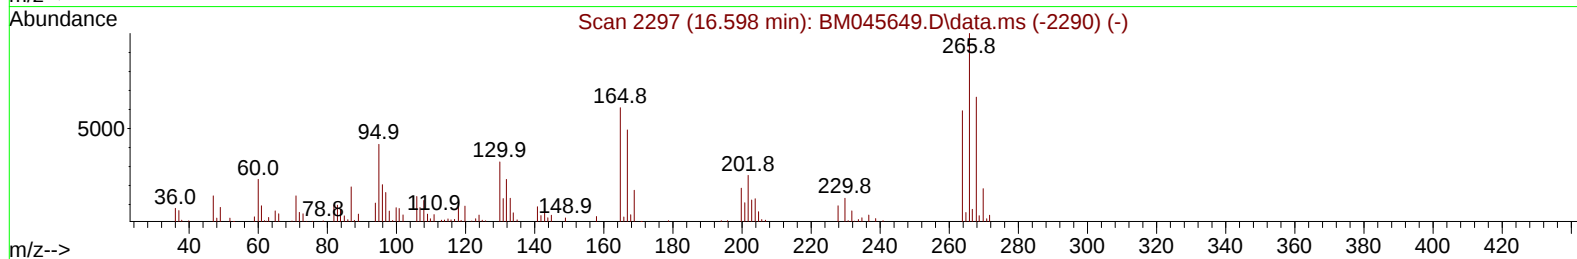
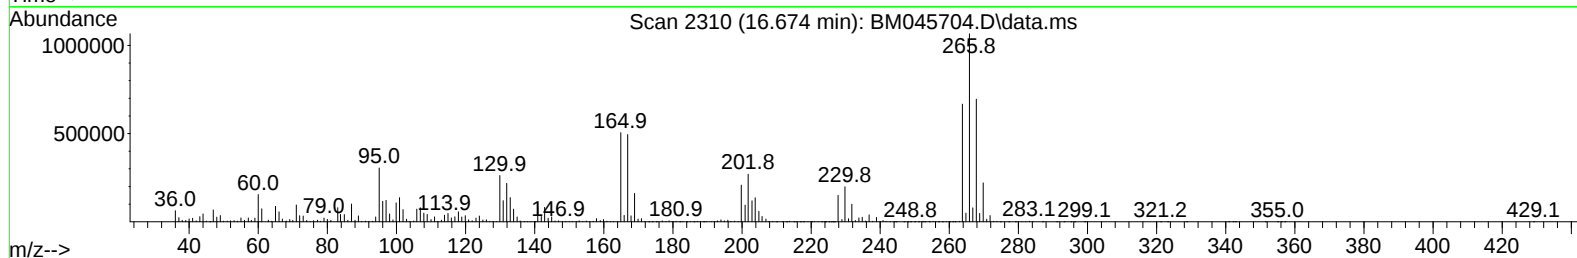


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050824\
Data File : BM045704.D
Acq On : 08 May 2024 09:10
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 08 13:09:49 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM050824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 03 15:08:07 2024
Response via : Initial Calibration

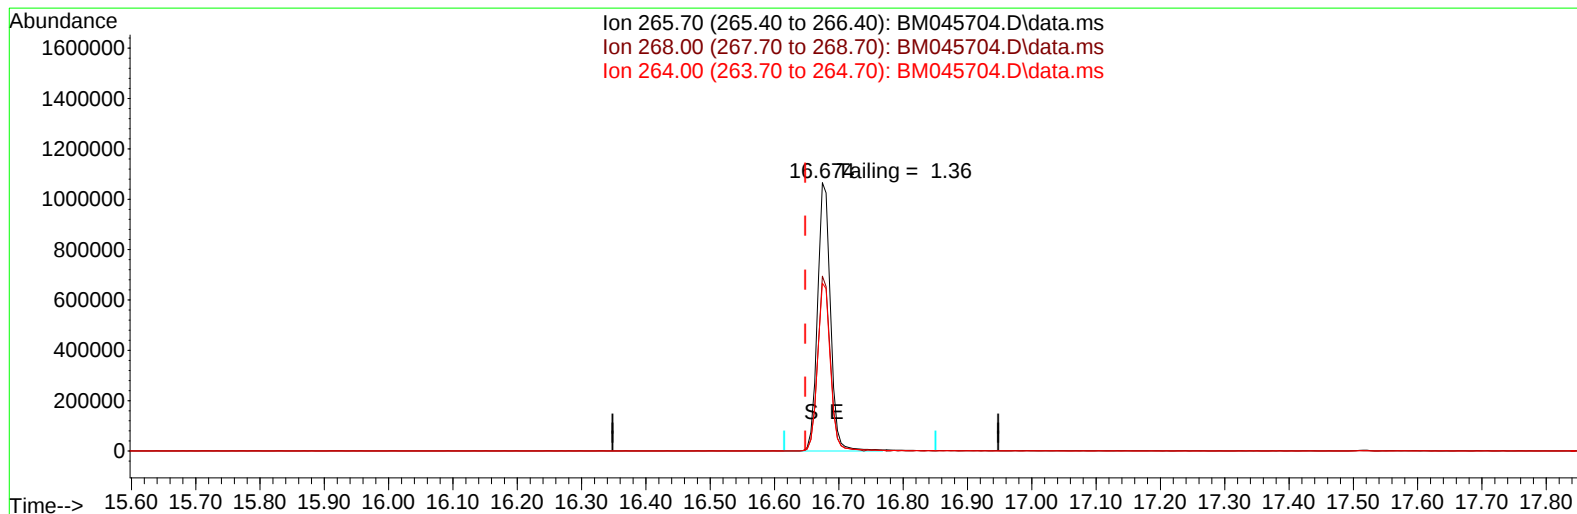

TIC: BM045704.D\data.ms

(70) Pentachlorophenol (C)**16.674min (+ 0.026) 418184.64 ng****response 1505406**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.70	65.18
264.00	59.40	62.58
0.00	0.00	0.00

