

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050824\
Data File : BM045714.D
Acq On : 08 May 2024 15:58
Operator : MA/JU
Sample : PB160503BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB160503BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM050824.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM045714.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.257	363	369	383	rBV	15054246	21118021	45.88%	10.387%
2	6.822	627	635	644	rBV	14757085	22512026	48.91%	11.073%
3	7.645	768	775	785	rVB	2512729	3826614	8.31%	1.882%
4	8.787	961	969	978	rBV	8460818	13892923	30.18%	6.833%
5	10.416	1239	1246	1254	rBV	3549191	5688667	12.36%	2.798%
6	12.910	1659	1670	1677	rBV	21124448	31108777	67.58%	15.301%
7	14.280	1896	1903	1911	rBV	5576921	7682906	16.69%	3.779%
8	15.768	2146	2156	2176	rBV	16706320	23155169	50.30%	11.389%
9	17.027	2360	2370	2376	rBV	6433603	9173748	19.93%	4.512%
10	19.674	2814	2820	2825	rBV	38076678	46031290	100.00%	22.641%
11	21.215	3076	3082	3094	rBV	7726139	9281533	20.16%	4.565%
12	23.415	3448	3456	3467	rBV	5419516	9835190	21.37%	4.838%




Sum of corrected areas: 203306864

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050824\
Data File : BM045714.D
Acq On : 08 May 2024 15:58
Operator : MA/JU
Sample : PB160503BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB160503BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM050824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

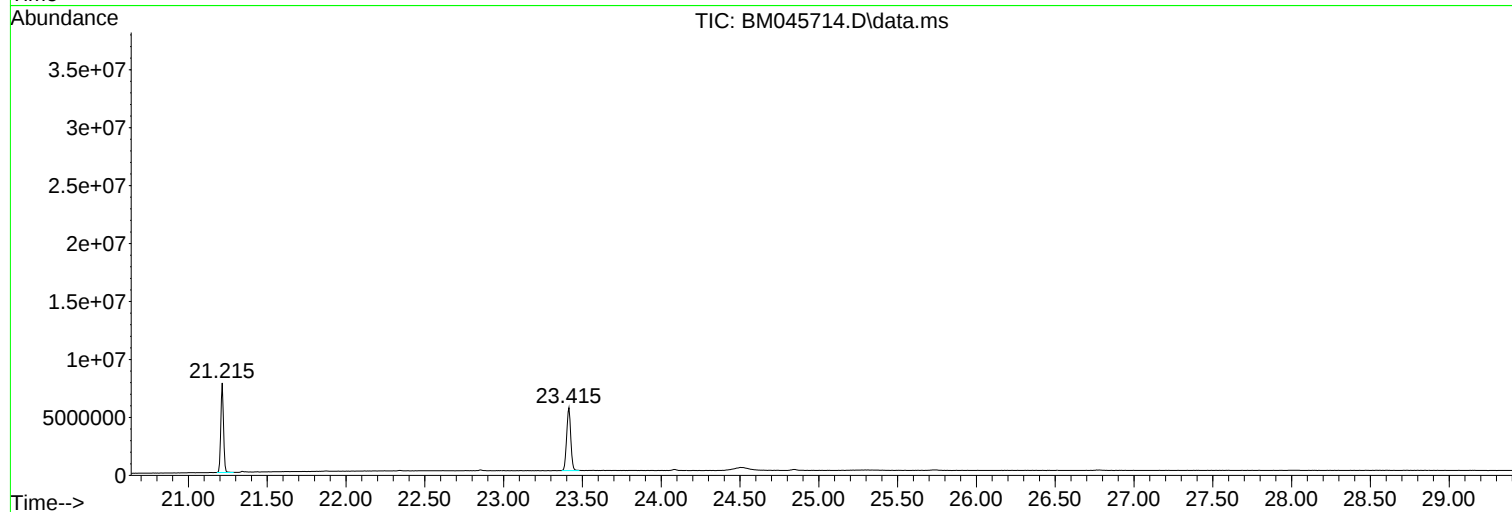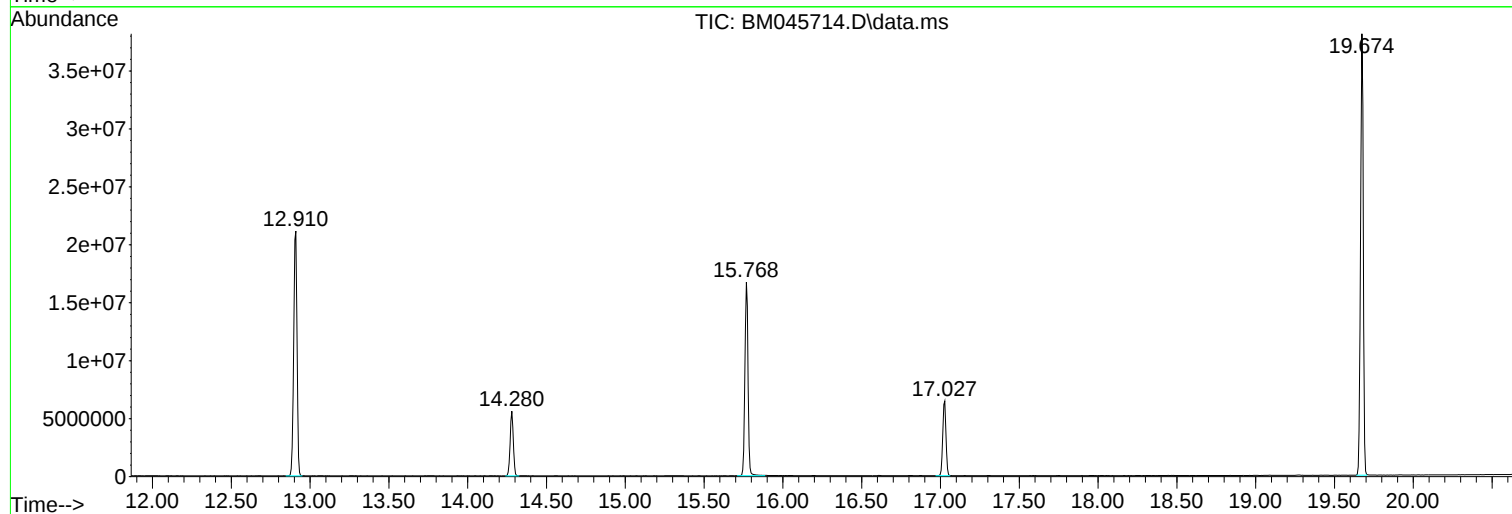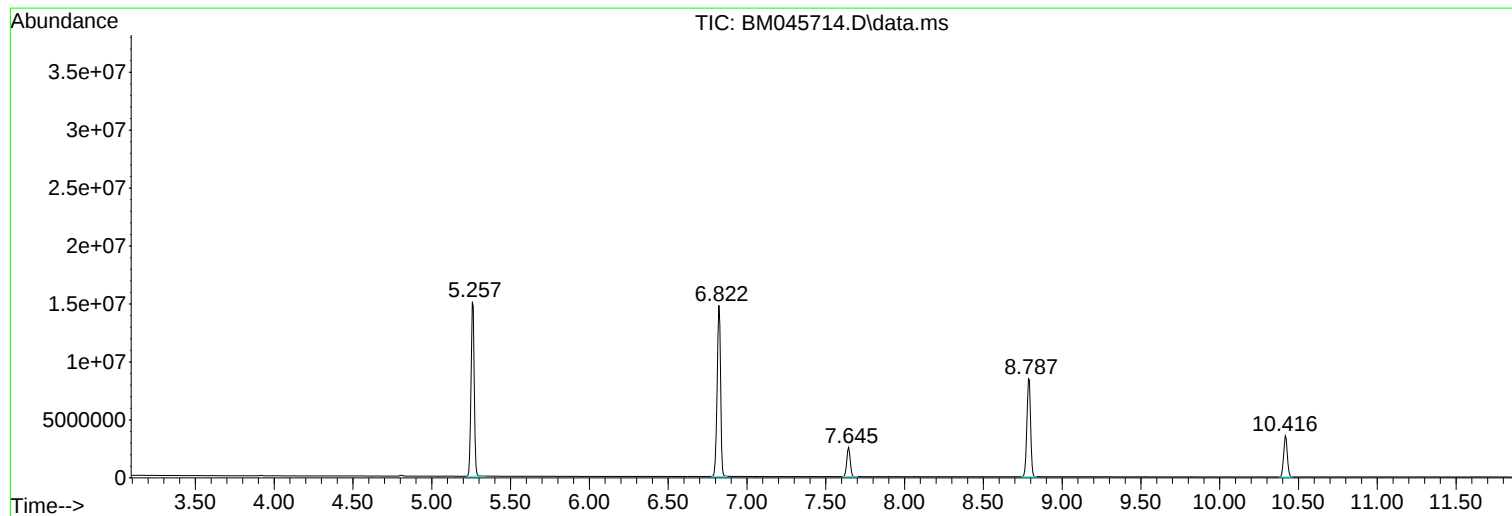

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050824\
Data File : BM045714.D
Acq On : 08 May 2024 15:58
Operator : MA/JU
Sample : PB160503BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB160503BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM050824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050824\
Data File : BM045714.D
Acq On : 08 May 2024 15:58
Operator : MA/JU
Sample : PB160503BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB160503BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM050824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------