


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050824\
Data File : BM045704.D
Acq On : 08 May 2024 09:10
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM050824.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed May 08 16:45:57 2024

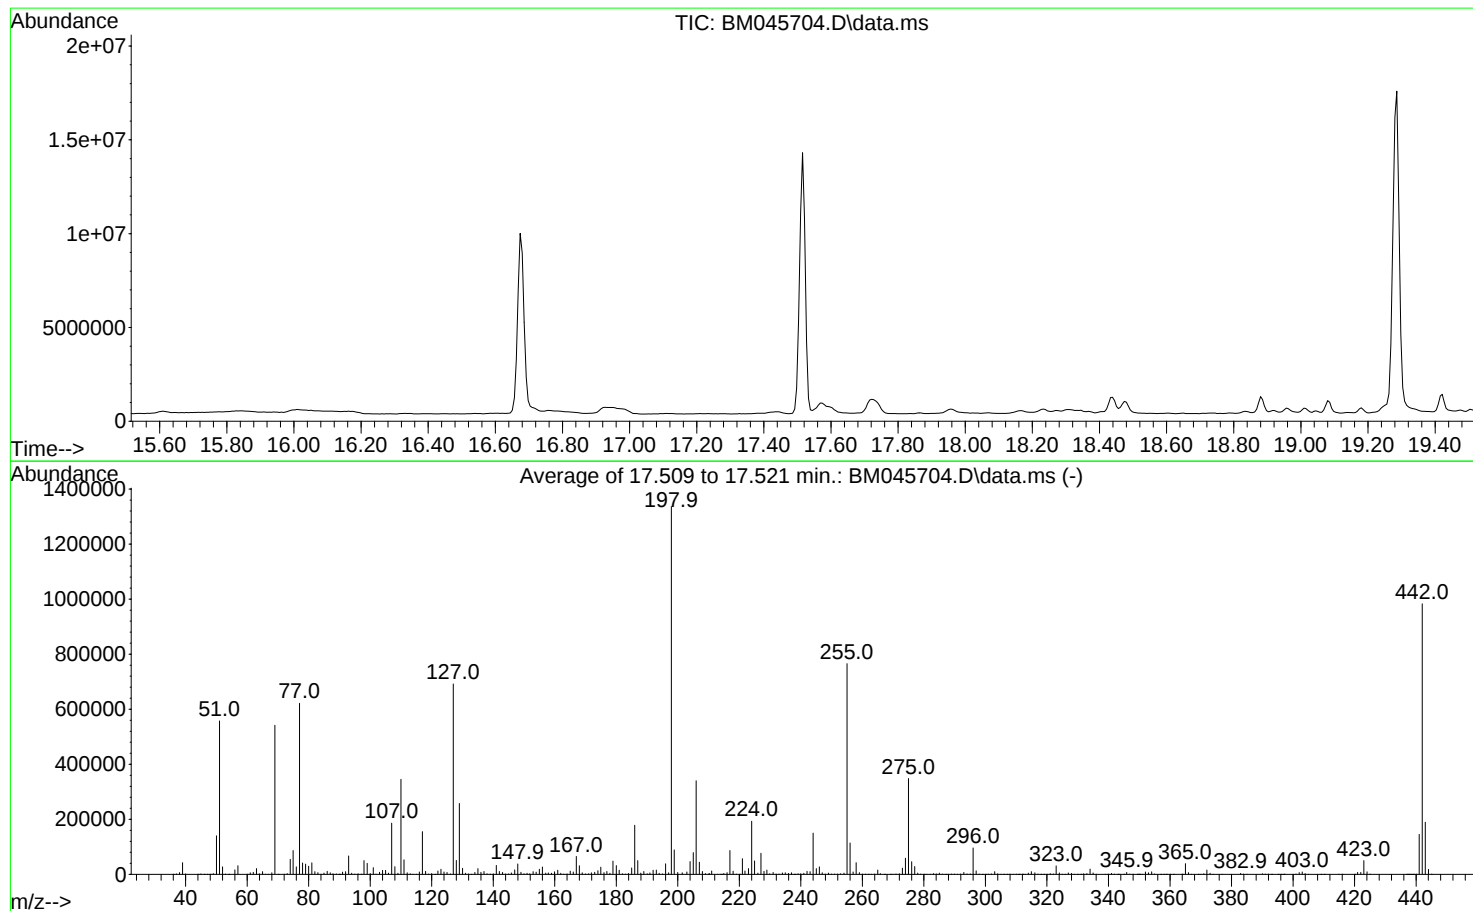




AutoFind: Scans 2452, 2453, 2454; Background Corrected with Scan 2440

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	41.7	557426	PASS
68	69	0.00	2	1.1	6072	PASS
69	198	0.00	100	40.6	541995	PASS
70	69	0.00	2	0.0	247	PASS
127	198	10	80	51.8	691986	PASS
197	198	0.00	2	0.4	5919	PASS
198	198	100	100	100.0	1336529	PASS
199	198	5	9	6.7	88925	PASS
275	198	10	60	26.0	348160	PASS
365	198	1	100	2.9	39163	PASS
441	198	0.01	100	10.9	145563	PASS
442	442	50	100	100.0	983339	PASS
443	442	15	24	19.3	189397	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050824\
Data File : BM045704.D
Acq On : 08 May 2024 09:10
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: May 08 13:09:49 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM050824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 03 15:08:07 2024
Response via : Initial Calibration

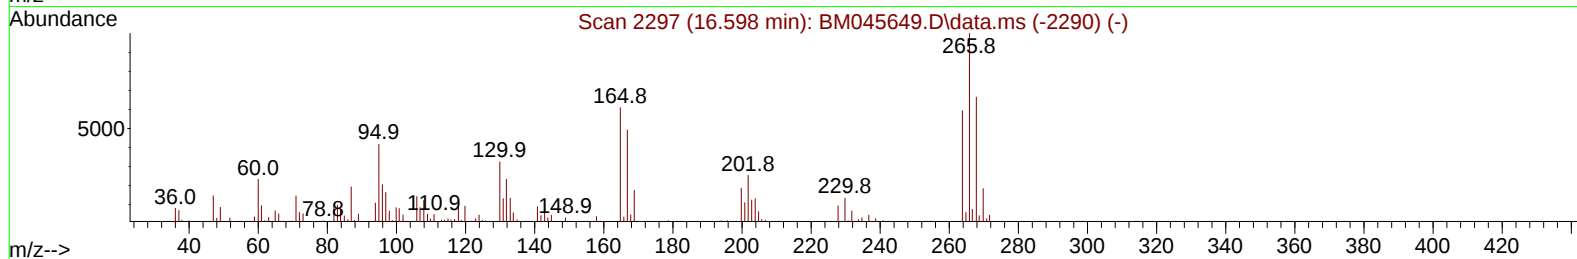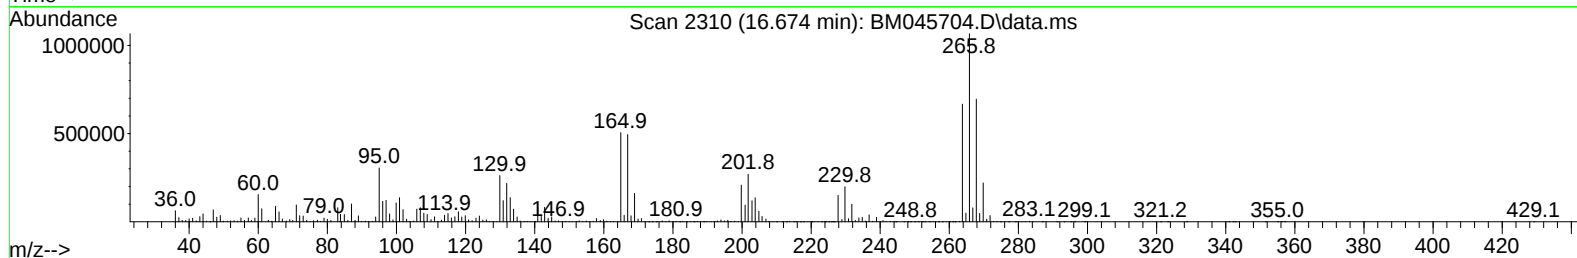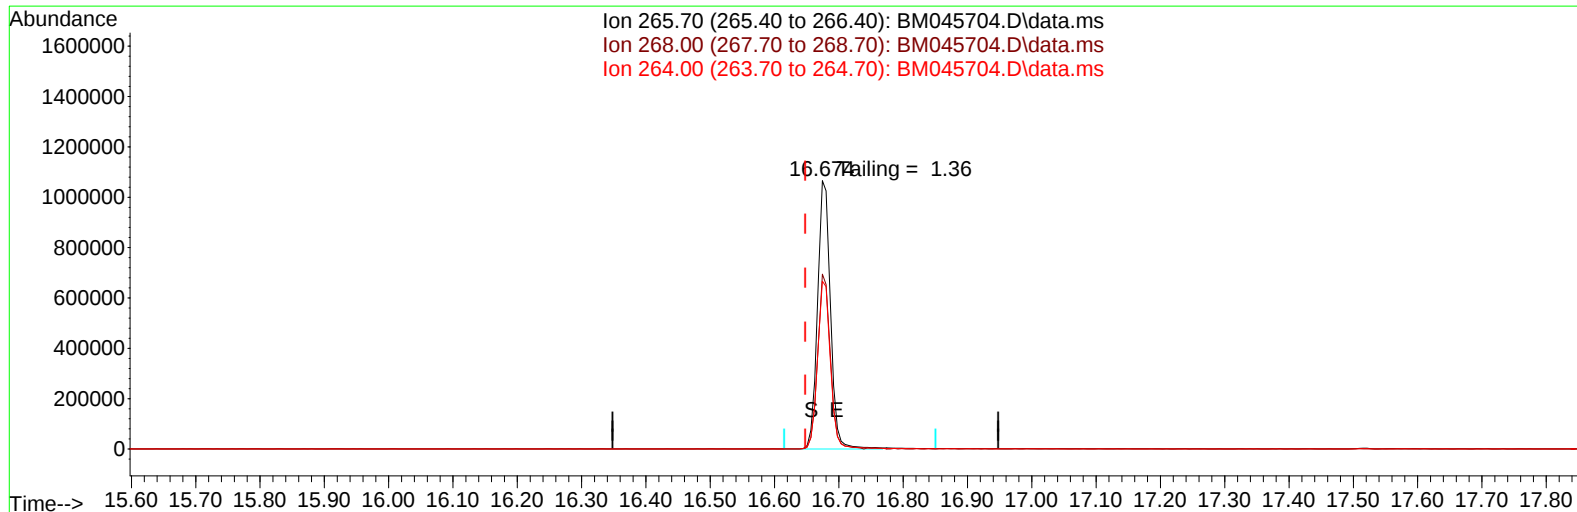

TIC: BM045704.D\data.ms

(70) Pentachlorophenol (C)

16.674min (+ 0.026) 418184.64 ng




response 1505406

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.70	65.18
264.00	59.40	62.58
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050824\
Data File : BM045704.D
Acq On : 08 May 2024 09:10
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: May 08 13:09:49 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM050824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 03 15:08:07 2024
Response via : Initial Calibration

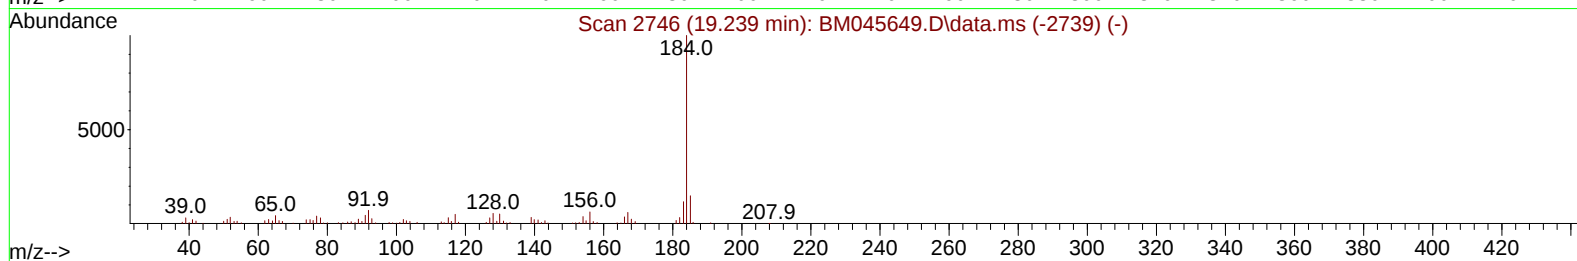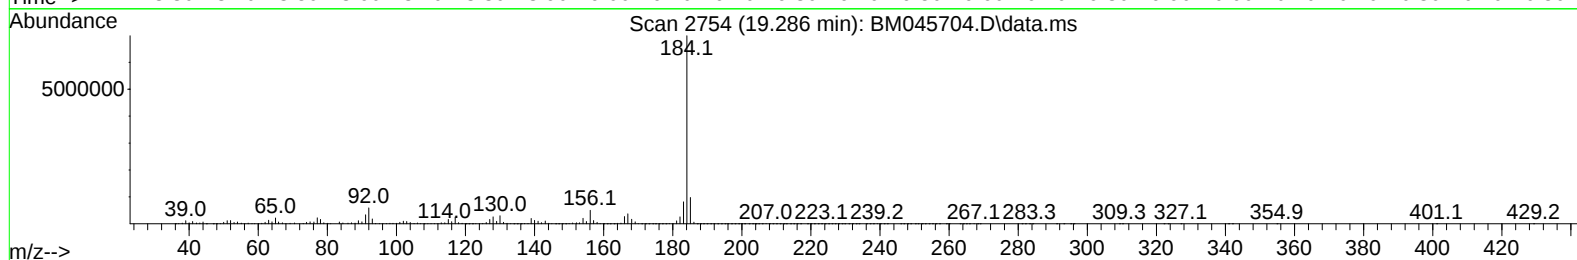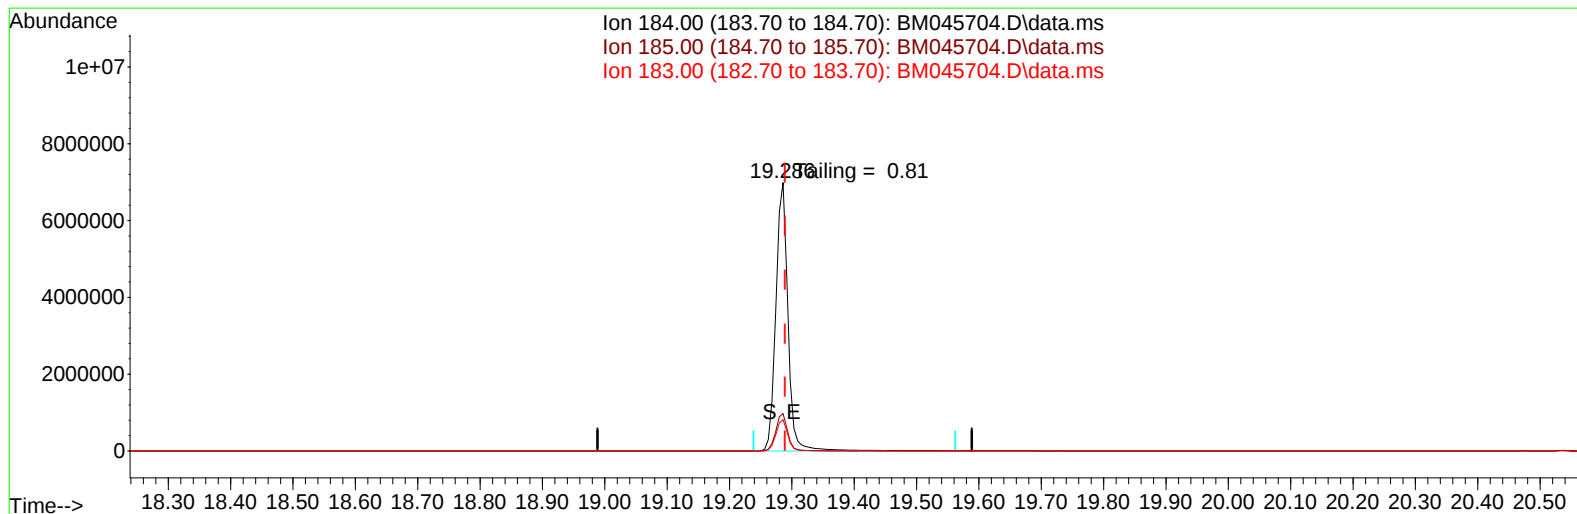

TIC: BM045704.D\data.ms

(77) Benzidine**19.286min (-0.003) 502590.34 ng****response 9520773**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	13.97
183.00	11.70	11.70
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/8/2024	BNA_M	<u>BM045704.D</u>
Compound Name	Response	Retention Time
DDT	4139842	20.539
DDD	38531	20.145
DDE	0	19.498
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
38531	4178373	0.92

Instrument :
BNA_M
ClientSampleId :
DFTPP