


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM050919\
 Data File : BM020210.D
 Acq On : 09 May 2019 10:51
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM043019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 01 03:58:37 2019

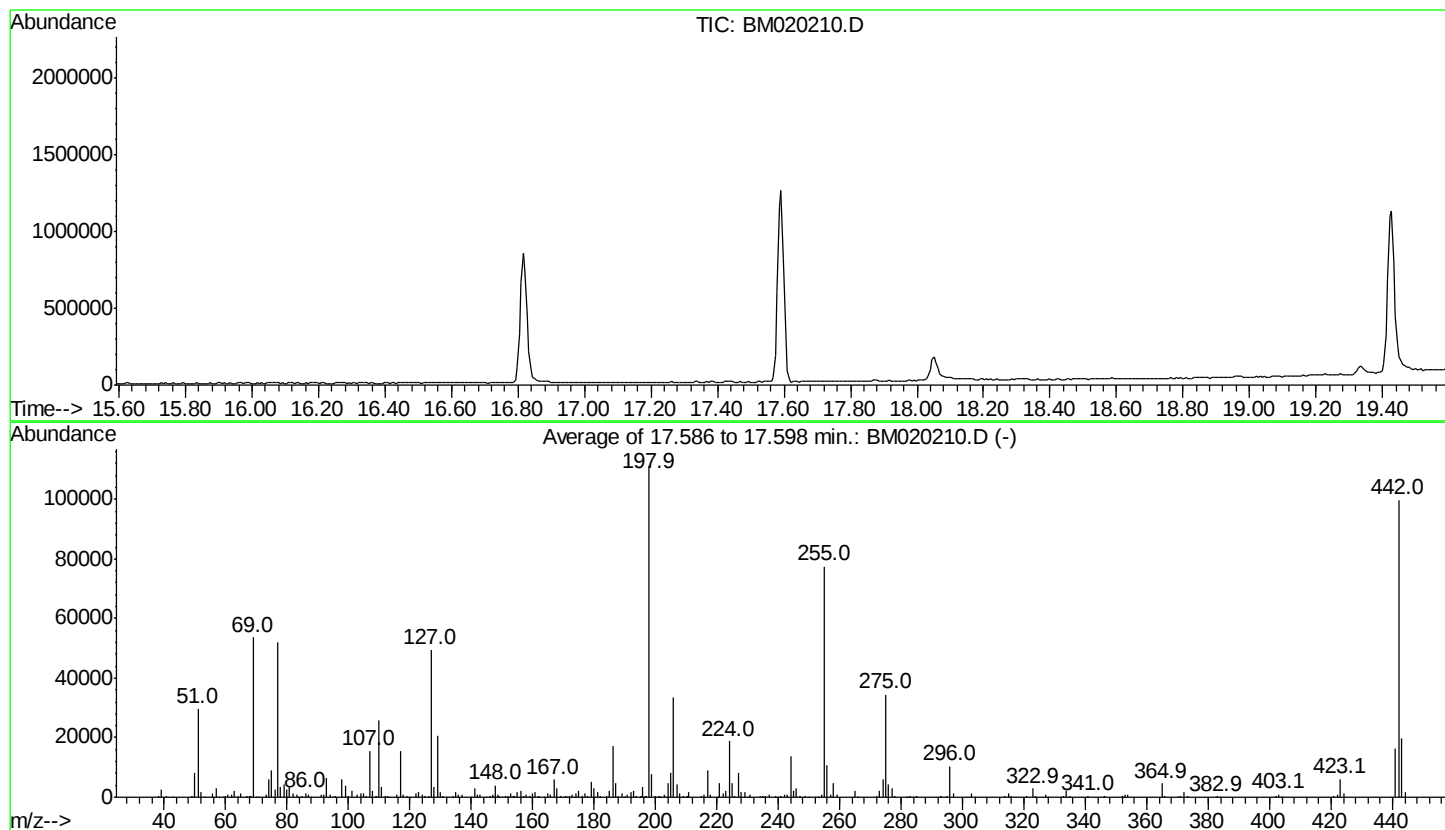

AutoFind: Scans 2482, 2483, 2484; Background Corrected with Scan 2475

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.7	29733	PASS
68	69	0.00	2	0.9	474	PASS
69	198	0.00	100	48.1	53590	PASS
70	69	0.00	2	0.4	212	PASS
127	198	10	80	44.6	49613	PASS
197	198	0.00	2	0.5	542	PASS
198	198	100	100	100.0	111306	PASS
199	198	5	9	7.1	7917	PASS
275	198	10	60	30.9	34418	PASS
365	198	1	100	4.2	4658	PASS
441	198	0.01	100	14.6	16233	PASS
442	198	50	100	89.7	99797	PASS
443	442	15	24	19.9	19874	PASS