


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM050919\
 Data File : BM020229.D
 Acq On : 10 May 2019 06:00
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM043019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 01 03:58:37 2019

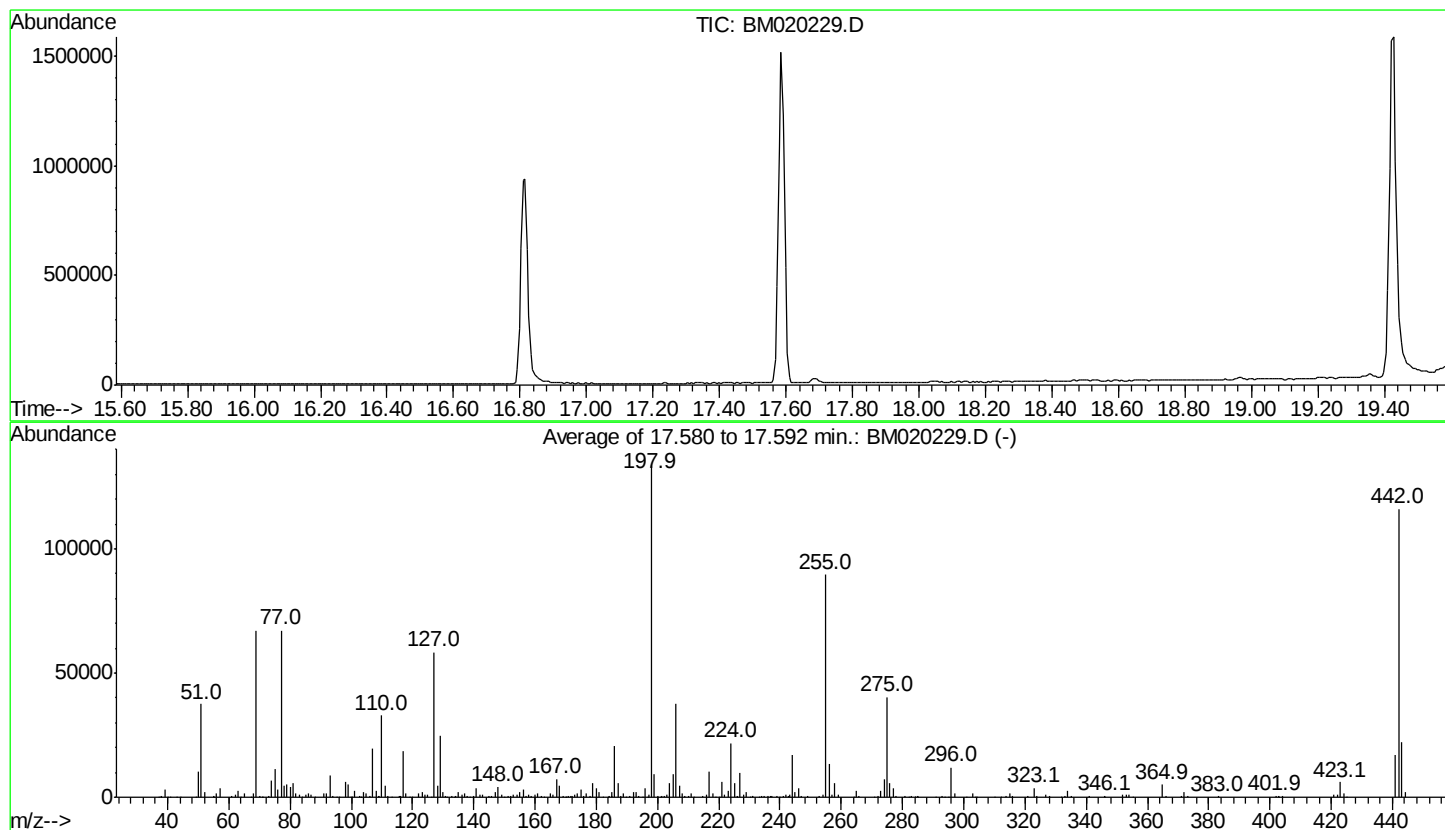

AutoFind: Scans 2481, 2482, 2483; Background Corrected with Scan 2475

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.0	37456	PASS
68	69	0.00	2	2.0	1322	PASS
69	198	0.00	100	50.1	66946	PASS
70	69	0.00	2	0.7	440	PASS
127	198	10	80	43.7	58405	PASS
197	198	0.00	2	0.7	980	PASS
198	198	100	100	100.0	133544	PASS
199	198	5	9	7.1	9472	PASS
275	198	10	60	30.1	40261	PASS
365	198	1	100	3.8	5039	PASS
441	198	0.01	100	12.7	16894	PASS
442	198	50	100	86.9	116112	PASS
443	442	15	24	18.9	21987	PASS