

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM051019\
 Data File : BM020239.D
 Acq On : 10 May 2019 13:27
 Operator : JU/SJ
 Sample : PB119565BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB119565BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM043019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.357	397	403	420	rBV	1077633	1620646	29.29%	6.710%
2	6.940	665	672	686	rBV	1094164	1777696	32.12%	7.360%
3	7.304	727	734	752	rBV	1093104	1783397	32.23%	7.383%
4	7.775	808	814	823	rBV	216998	348850	6.30%	1.444%
5	8.093	860	868	876	rBV	759913	1229702	22.22%	5.091%
6	8.940	1005	1012	1035	rBV	614005	1065482	19.25%	4.411%
7	10.569	1280	1289	1304	rBV	281461	494124	8.93%	2.046%
8	13.033	1702	1708	1730	rBV	1741452	2701846	48.82%	11.186%
9	14.422	1937	1944	1954	rBV2	498979	781359	14.12%	3.235%
10	15.910	2191	2197	2211	rBV	1757150	2529467	45.71%	10.472%
11	17.168	2405	2411	2426	rBV2	731924	1117060	20.19%	4.625%
12	19.798	2852	2858	2869	rBV	4530039	5533760	100.00%	22.910%
13	21.356	3117	3123	3133	rBV	1205411	1562088	28.23%	6.467%
14	23.644	3505	3512	3521	rVB	820666	1608956	29.08%	6.661%


Sum of corrected areas: 24154433

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM051019\
Data File : BM020239.D
Acq On : 10 May 2019 13:27
Operator : JU/SJ
Sample : PB119565BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB119565BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM043019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

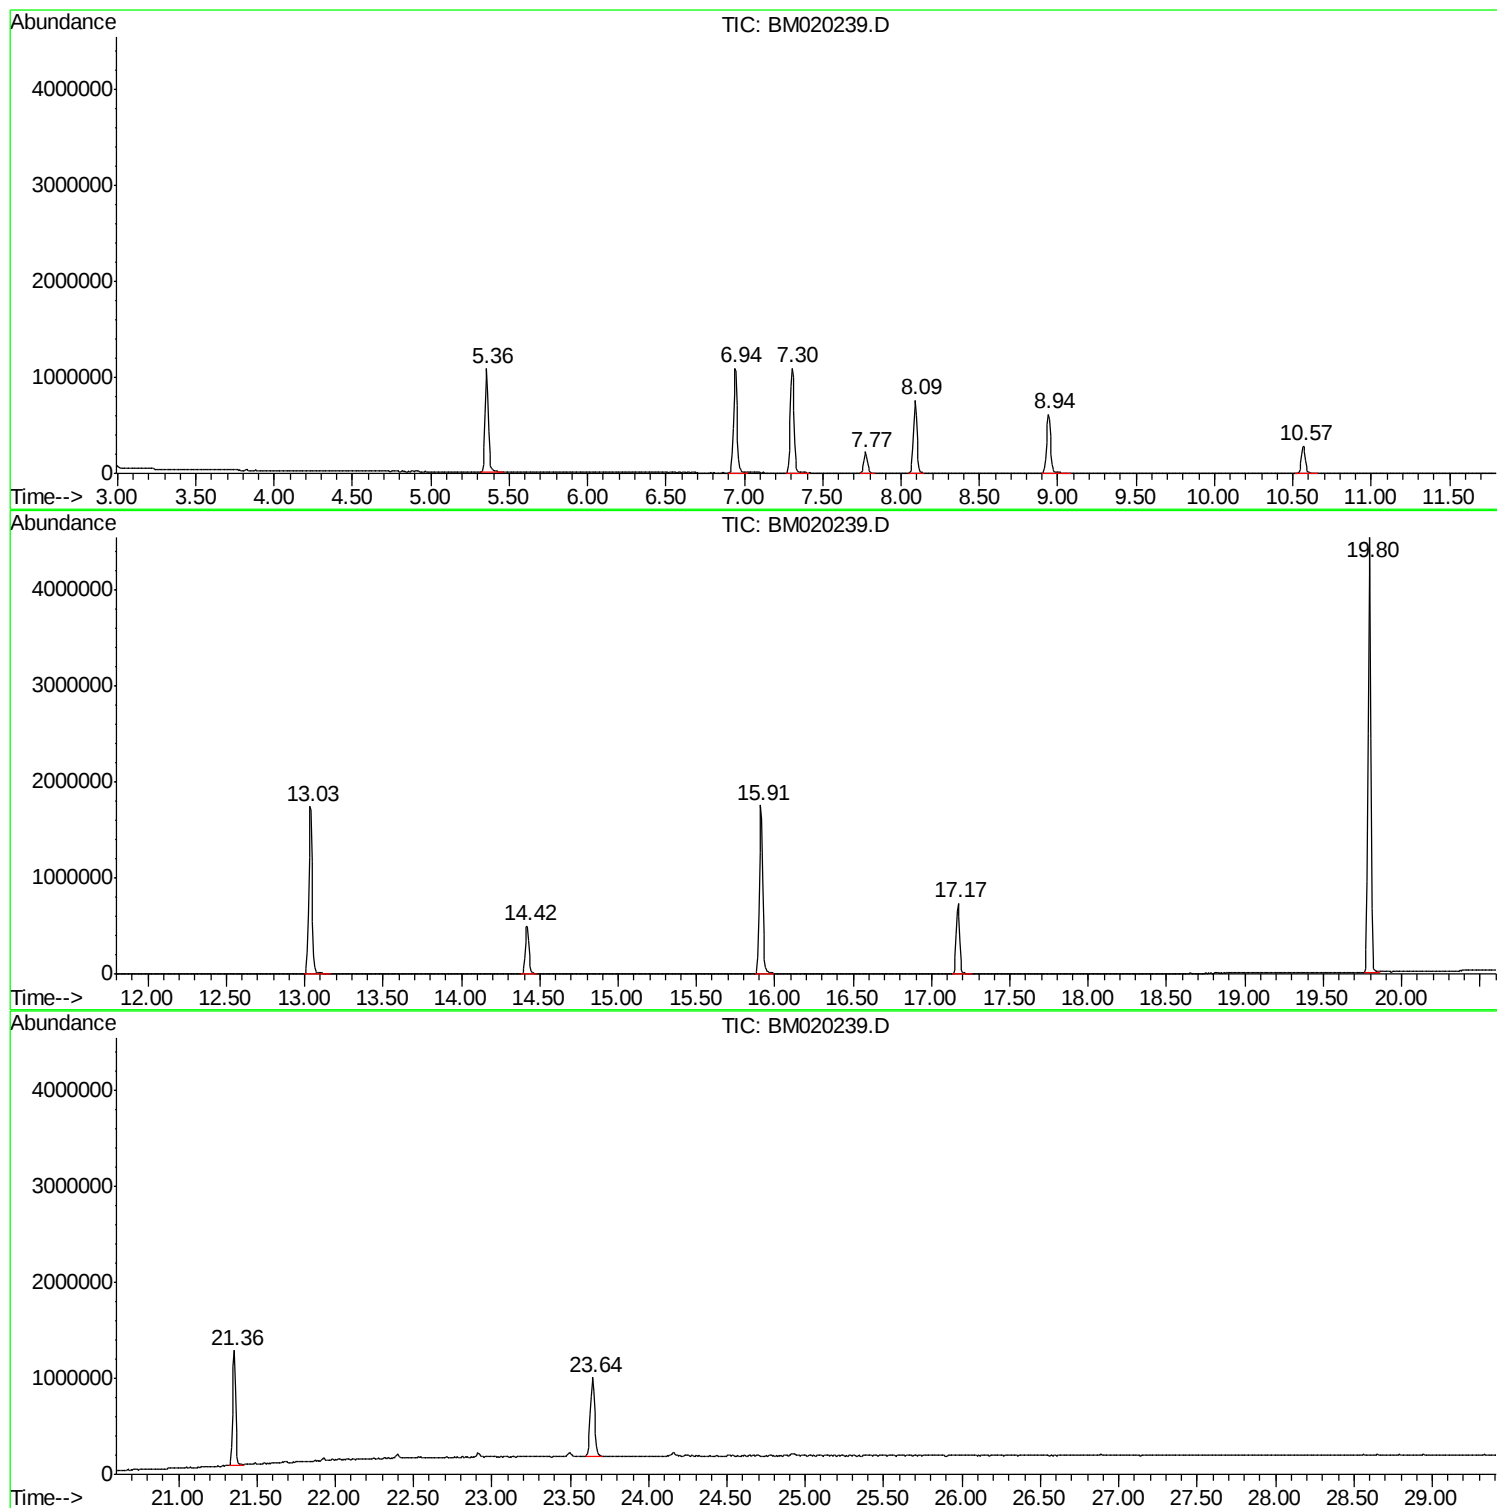

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM051019\
Data File : BM020239.D
Acq On : 10 May 2019 13:27
Operator : JU/SJ
Sample : PB119565BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB119565BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM043019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.30 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.30	102.24 ng	1783400	1,4-Dichlorobenzene-d4	7.77

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	27
2		1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	22
3		3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	16
4		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	12
5		2H-Cyclopenta[d]pyridazine, 2-me...	132	C8H8N2	022291-85-6	12

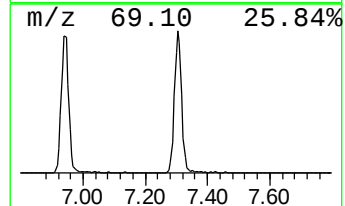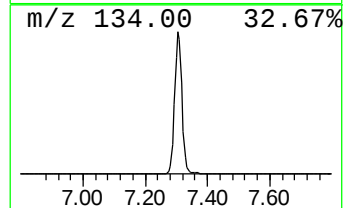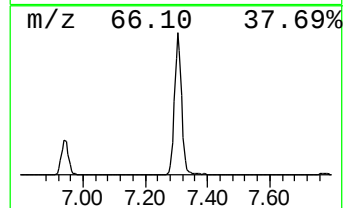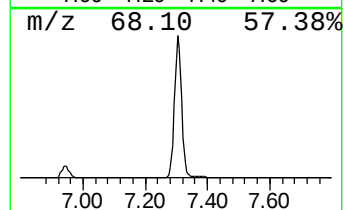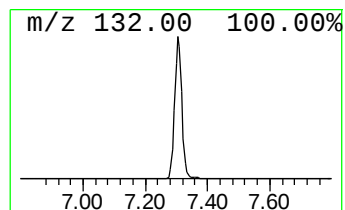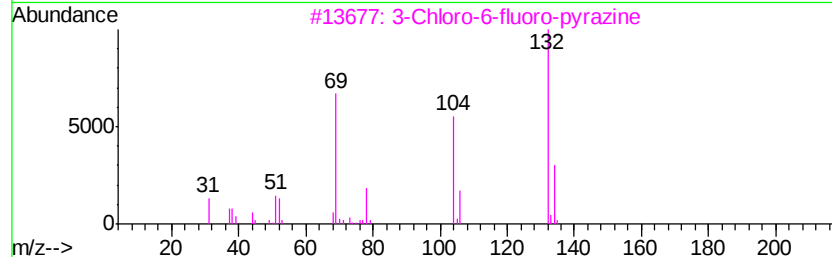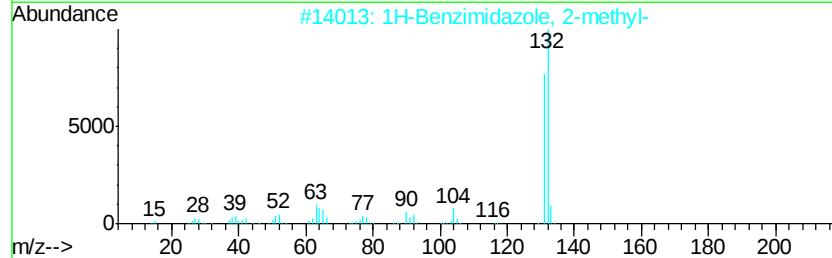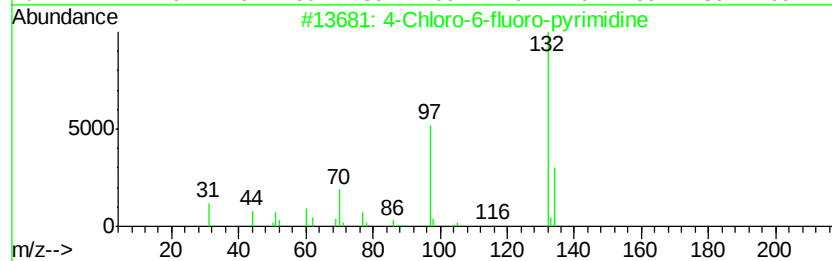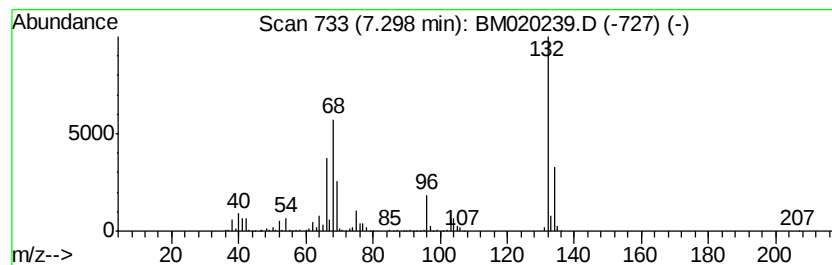

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM051019\
Data File : BM020239.D
Acq On : 10 May 2019 13:27
Operator : JU/SJ
Sample : PB119565BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB119565BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM043019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.30	7.30	102.2	ng	1783400	1	7.77	348850	20.0