

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM051019\
 Data File : BM020250.D
 Acq On : 10 May 2019 21:54
 Operator : JU/SJ
 Sample : PB119597BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB119597BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM043019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.357	396	403	418	rBV	1370700	2017224	30.35%	7.074%
2	6.939	665	672	684	rBV	1334927	2194850	33.02%	7.697%
3	7.304	727	734	748	rBV	1369001	2208683	33.23%	7.746%
4	7.775	806	814	824	rBV	253663	414660	6.24%	1.454%
5	8.092	860	868	881	rBV	930460	1568889	23.60%	5.502%
6	8.939	1004	1012	1022	rBV	760399	1302803	19.60%	4.569%
7	10.563	1281	1288	1299	rBV	309205	547085	8.23%	1.919%
8	13.033	1701	1708	1725	rBV	2284522	3317446	49.91%	11.634%
9	14.415	1937	1943	1951	rBV2	546096	843625	12.69%	2.959%
10	15.910	2191	2197	2217	rBV	2087180	3073434	46.23%	10.778%
11	17.168	2403	2411	2425	rBV2	787172	1203322	18.10%	4.220%
12	19.792	2851	2857	2871	rBV	5562864	6647425	100.00%	23.312%
13	21.350	3117	3122	3133	rBV	1270127	1606534	24.17%	5.634%
14	23.638	3504	3511	3521	rVB2	787960	1568698	23.60%	5.501%


Sum of corrected areas: 28514678

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM051019\
Data File : BM020250.D
Acq On : 10 May 2019 21:54
Operator : JU/SJ
Sample : PB119597BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB119597BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM043019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

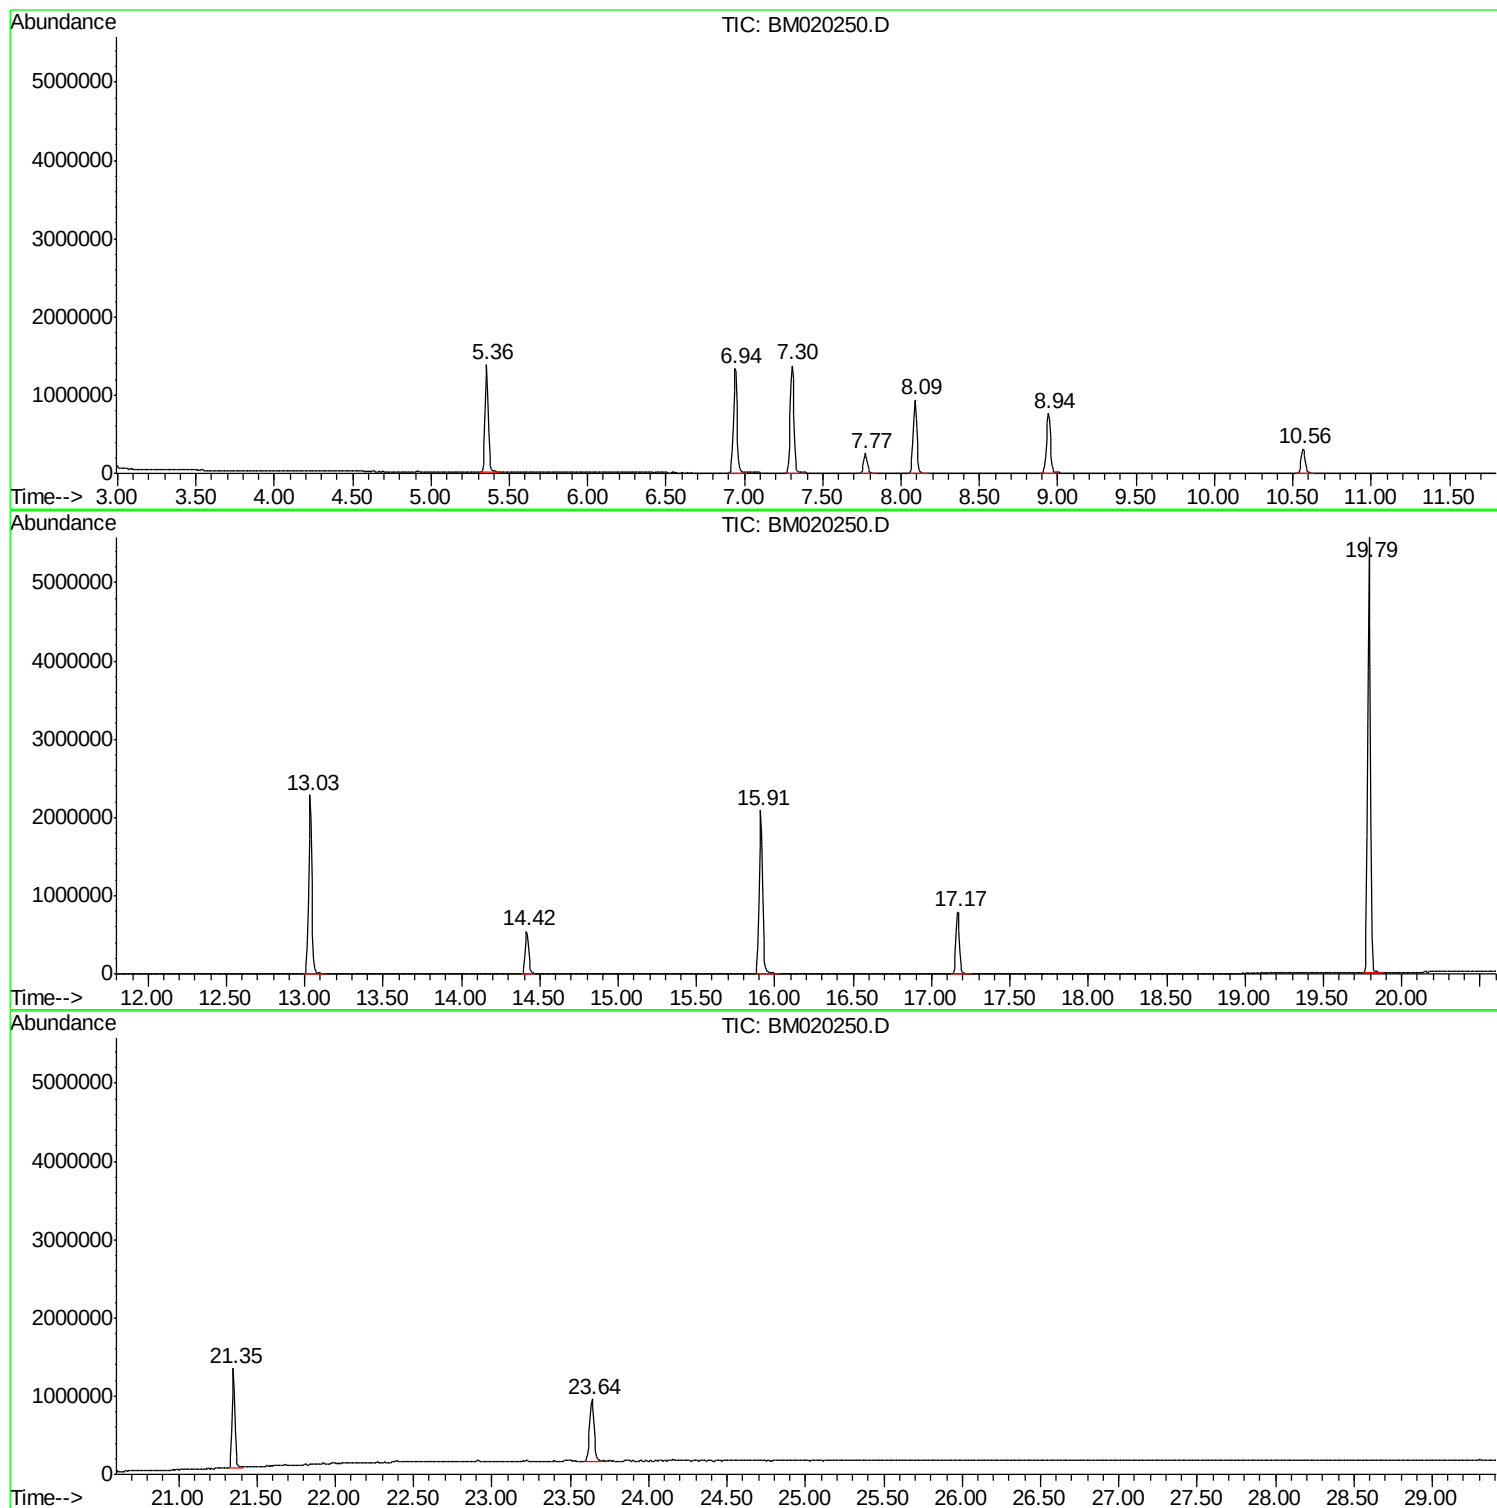

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM051019\
Data File : BM020250.D
Acq On : 10 May 2019 21:54
Operator : JU/SJ
Sample : PB119597BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB119597BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM043019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.30 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.30	106.53 ng	2208680	1,4-Dichlorobenzene-d4	7.77

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	27
2		1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	22
3		3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	16
4		1,3-Cyclopentanedione, 2-chloro-	132	C5H5ClO2	014203-19-1	13
5		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	12

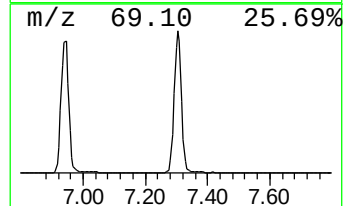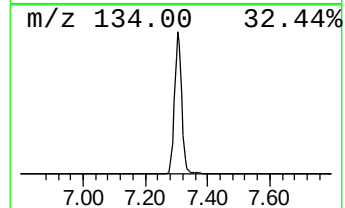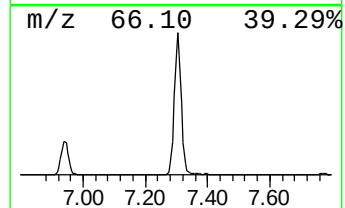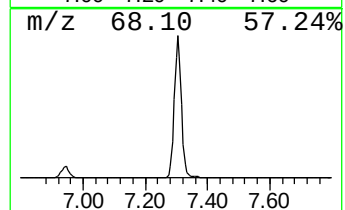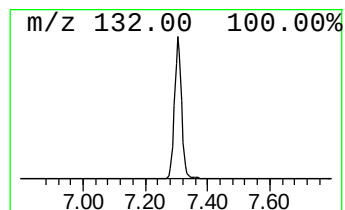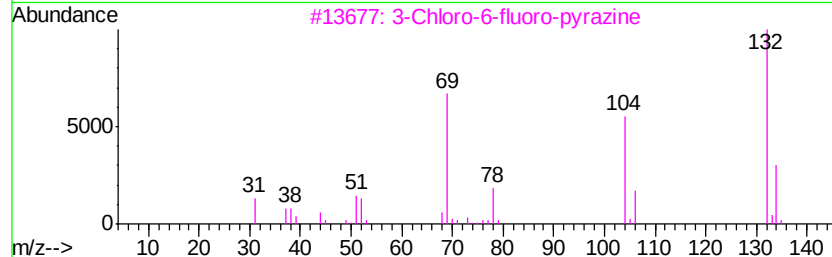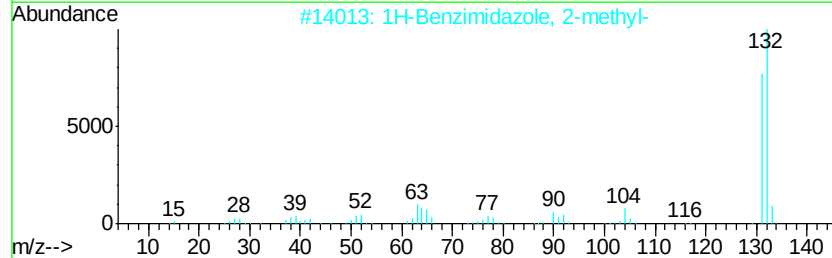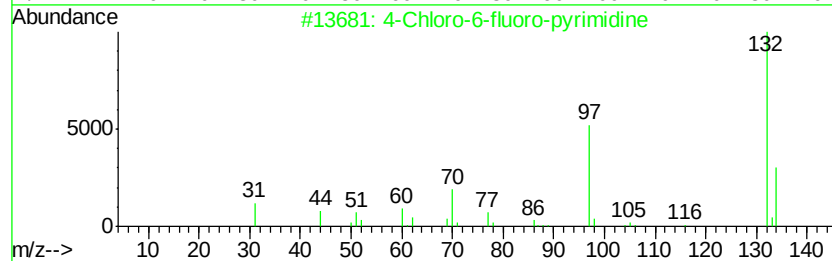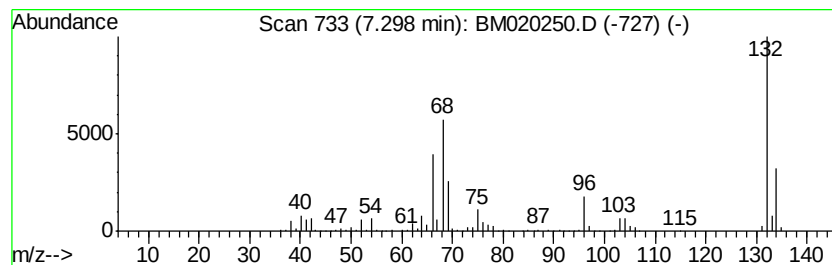

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM051019\
Data File : BM020250.D
Acq On : 10 May 2019 21:54
Operator : JU/SJ
Sample : PB119597BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB119597BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM043019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---			
					#	RT	Resp	Conc
unknown7.30	7.30	106.5	ng	2208680	1	7.77	414660	20.0