


Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM051019\
 Data File : BM020234.D
 Acq On : 10 May 2019 09:17
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM043019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 01 03:58:37 2019

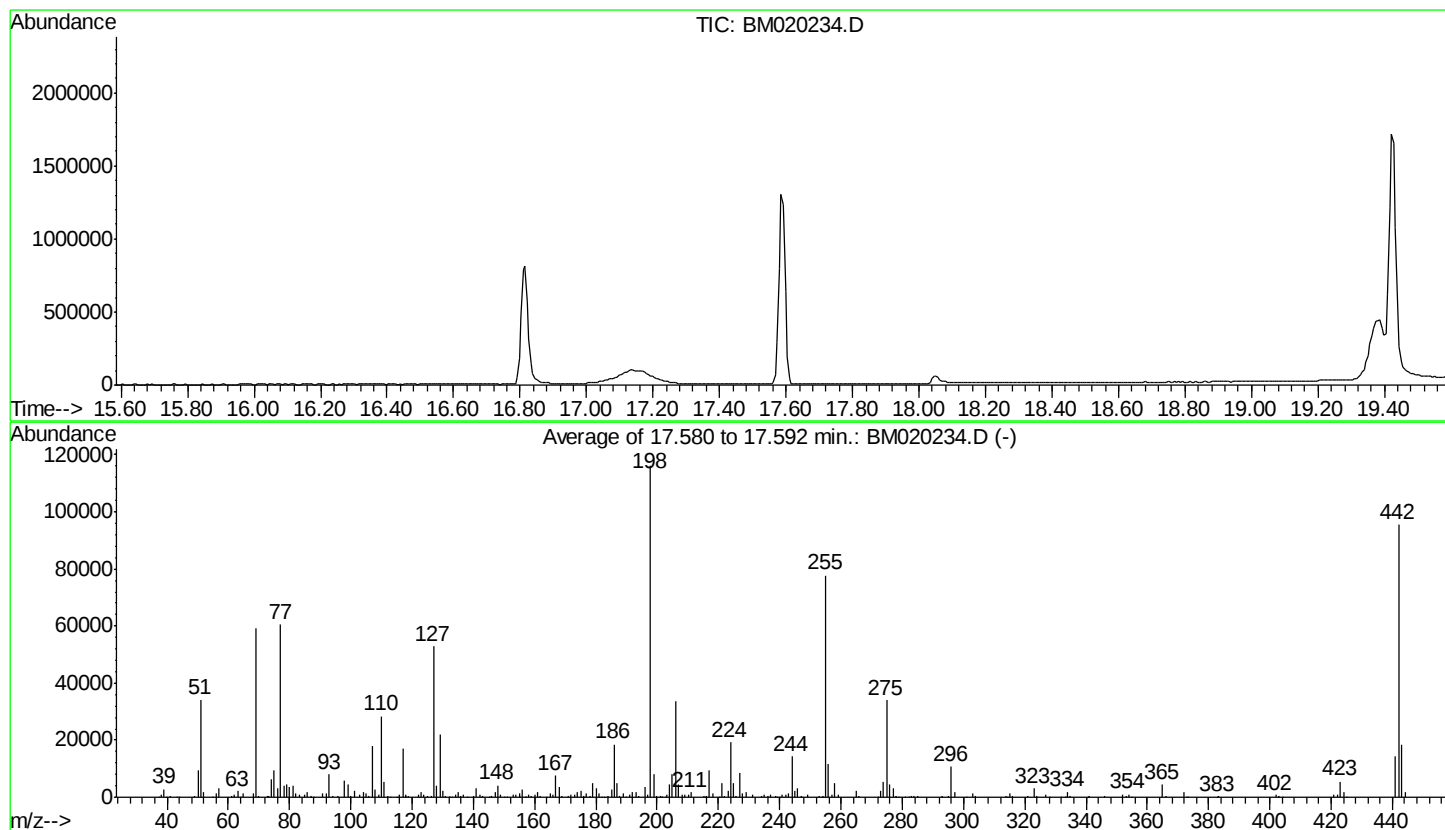

AutoFind: Scans 2481, 2482, 2483; Background Corrected with Scan 2475

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.4	34109	PASS
68	69	0.00	2	2.0	1177	PASS
69	198	0.00	100	51.0	59304	PASS
70	69	0.00	2	0.9	530	PASS
127	198	10	80	45.4	52754	PASS
197	198	0.00	2	0.8	875	PASS
198	198	100	100	100.0	116189	PASS
199	198	5	9	6.9	7965	PASS
275	198	10	60	29.2	33898	PASS
365	198	1	100	3.8	4469	PASS
441	198	0.01	100	12.5	14561	PASS
442	198	50	100	82.1	95352	PASS
443	442	15	24	19.3	18368	PASS