

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM051119\
 Data File : BM020280.D
 Acq On : 11 May 2019 19:44
 Operator : JU/SJ
 Sample : K2763-05
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 P021-SS005-0612-01

Quant Time: May 12 03:12:27 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM043019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 01 03:58:37 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.77	152	49082	20.00	ng	-0.02
21) Naphthalene-d8	10.56	136	165328	20.00	ng	-0.03
39) Acenaphthene-d10	14.41	164	100735	20.00	ng	-0.02
64) Phenanthrene-d10	17.16	188	245441	20.00	ng	-0.02
76) Chrysene-d12	21.35	240	270628	20.00	ng	-0.02
87) Perylene-d12	23.64	264	320526	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.35	112	380641	126.77	ng	-0.02
7) Phenol-d6	6.93	99	512596	124.96	ng	-0.02
23) Nitrobenzene-d5	8.93	82	349760	83.52	ng	-0.02
42) 2,4,6-Tribromophenol	15.91	330	199828	127.80	ng	-0.01
45) 2-Fluorobiphenyl	13.03	172	514659	62.86	ng	-0.03
79) Terphenyl-d14	19.79	244	995353	64.15	ng	-0.02
Target Compounds						
50) Dimethylphthalate	13.87	163	92459	10.799	ng	Qvalue 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM051119\
Data File : BM020280.D
Acq On : 11 May 2019 19:44
Operator : JU/SJ
Sample : K2763-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
P021-SS005-0612-01

Quant Time: May 12 03:12:27 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM043019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 01 03:58:37 2019
Response via : Initial Calibration

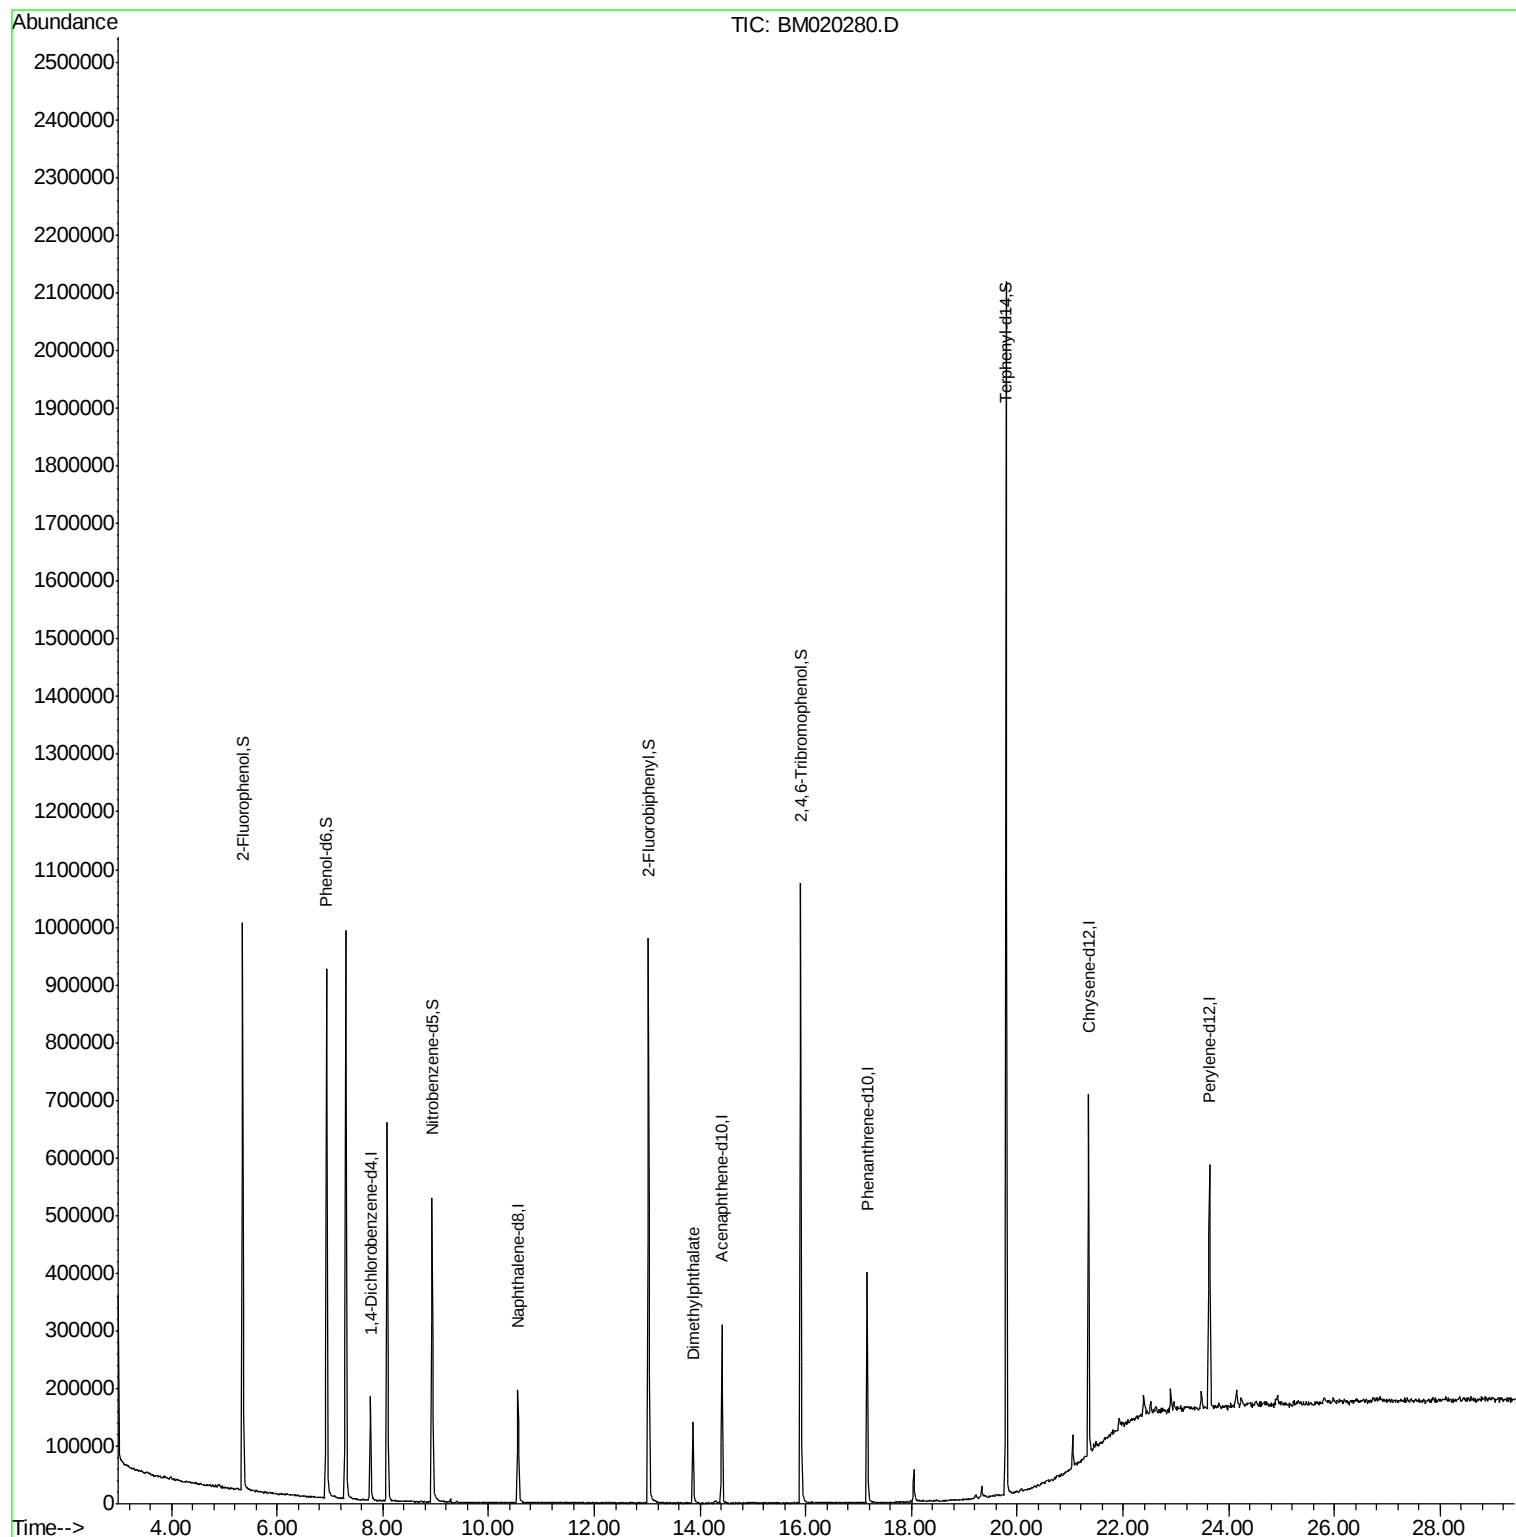

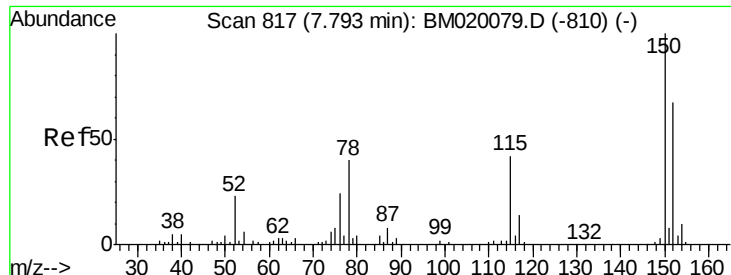


#1



1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.77 min Scan# 813
Delta R.T. -0.02 min
Lab File: BM020280.D
Acq: 11 May 2019 19:44

Instrument :
BNA_M
ClientSampleId :
P021-SS005-0612-01

Tot Ion:152 Resp: 49082
Ion Ratio Lower Upper
152 100
150 150.7 119.8 179.8
115 61.5 50.8 76.2

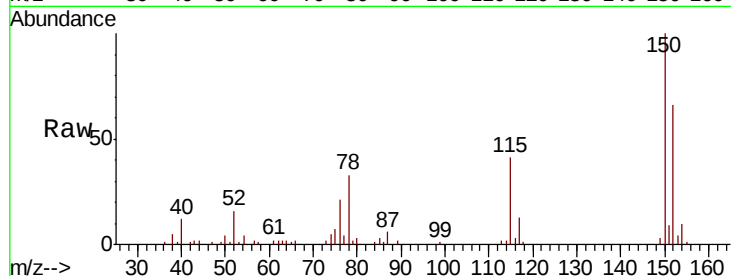


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

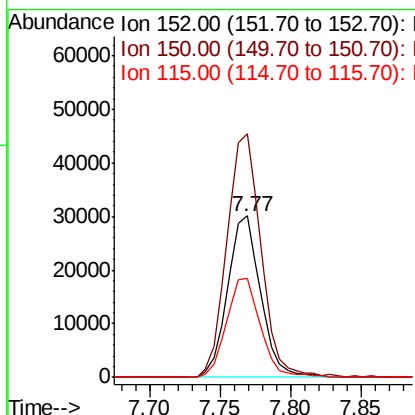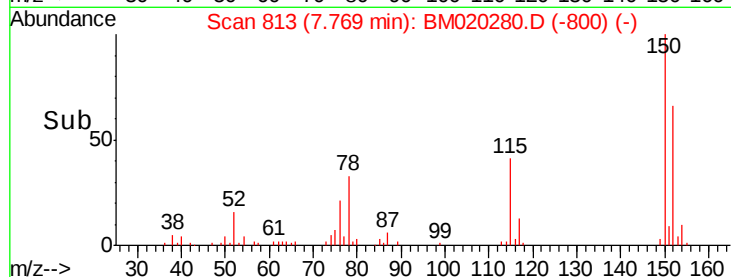



#5


2-Fluorophenol
Concen: 126.766 ng
RT: 5.35 min Scan# 402
Delta R.T. -0.02 min
Lab File: BM020280.D
Acq: 11 May 2019 19:44

Tgt Ion:112 Resp: 380641
Ion Ratio Lower Upper
112 100
64 65.6 53.8 80.6
63 35.4 32.3 48.5

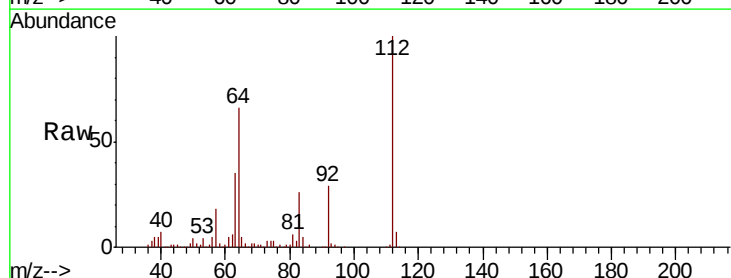

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BM0
Ion 63.00 (62.70 to 63.70): BM0

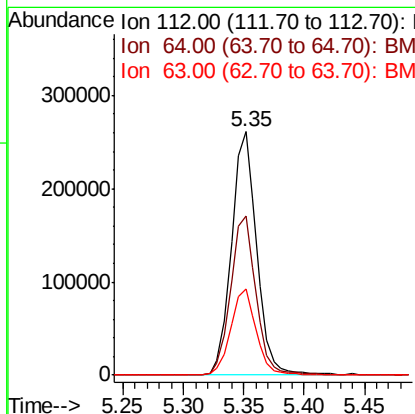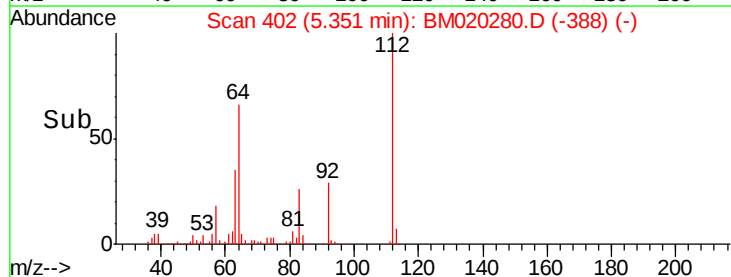

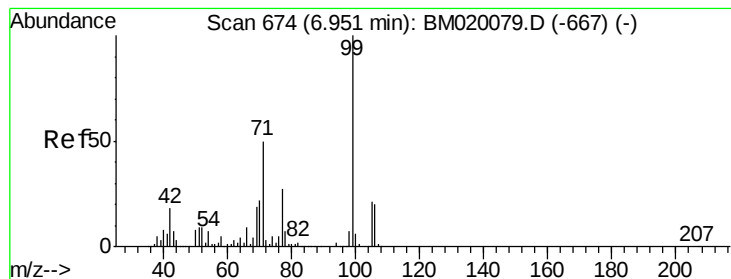

#7

Phenol-d6

Concen: 124.959 ng

RT: 6.93 min Scan# 671

Delta R.T. -0.02 min

Lab File: BM020280.D

Acq: 11 May 2019 19:44

Instrument :

BNA_M

ClientSampleId :

P021-SS005-0612-01


Tot Ion: 99 Resp: 512596

Ion Ratio Lower Upper

99 100

42 14.7 14.2 21.2




71 44.9 40.3 60.5

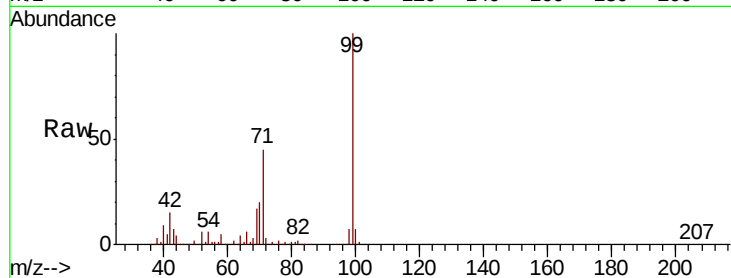

Abundance Ion 99.00 (98.70 to 99.70): BM020079.D (-667) (-)

Ion 42.00 (41.70 to 42.70): BM020079.D (-667) (-)

Ion 71.00 (70.70 to 71.70): BM020079.D (-667) (-)

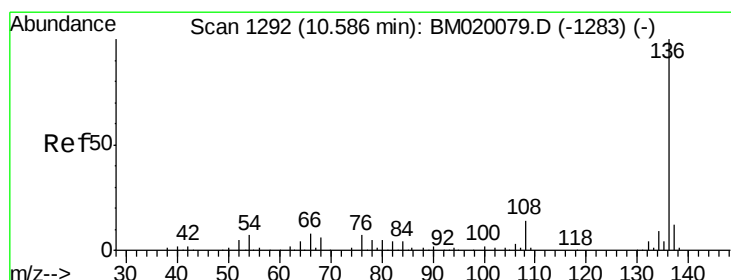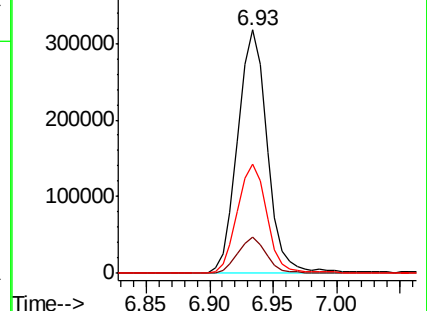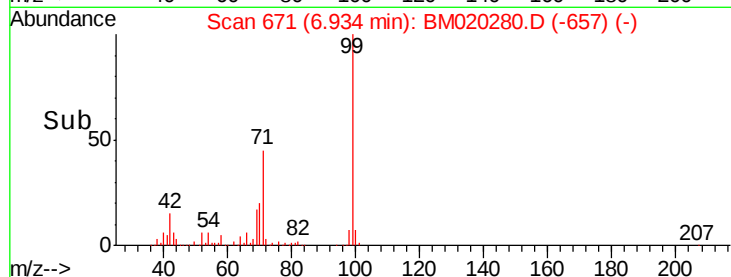

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.56 min Scan# 1287

Delta R.T. -0.03 min

Lab File: BM020280.D

Acq: 11 May 2019 19:44

Tgt Ion: 136 Resp: 165328


Ion Ratio Lower Upper

136 100

137 10.6 9.6 14.4

54 6.5 5.5 8.3

68 6.9 4.6 6.8#


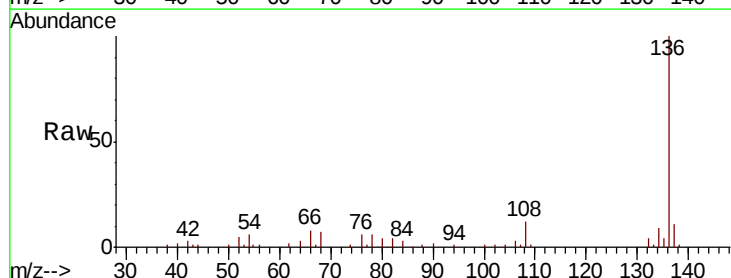


Abundance Ion 136.00 (135.70 to 136.70): BM020079.D (-1283) (-)

Ion 137.00 (136.70 to 137.70): BM020079.D (-1283) (-)

Ion 54.00 (53.70 to 54.70): BM020079.D (-1283) (-)

Ion 68.00 (67.70 to 68.70): BM020079.D (-1283) (-)



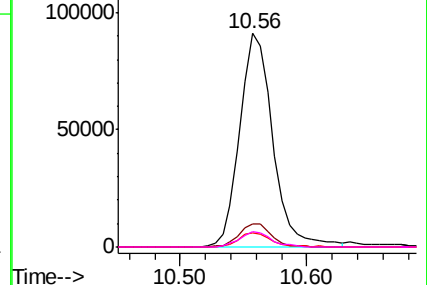
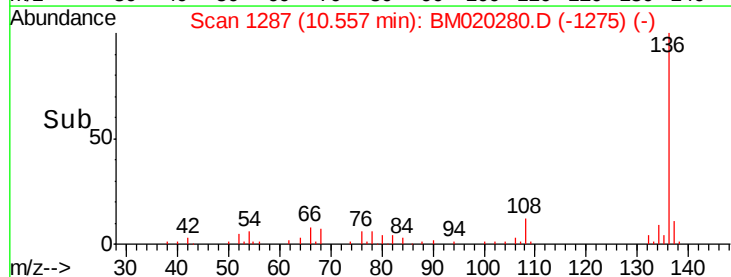




#23
Nitrobenzene-d5
Concen: 83.522 ng
RT: 8.93 min Scan# 1011
Delta R.T. -0.02 min
Lab File: BM020280.D
Acq: 11 May 2019 19:44




Instrument :
BNA_M
ClientSampleId :
P021-SS005-0612-01


Tot Ion	Ratio	Lower	Upper
82	100		
128	33.4	25.2	37.8
54	37.5	31.9	47.9

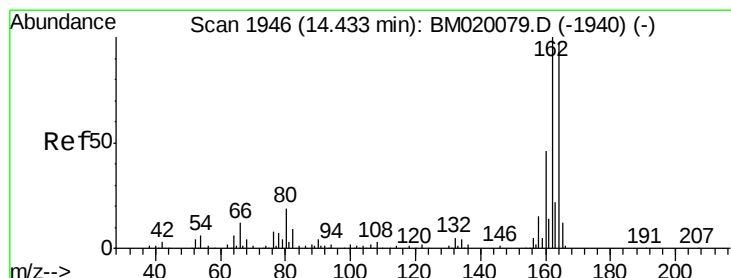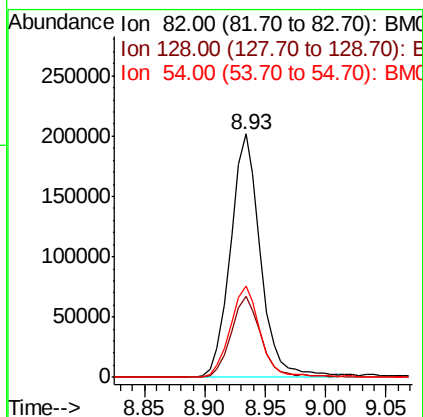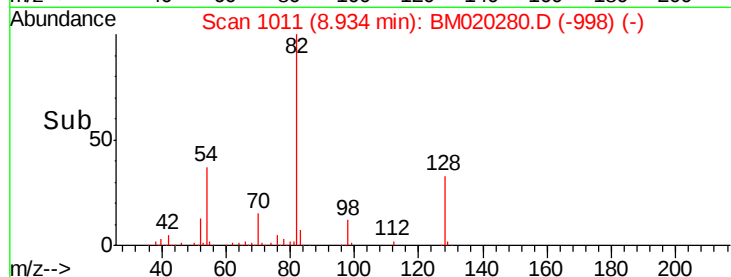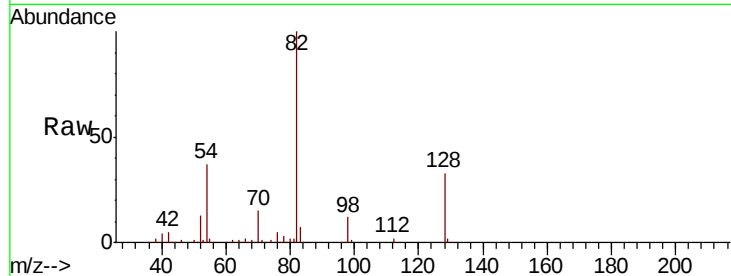

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.41 min Scan# 1942
Delta R.T. -0.02 min
Lab File: BM020280.D
Acq: 11 May 2019 19:44

Tgt Ion	Ratio	Lower	Upper
164	100		
162	101.4	82.2	123.2
160	45.3	37.6	56.4

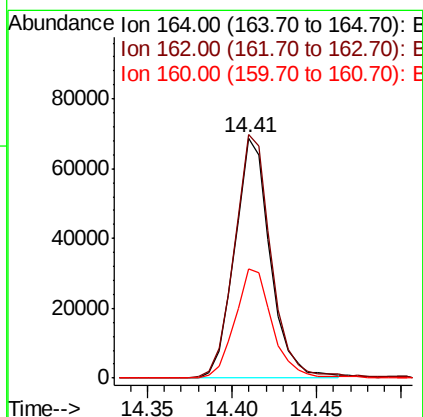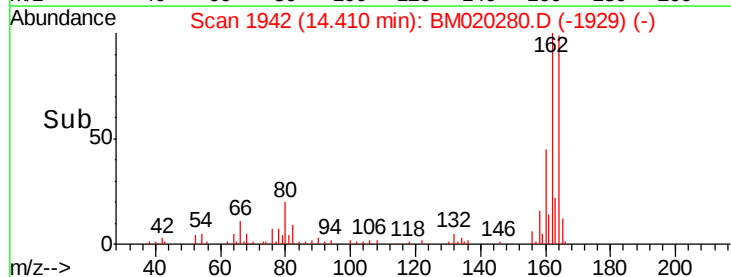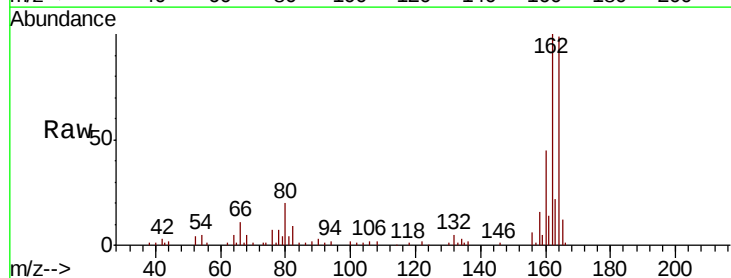


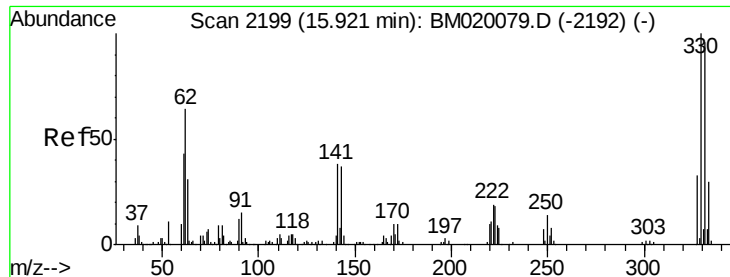

#42
 2,4,6-Tribromophenol
 Concen: 127.800 ng
 RT: 15.91 min Scan# 2197
 Delta R.T. -0.01 min
 Lab File: BM020280.D
 Acq: 11 May 2019 19:44

Instrument :
 BNA_M
 ClientSampleId :
 P021-SS005-0612-01

Tot Ion	Ratio	Lower	Upper
330	100		
332	97.4	76.8	115.2
141	33.8	29.2	43.8


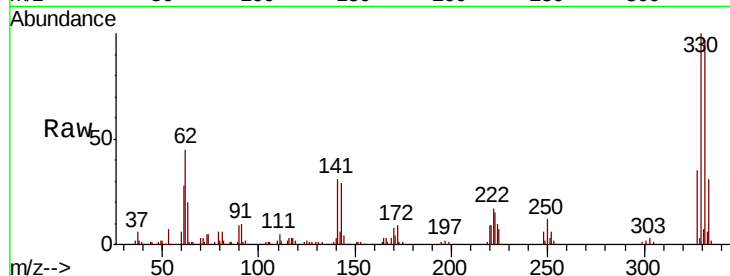


Abundance

Ion 329.80 (329.50 to 330.50): E


Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

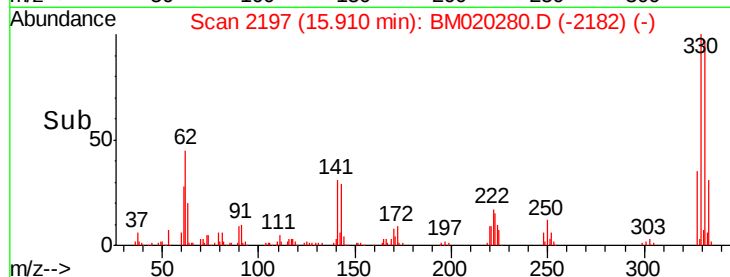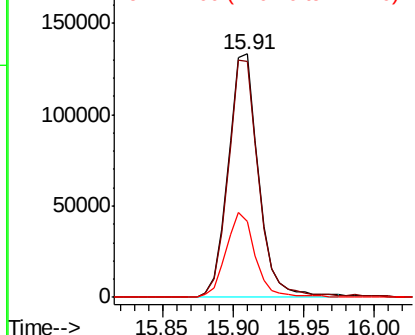

#45
 2-Fluorobiphenyl
 Concen: 62.860 ng
 RT: 13.03 min Scan# 1707
 Delta R.T. -0.03 min
 Lab File: BM020280.D
 Acq: 11 May 2019 19:44

Tgt Ion	Ratio	Lower	Upper
172	100		
171	35.7	27.3	40.9
170	23.3	17.9	26.9


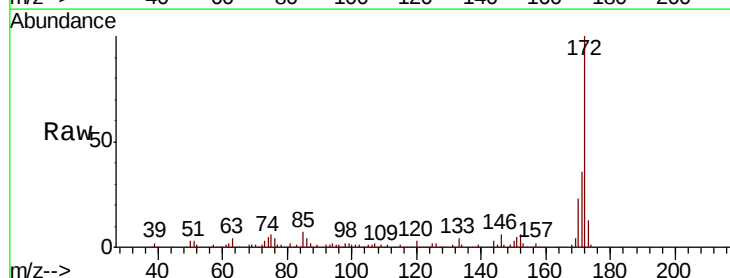


Abundance

Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

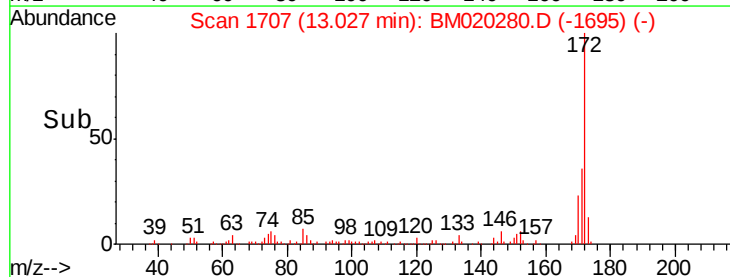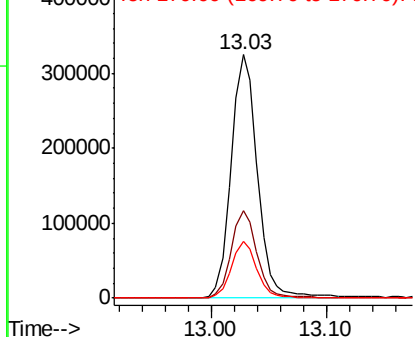



#50

Dimethylphthalate

Concen: 10.799 ng

RT: 13.87 min Scan# 1850

Delta R.T. -0.03 min

Lab File: BM020280.D

Acq: 11 May 2019 19:44

Instrument :

BNA_M

ClientSampleId :

P021-SS005-0612-01


Tot Ion:163 Resp: 92459

Ion Ratio Lower Upper




163 100

194 4.4 3.6 5.4

164 10.6 8.4 12.6

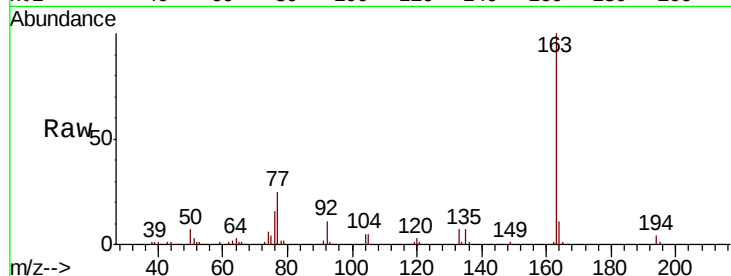

Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

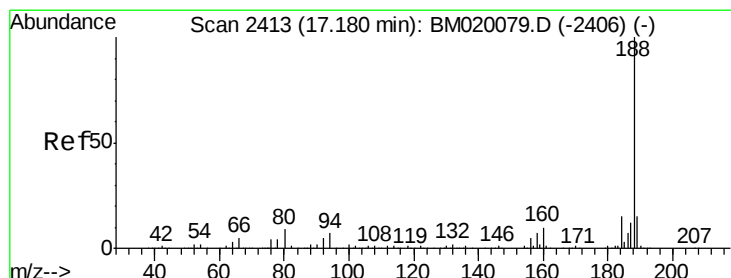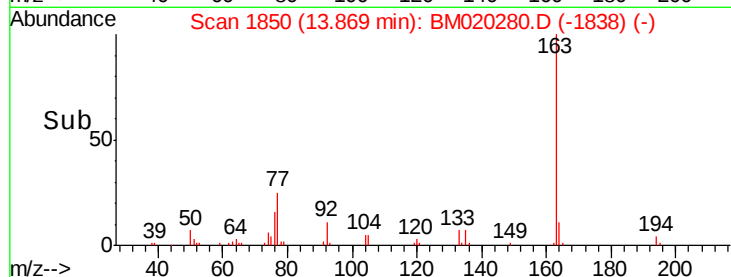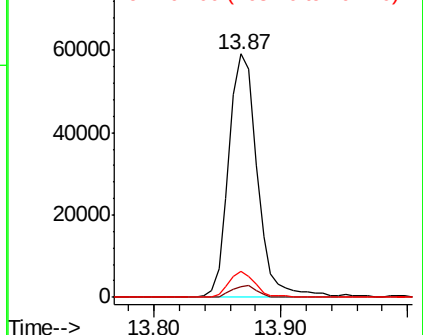

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.16 min Scan# 2410

Delta R.T. -0.02 min

Lab File: BM020280.D

Acq: 11 May 2019 19:44


Tgt Ion:188 Resp: 245441

Ion Ratio Lower Upper



188 100

94 7.8 5.8 8.6

80 10.0 7.4 11.2

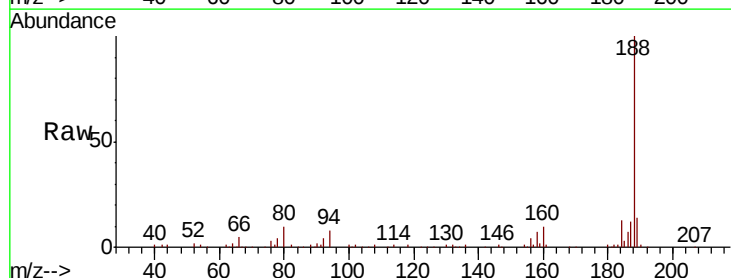

Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BM0
Ion 80.00 (79.70 to 80.70): BM0


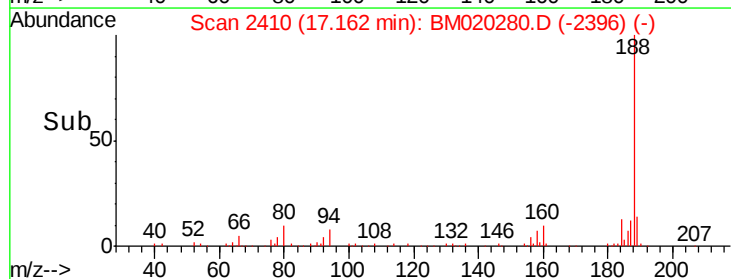
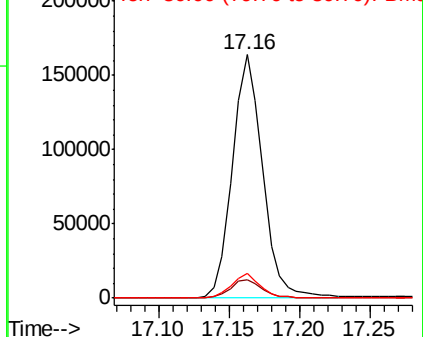




#76
 Chrvsene-d12
 Concen: 20.000 ng
 RT: 21.35 min Scan# 3122
 Delta R.T. -0.02 min
 Lab File: BM020280.D
 Acq: 11 May 2019 19:44




Instrument :
 BNA_M
 ClientSampleId :
 P021-SS005-0612-01


Tot Ion	Ratio	Lower	Upper
240	100		
120	7.9	5.6	8.4
236	25.9	20.9	31.3

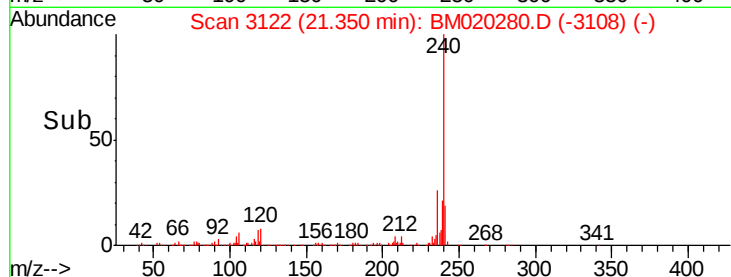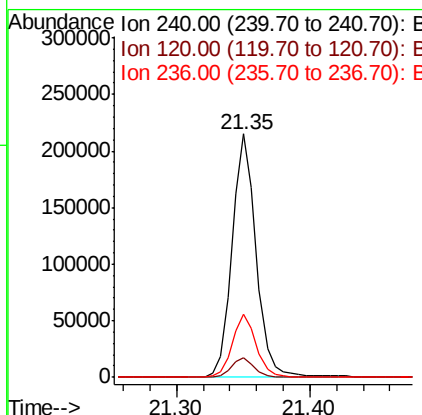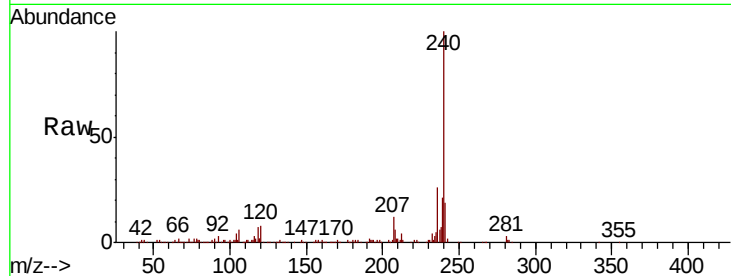

#79
 Terphenyl-d14
 Concen: 64.151 ng
 RT: 19.79 min Scan# 2857
 Delta R.T. -0.02 min
 Lab File: BM020280.D
 Acq: 11 May 2019 19:44

Tgt Ion	Ratio	Lower	Upper
244	100		
212	6.4	5.7	8.5
122	7.0	6.2	9.2

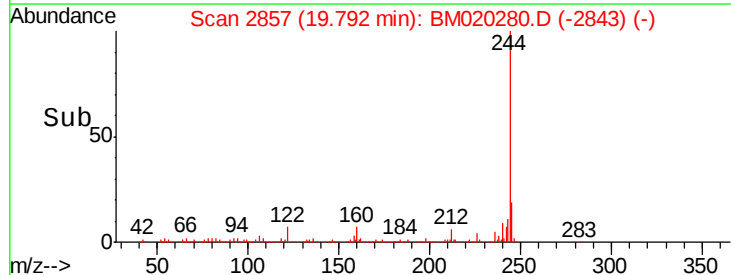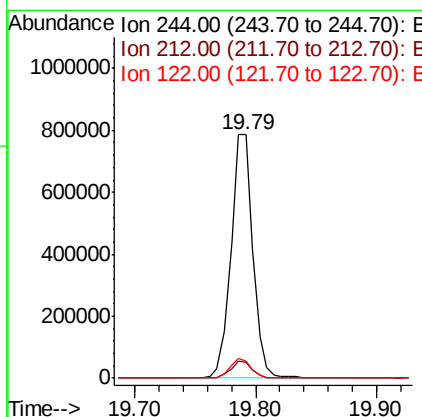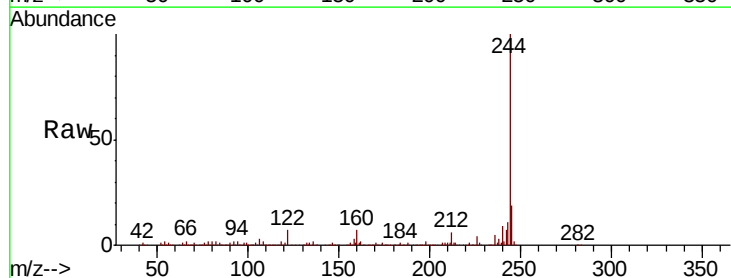


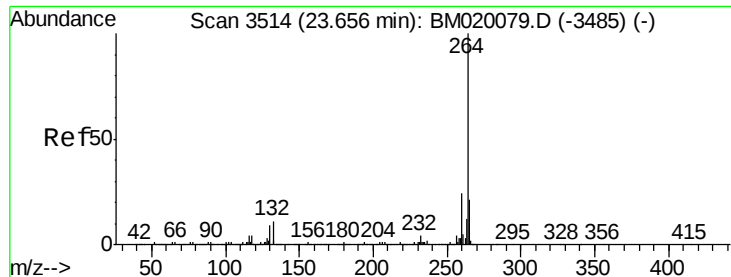

#87
 Pervlene-d12
 Concen: 20.000 ng
 RT: 23.64 min Scan# 3511
 Delta R.T. -0.02 min
 Lab File: BM020280.D
 Acq: 11 May 2019 19:44

Instrument :
 BNA_M
 ClientSampleId :
 P021-SS005-0612-01

Tot Ion:	264	Resp:	320526
Ion	Ratio	Lower	Upper
264	100		
260	22.3	19.2	28.8
265	22.2	16.9	25.3

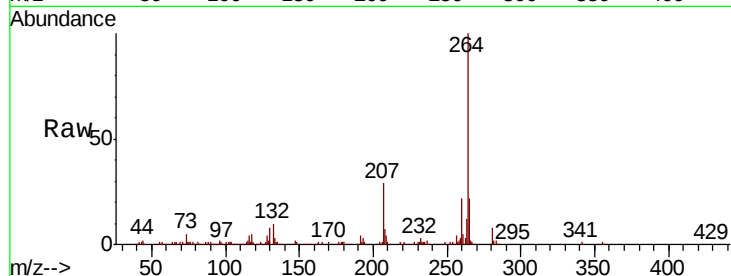

Abundance

Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

