


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM051119\
Data File : BM020286.D
Acq On : 12 May 2019 00:33
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM043019.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed May 01 03:58:37 2019

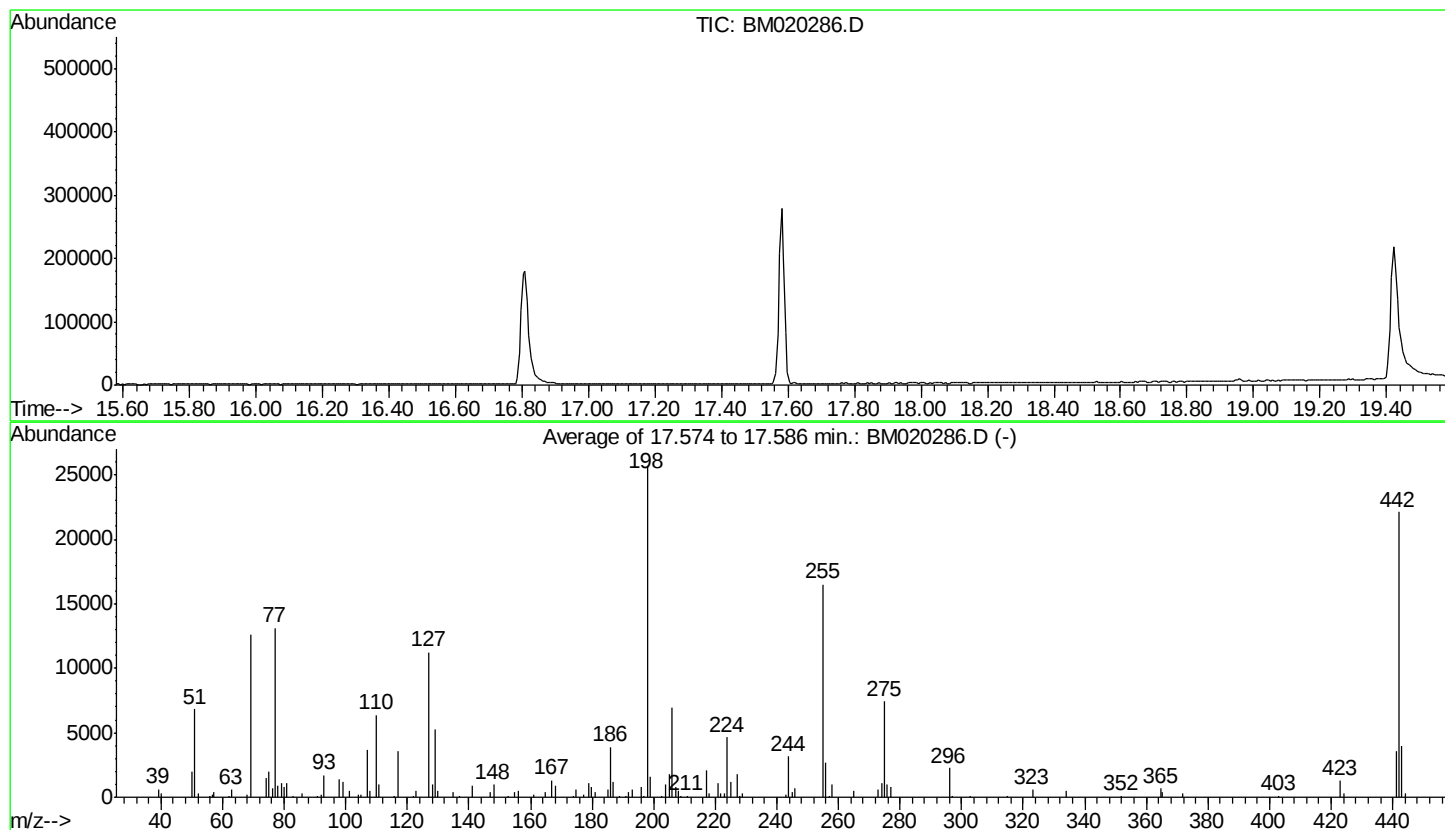

AutoFind: Scans 2480, 2481, 2482; Background Corrected with Scan 2474

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.5	6825	PASS
68	69	0.00	2	1.8	232	PASS
69	198	0.00	100	48.9	12583	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	43.8	11265	PASS
197	198	0.00	2	0.4	109	PASS
198	198	100	100	100.0	25709	PASS
199	198	5	9	6.1	1564	PASS
275	198	10	60	28.8	7399	PASS
365	198	1	100	2.6	674	PASS
441	198	0.01	100	13.7	3533	PASS
442	198	50	100	86.0	22120	PASS
443	442	15	24	18.2	4016	PASS