
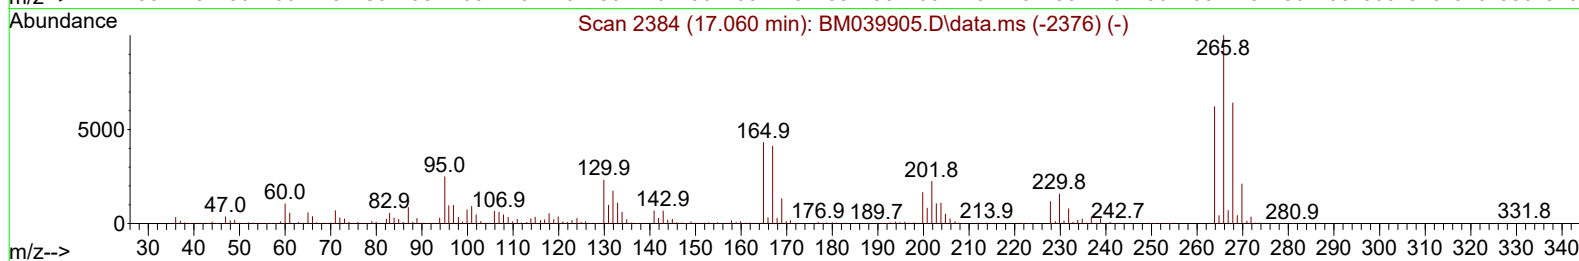
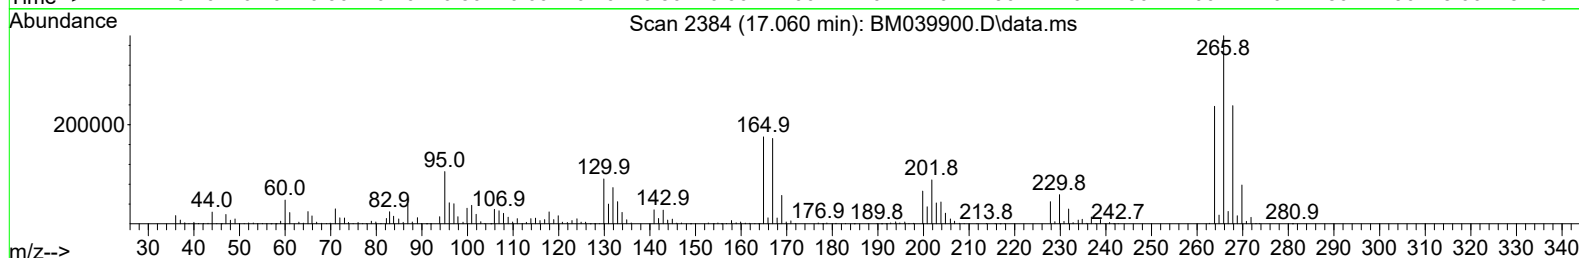


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051123\
Data File : BM039900.D
Acq On : 11 May 2023 15:57
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 12 07:05:48 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM051123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 12 02:40:29 2023
Response via : Initial Calibration

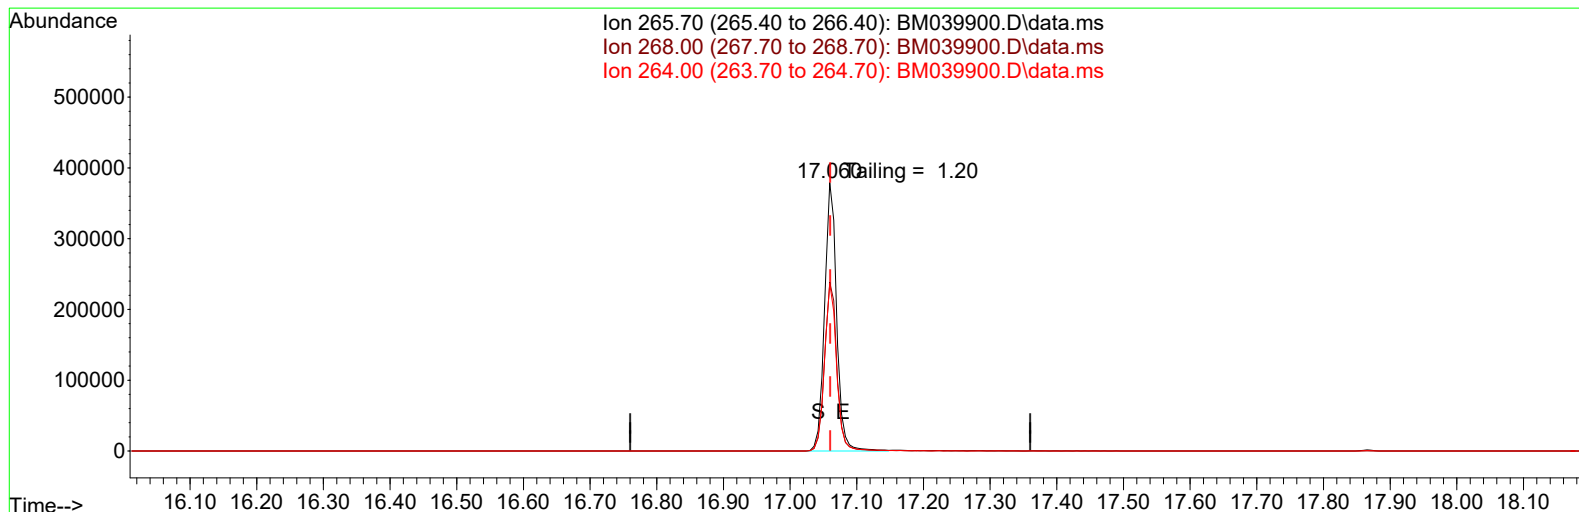

TIC: BM039900.D\data.ms

(70) Pentachlorophenol (C)




17.060min (-0.000) 0.00 ng

response 480482

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.10	62.85
264.00	62.20	62.51
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051123\
Data File : BM039900.D
Acq On : 11 May 2023 15:57
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 12 07:05:48 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM051123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 12 02:40:29 2023
Response via : Initial Calibration

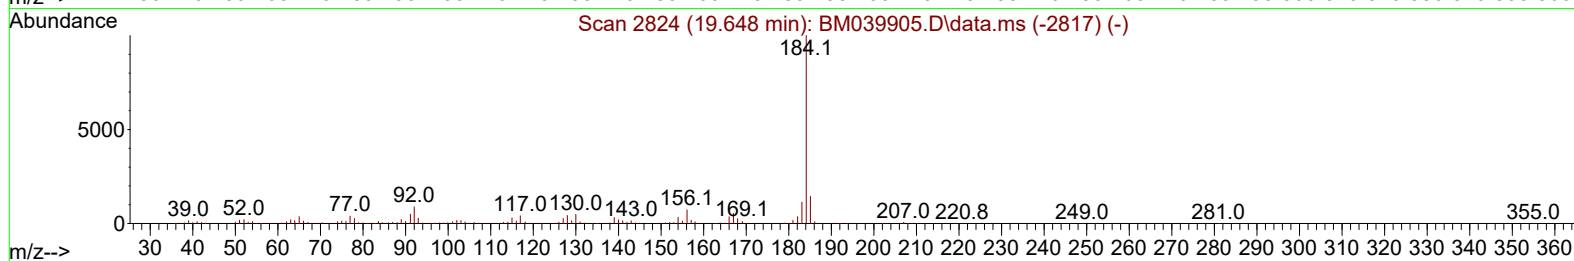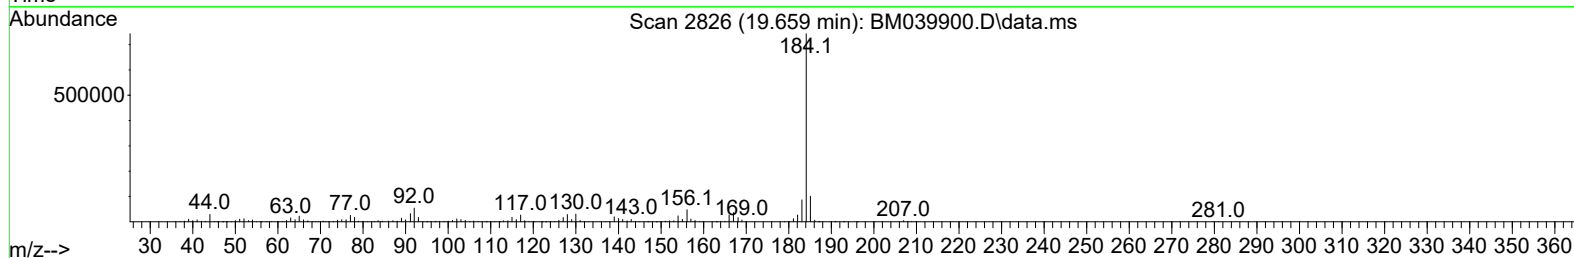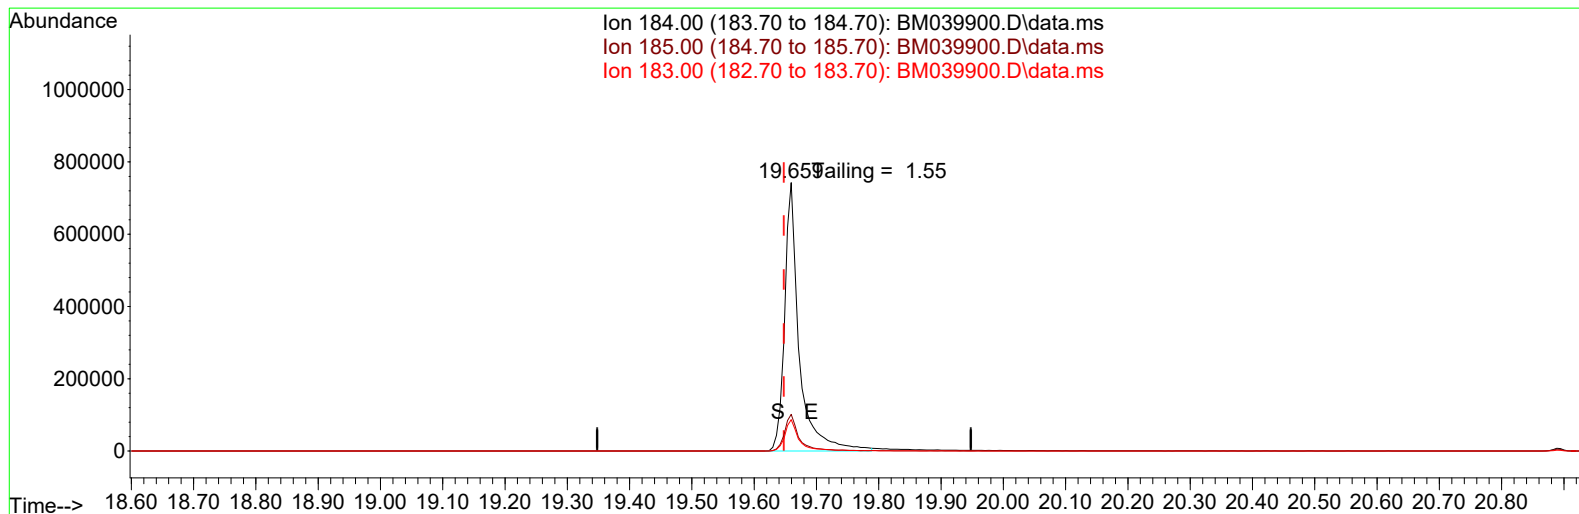

TIC: BM039900.D\data.ms

(77) Benzidine

19.659min (+ 0.011) 0.00 ng

response 1240342

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.67
183.00	11.30	11.70
0.00	0.00	0.00