


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM051219\
 Data File : BM020291.D
 Acq On : 12 May 2019 10:09
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM043019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 01 03:58:37 2019

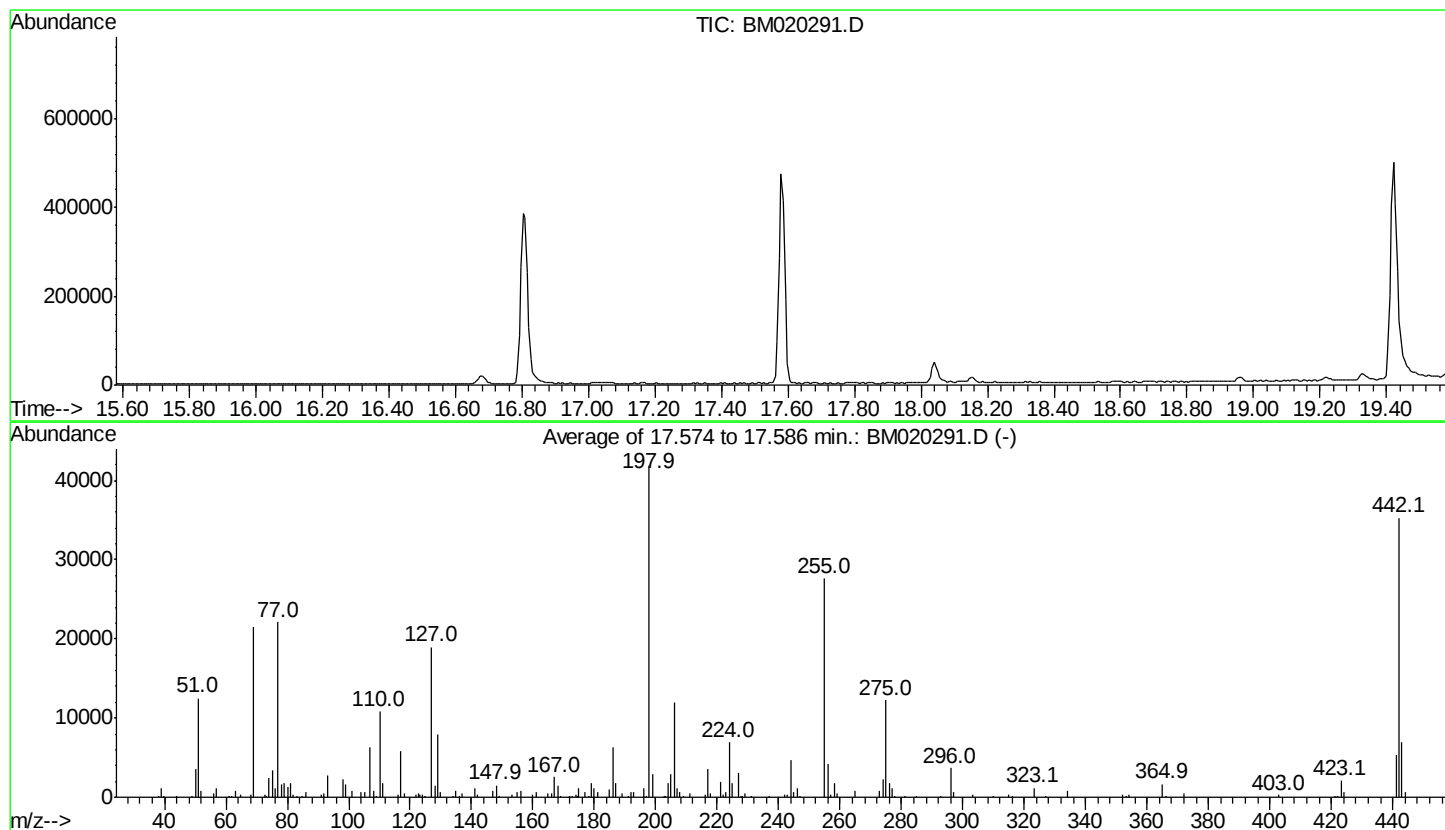

AutoFind: Scans 2480, 2481, 2482; Background Corrected with Scan 2475

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.9	12532	PASS
68	69	0.00	2	1.3	288	PASS
69	198	0.00	100	51.3	21490	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	45.2	18920	PASS
197	198	0.00	2	0.3	119	PASS
198	198	100	100	100.0	41877	PASS
199	198	5	9	7.1	2956	PASS
275	198	10	60	29.3	12284	PASS
365	198	1	100	3.9	1647	PASS
441	198	0.01	100	12.7	5327	PASS
442	198	50	100	84.3	35298	PASS
443	442	15	24	19.6	6913	PASS