


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM051319\
 Data File : BM020310.D
 Acq On : 13 May 2019 11:28
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM043019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 01 03:58:37 2019

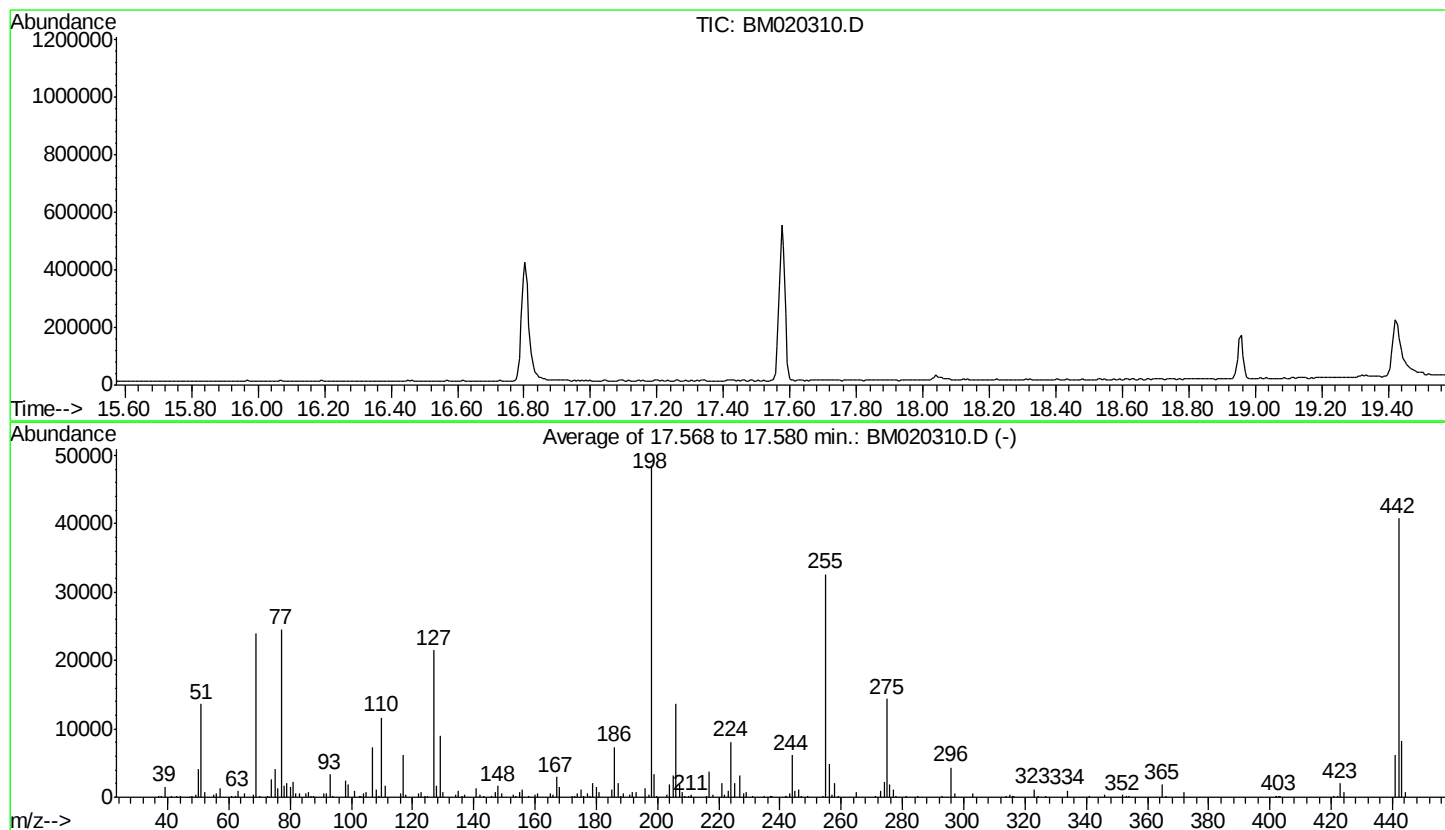

AutoFind: Scans 2479, 2480, 2481; Background Corrected with Scan 2473

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.0	13589	PASS
68	69	0.00	2	1.8	432	PASS
69	198	0.00	100	49.5	23991	PASS
70	69	0.00	2	1.1	252	PASS
127	198	10	80	44.2	21453	PASS
197	198	0.00	2	0.7	354	PASS
198	198	100	100	100.0	48504	PASS
199	198	5	9	7.0	3377	PASS
275	198	10	60	29.6	14365	PASS
365	198	1	100	3.7	1814	PASS
441	198	0.01	100	12.7	6143	PASS
442	198	50	100	84.1	40800	PASS
443	442	15	24	20.0	8160	PASS