

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM051419\
 Data File : BM020333.D
 Acq On : 14 May 2019 15:28
 Operator : JU/SJ
 Sample : K2769-05
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 P026-SS017-1824-01

Quant Time: May 15 03:48:29 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM043019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 01 03:58:37 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.76	152	55994	20.00	ng	-0.04
21) Naphthalene-d8	10.55	136	177962	20.00	ng	-0.04
39) Acenaphthene-d10	14.40	164	108837	20.00	ng	-0.03
64) Phenanthrene-d10	17.16	188	255834	20.00	ng	-0.02
76) Chrysene-d12	21.35	240	289255	20.00	ng	-0.02
87) Perylene-d12	23.63	264	347690	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.35	112	470523	137.36	ng	-0.02
7) Phenol-d6	6.93	99	592838	126.68	ng	-0.02
23) Nitrobenzene-d5	8.93	82	397425	88.17	ng	-0.03
42) 2,4,6-Tribromophenol	15.90	330	243645	144.22	ng	-0.02
45) 2-Fluorobiphenyl	13.02	172	783130	88.53	ng	-0.04
79) Terphenyl-d14	19.78	244	1355352	81.73	ng	-0.03
Target Compounds						
50) Dimethylphthalate	13.86	163	87979	9.511	ng	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM051419\
Data File : BM020333.D
Acq On : 14 May 2019 15:28
Operator : JU/SJ
Sample : K2769-05
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
P026-SS017-1824-01

Quant Time: May 15 03:48:29 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM043019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 01 03:58:37 2019
Response via : Initial Calibration

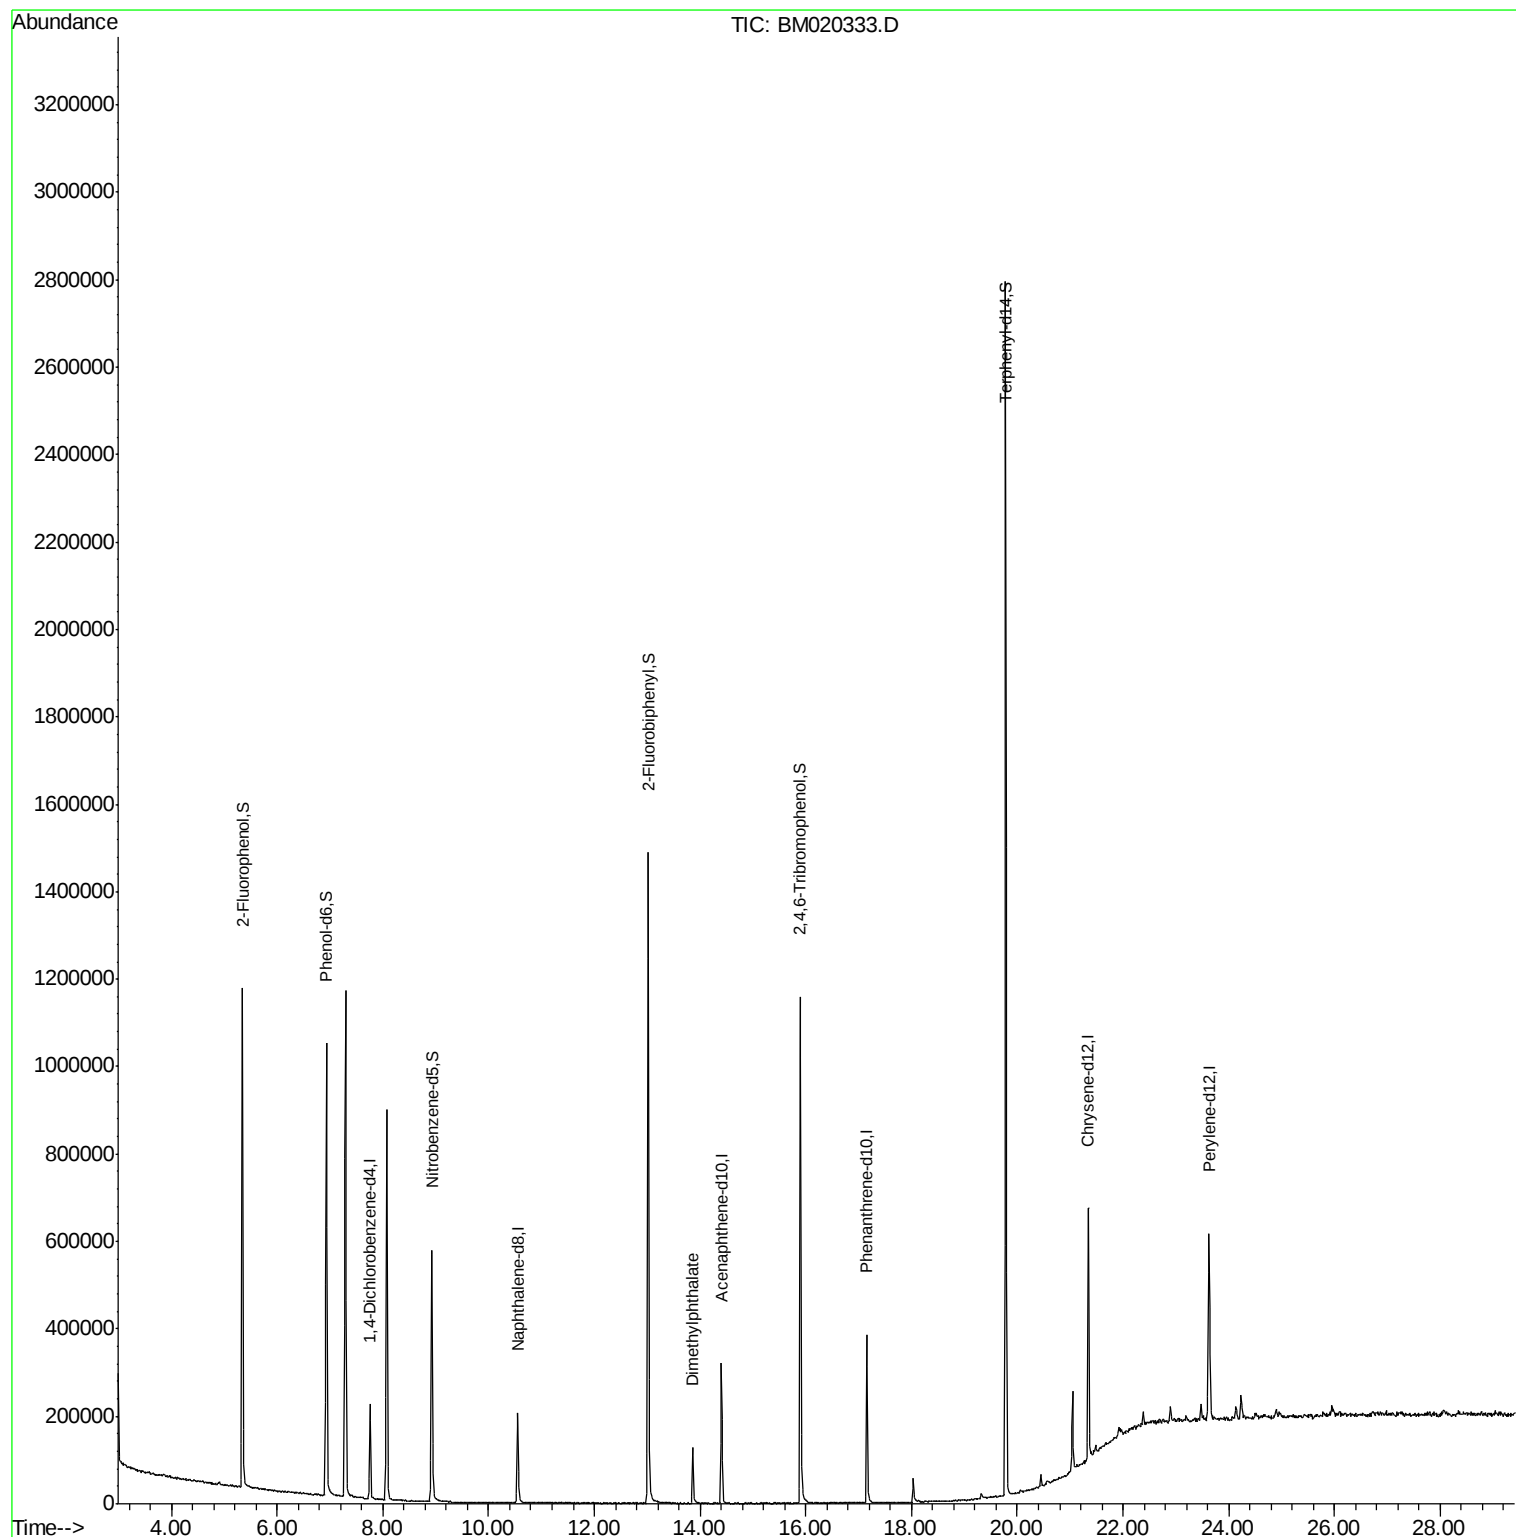

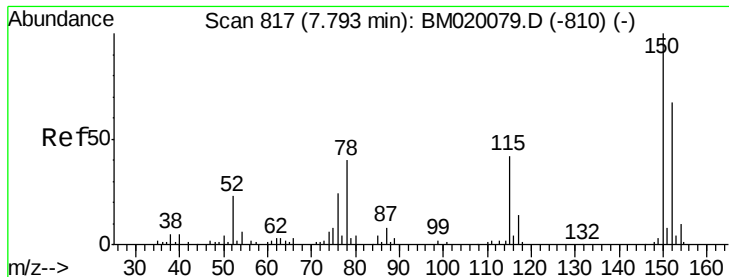


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.76 min Scan# 811
Delta R.T. -0.04 min
Lab File: BM020333.D
Acq: 14 May 2019 15:28

Instrument :
BNA_M
ClientSampleId :
P026-SS017-1824-01

Tgt Ion:152 Resp: 55994
Ion Ratio Lower Upper
152 100
150 160.0 119.8 179.8
115 63.6 50.8 76.2

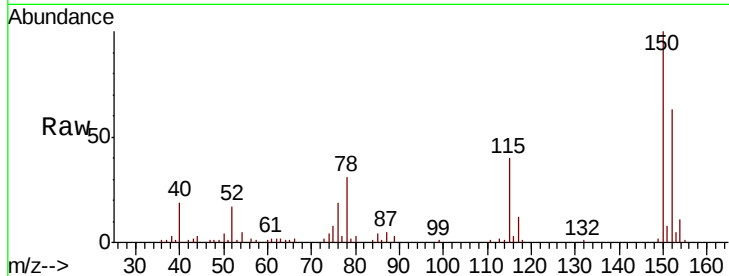


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

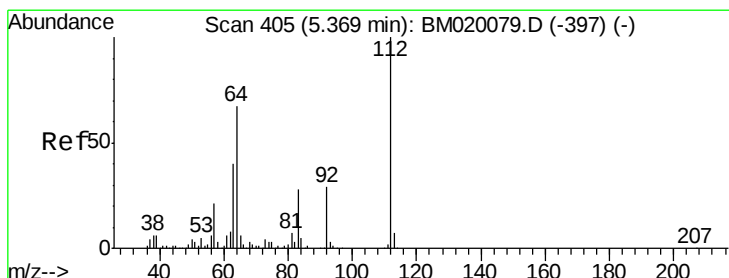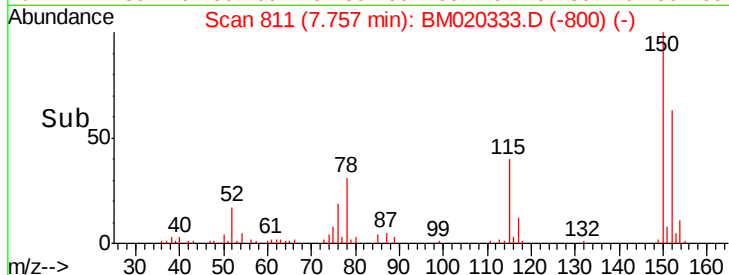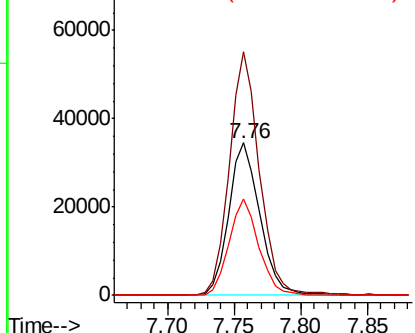



#5


2-Fluorophenol
Concen: 137.356 ng
RT: 5.35 min Scan# 401
Delta R.T. -0.02 min
Lab File: BM020333.D
Acq: 14 May 2019 15:28

Tgt Ion:112 Resp: 470523
Ion Ratio Lower Upper
112 100
64 61.6 53.8 80.6
63 33.3 32.3 48.5

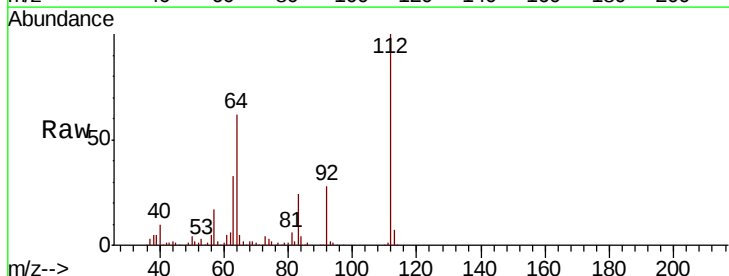

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BM0
Ion 63.00 (62.70 to 63.70): BM0

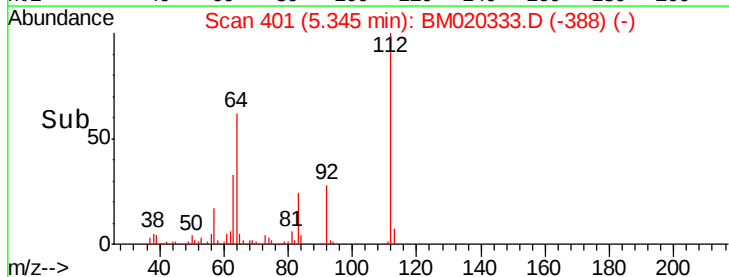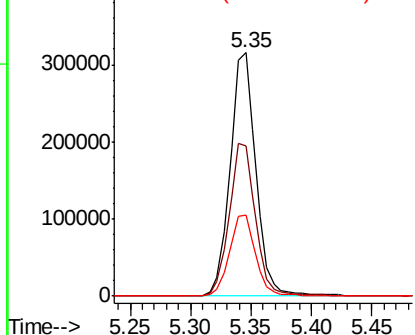

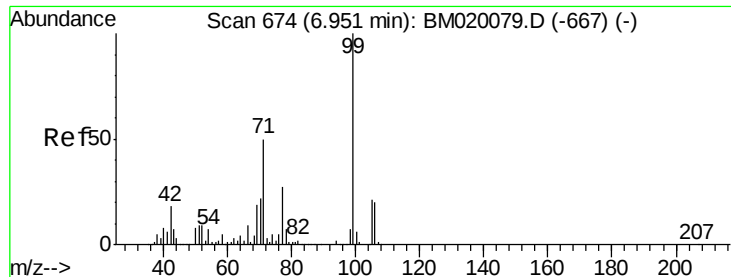

#7

Phenol-d6

Concen: 126.680 ng

RT: 6.93 min Scan# 670

Delta R.T. -0.02 min

Lab File: BM020333.D

Acq: 14 May 2019 15:28

Instrument :

BNA_M

ClientSampleId :

P026-SS017-1824-01


Tgt Ion: 99 Resp: 592838

Ion Ratio Lower Upper

99 100

42 14.2 14.2 21.2




71 44.1 40.3 60.5

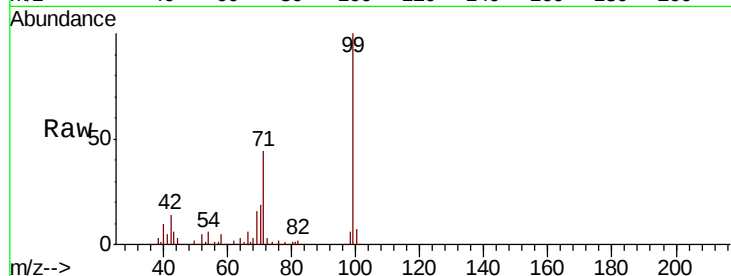

Abundance Ion 99.00 (98.70 to 99.70): BM020333.D (-657) (-)

Ion 42.00 (41.70 to 42.70): BM020333.D (-657) (-)

Ion 71.00 (70.70 to 71.70): BM020333.D (-657) (-)

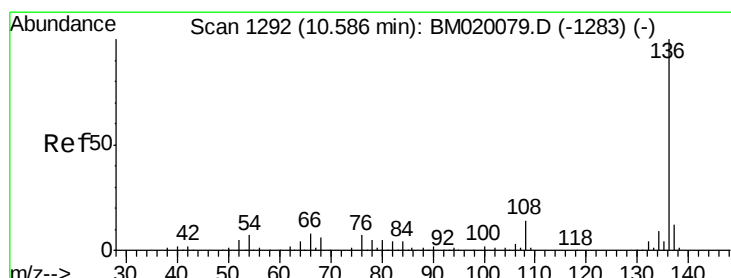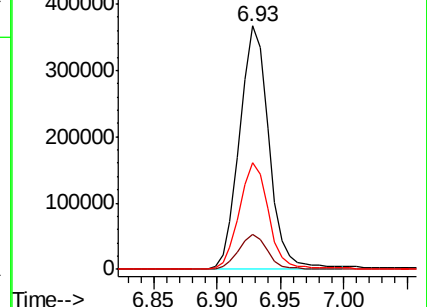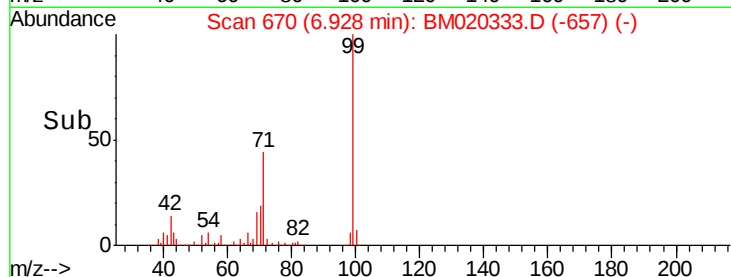

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.55 min Scan# 1286

Delta R.T. -0.04 min

Lab File: BM020333.D

Acq: 14 May 2019 15:28

Tgt Ion: 136 Resp: 177962


Ion Ratio Lower Upper

136 100

137 11.0 9.6 14.4

54 6.2 5.5 8.3

68 7.1 4.6 6.8#


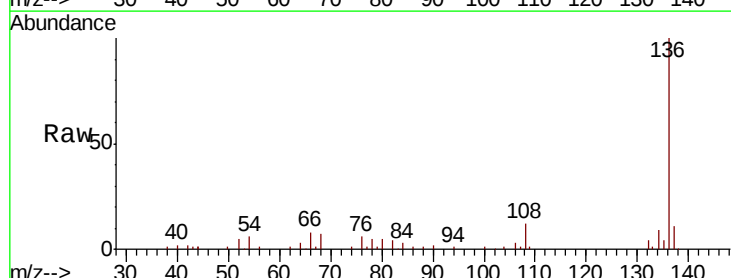


Abundance Ion 136.00 (135.70 to 136.70): BM020333.D (-1275) (-)

Ion 137.00 (136.70 to 137.70): BM020333.D (-1275) (-)

Ion 54.00 (53.70 to 54.70): BM020333.D (-1275) (-)

Ion 68.00 (67.70 to 68.70): BM020333.D (-1275) (-)


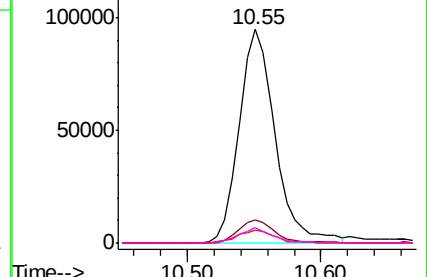
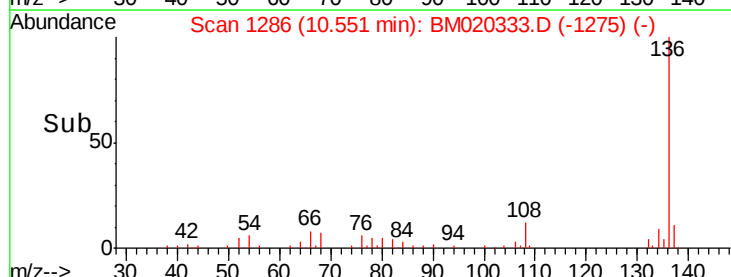




#23
 Nitrobenzene-d5
 Concen: 88.167 ng
 RT: 8.93 min Scan# 1010
 Delta R.T. -0.03 min
 Lab File: BM020333.D
 Acq: 14 May 2019 15:28




Instrument :
 BNA_M
 ClientSampleId :
 P026-SS017-1824-01


Tgt Ion	Ratio	Lower	Upper
82	100		
128	34.8	25.2	37.8
54	35.9	31.9	47.9

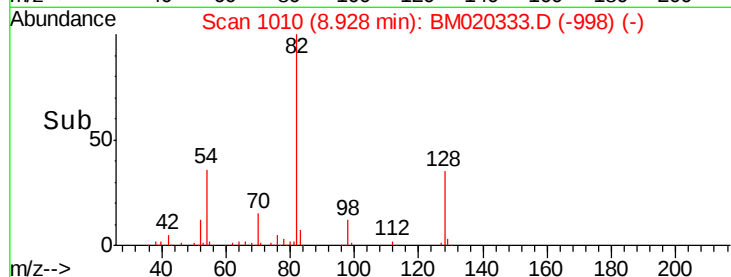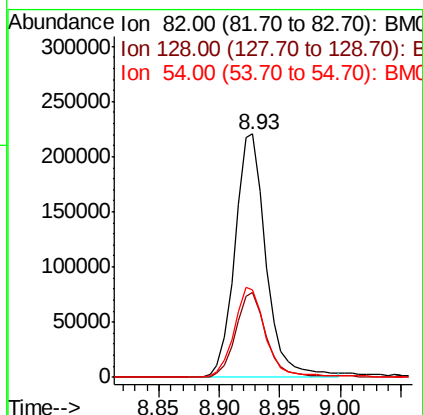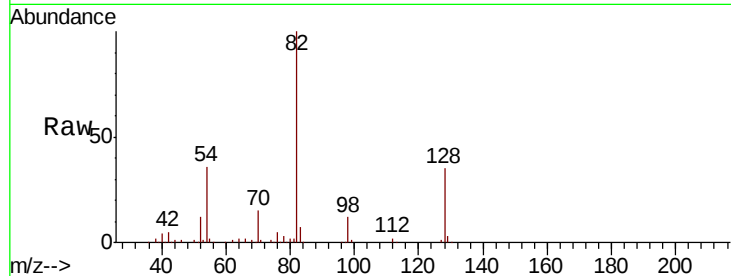

#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.40 min Scan# 1941
 Delta R.T. -0.03 min
 Lab File: BM020333.D
 Acq: 14 May 2019 15:28

Tgt Ion	Ratio	Lower	Upper
164	100		
162	106.9	82.2	123.2
160	45.2	37.6	56.4

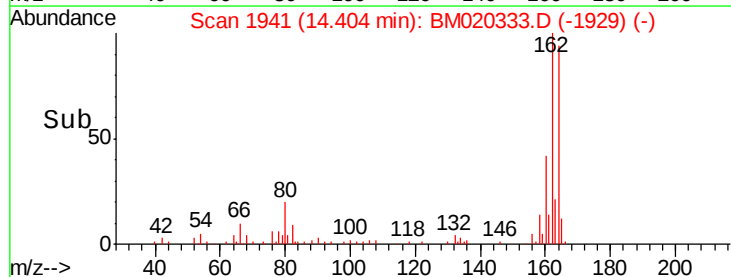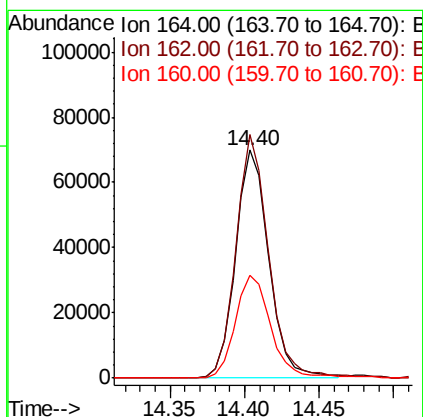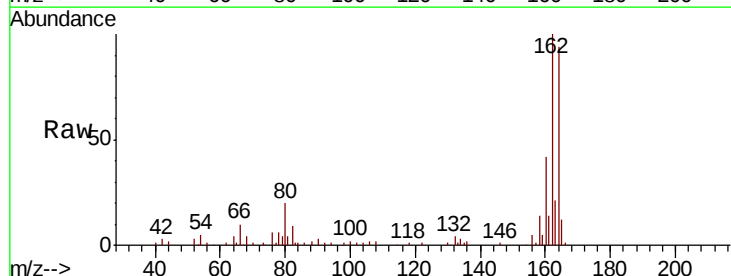


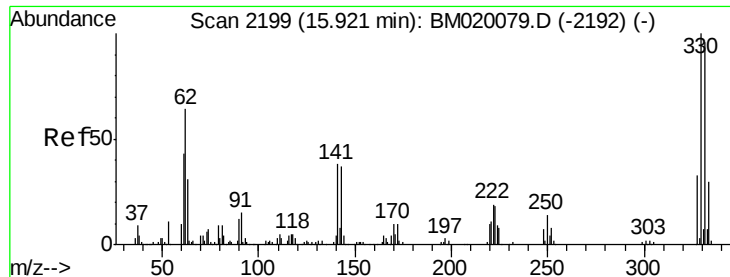

#42
 2,4,6-Tribromophenol
 Concen: 144.224 ng
 RT: 15.90 min Scan# 2195
 Delta R.T. -0.02 min
 Lab File: BM020333.D
 Acq: 14 May 2019 15:28

Instrument :
 BNA_M
 ClientSampleId :
 P026-SS017-1824-01

Tgt Ion	Ratio	Lower	Upper
330	100		
332	96.1	76.8	115.2
141	31.9	29.2	43.8



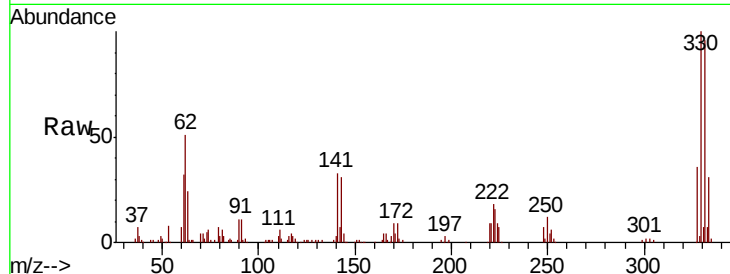


Abundance

Ion 329.80 (329.50 to 330.50): E


Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

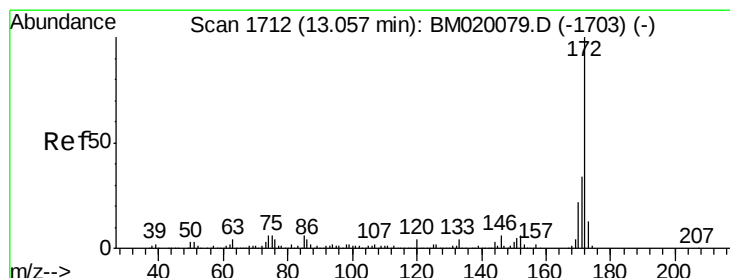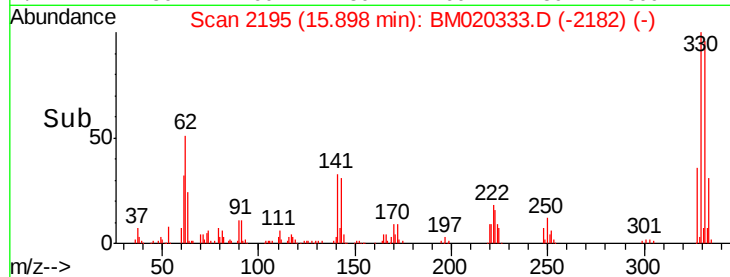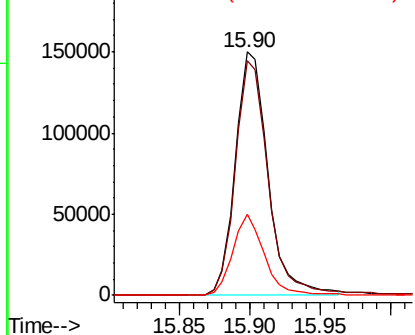

#45
 2-Fluorobiphenyl
 Concen: 88.530 ng
 RT: 13.02 min Scan# 1706
 Delta R.T. -0.04 min
 Lab File: BM020333.D
 Acq: 14 May 2019 15:28

Tgt Ion	Ratio	Lower	Upper
172	100		
171	34.8	27.3	40.9
170	23.0	17.9	26.9


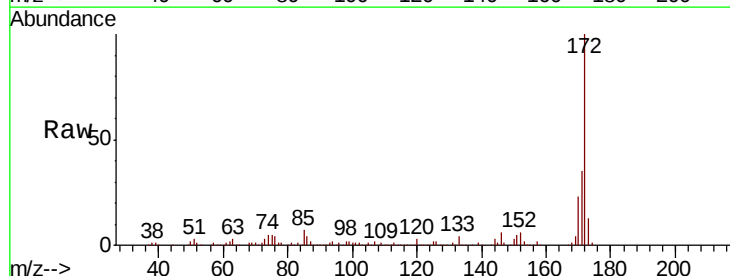


Abundance

Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

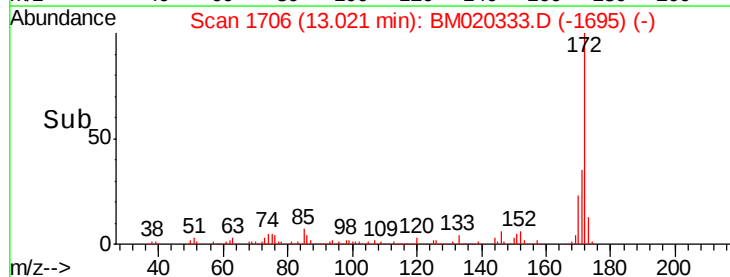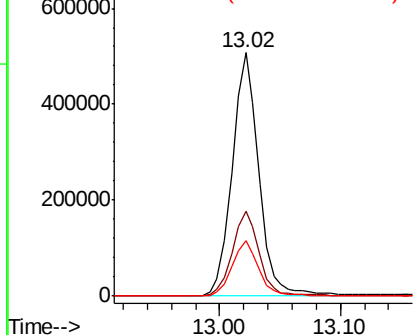



#50

Dimethylphthalate

Concen: 9.511 ng

RT: 13.86 min Scan# 1849

Delta R.T. -0.04 min

Lab File: BM020333.D

Acq: 14 May 2019 15:28

Instrument :

BNA_M

ClientSampleId :

P026-SS017-1824-01


Tgt Ion:163 Resp: 87979

Ion Ratio Lower Upper




163 100

194 4.2 3.6 5.4

164 10.0 8.4 12.6

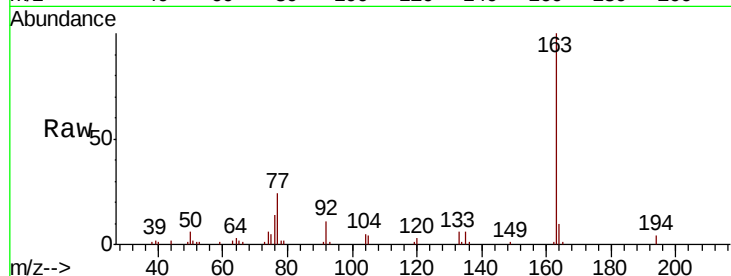

Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

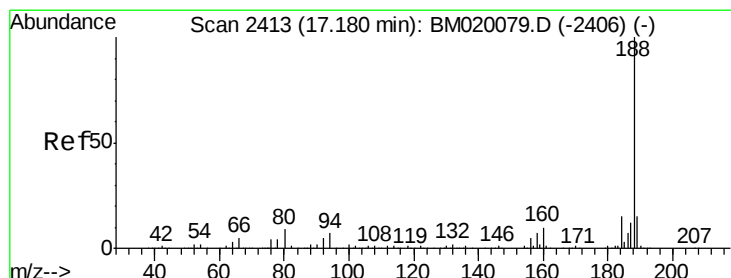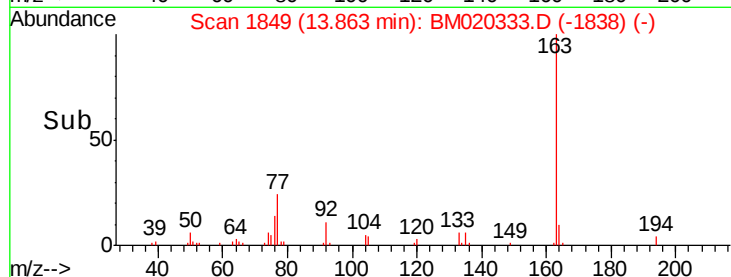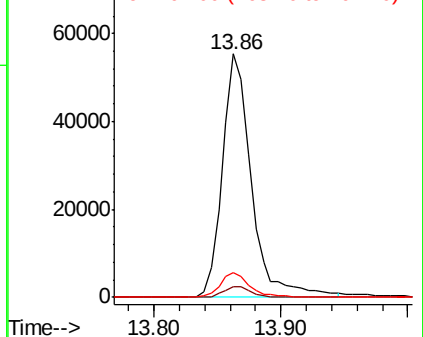

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.16 min Scan# 2409

Delta R.T. -0.02 min

Lab File: BM020333.D

Acq: 14 May 2019 15:28


Tgt Ion:188 Resp: 255834

Ion Ratio Lower Upper



188 100

94 7.3 5.8 8.6

80 9.7 7.4 11.2

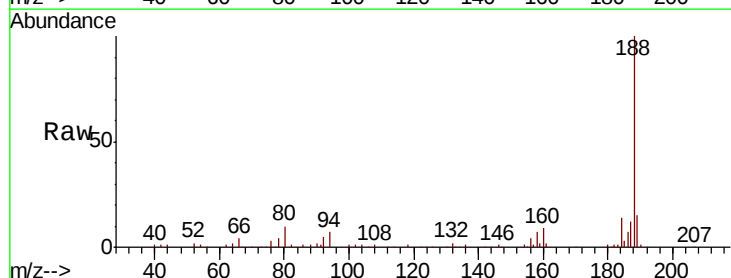

Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BM0
Ion 80.00 (79.70 to 80.70): BM0


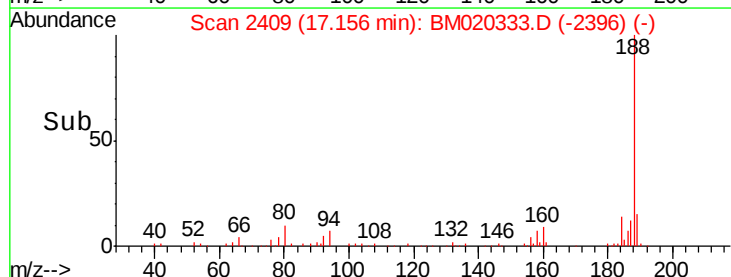
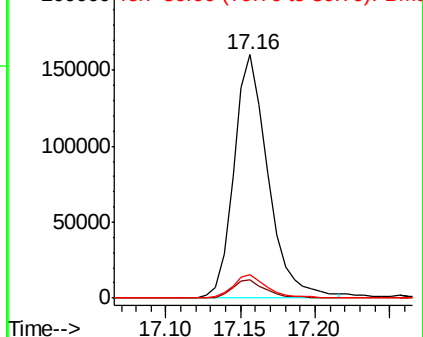




#76
 Chrysene-d12
 Concen: 20.000 ng
 RT: 21.35 min Scan# 3122
 Delta R.T. -0.02 min
 Lab File: BM020333.D
 Acq: 14 May 2019 15:28




Instrument :
 BNA_M
 ClientSampleId :
 P026-SS017-1824-01


Tgt Ion	Ratio	Lower	Upper
240	100		
120	6.9	5.6	8.4
236	25.4	20.9	31.3

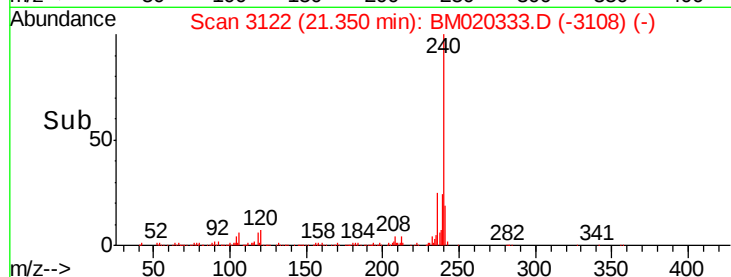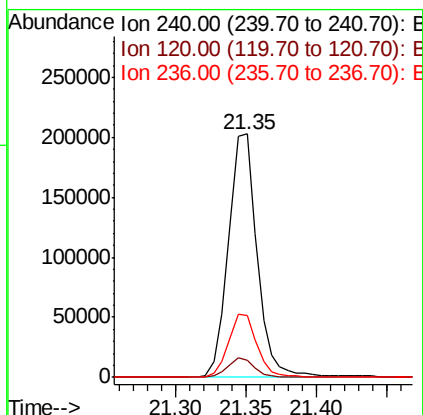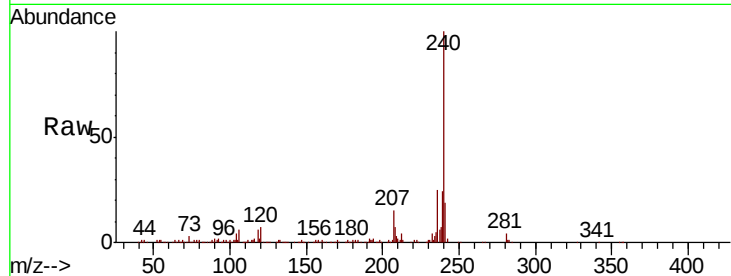

#79
 Terphenyl-d14
 Concen: 81.728 ng
 RT: 19.78 min Scan# 2855
 Delta R.T. -0.03 min
 Lab File: BM020333.D
 Acq: 14 May 2019 15:28

Tgt Ion	Ratio	Lower	Upper
244	100		
212	6.8	5.7	8.5
122	8.1	6.2	9.2

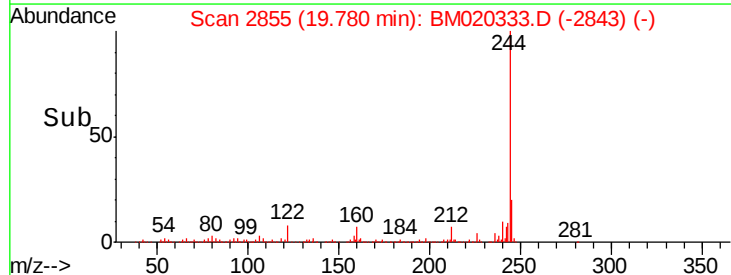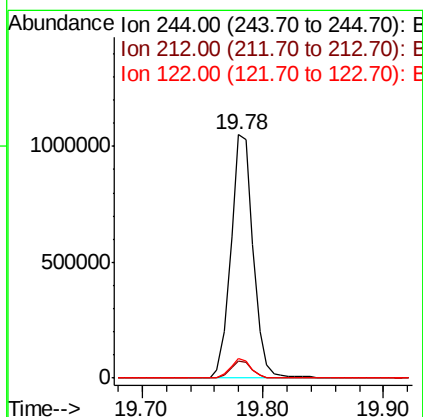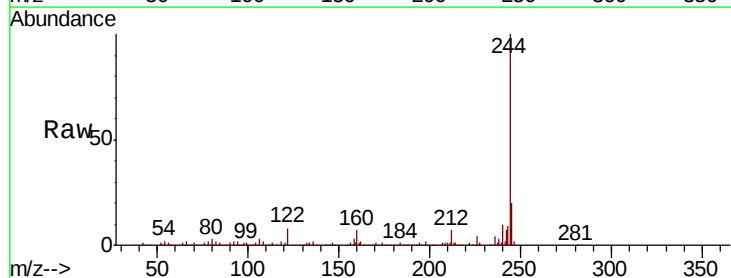

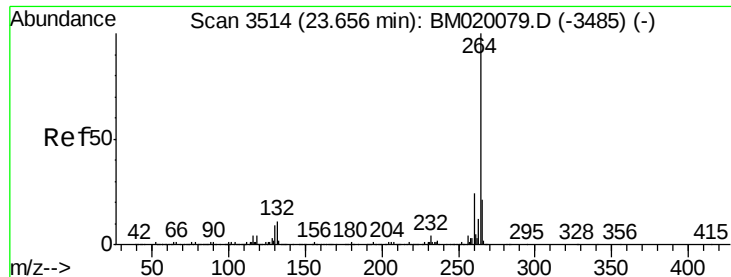

#87
Perylene-d12
Concen: 20.000 ng
RT: 23.63 min Scan# 3510
Delta R.T. -0.02 min
Lab File: BM020333.D
Acq: 14 May 2019 15:28

Instrument :
BNA_M
ClientSampleId :
P026-SS017-1824-01

Tgt Ion	Ratio	Lower	Upper
264	100		
260	21.9	19.2	28.8
265	22.3	16.9	25.3

