


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM051419\
 Data File : BM020327.D
 Acq On : 14 May 2019 11:12
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM043019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 01 03:58:37 2019

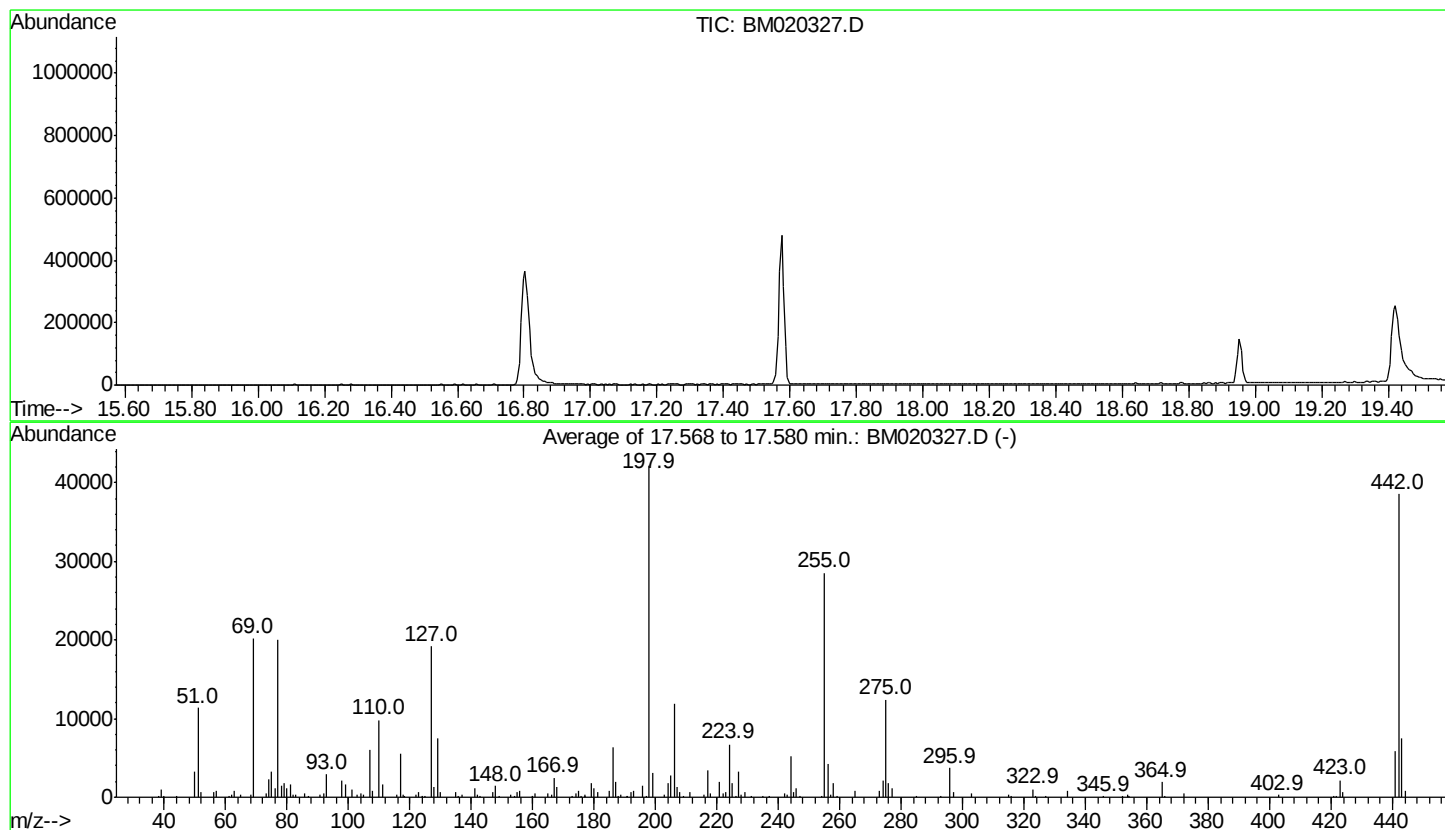

AutoFind: Scans 2479, 2480, 2481; Background Corrected with Scan 2473

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.9	11353	PASS
68	69	0.00	2	1.7	351	PASS
69	198	0.00	100	47.8	20148	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	45.4	19152	PASS
197	198	0.00	2	0.2	102	PASS
198	198	100	100	100.0	42165	PASS
199	198	5	9	7.2	3029	PASS
275	198	10	60	29.4	12411	PASS
365	198	1	100	4.5	1881	PASS
441	198	0.01	100	13.9	5863	PASS
442	198	50	100	91.4	38528	PASS
443	442	15	24	19.3	7444	PASS