

Data File : BM020353.D

Acq On : 16 May 2019 22:28

Operator : JU/SJ

Sample : SSTDICV020

Misc :

ALS Vial : 8 Sample Multiplier: 1




Quant Time: May 17 05:09:25 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051619MA.M

Quant Title : SVOA CALIBRATION

QLast Update : Fri May 17 04:58:03 2019

Response via : Initial Calibration

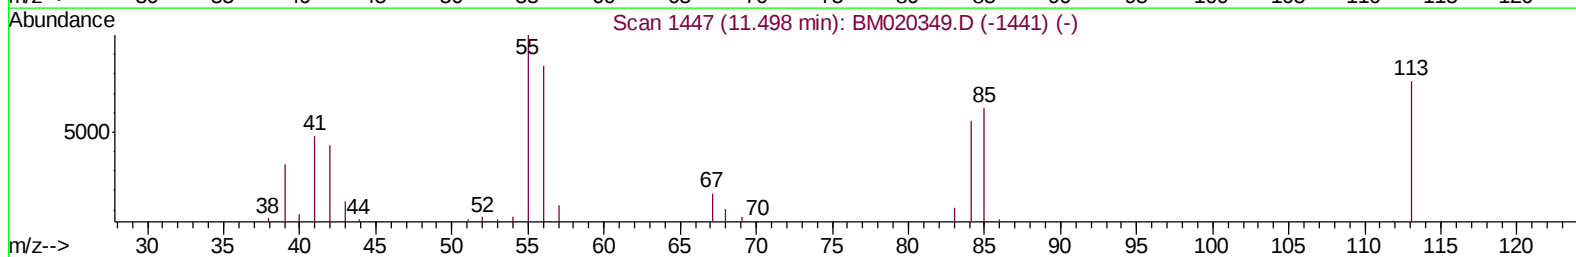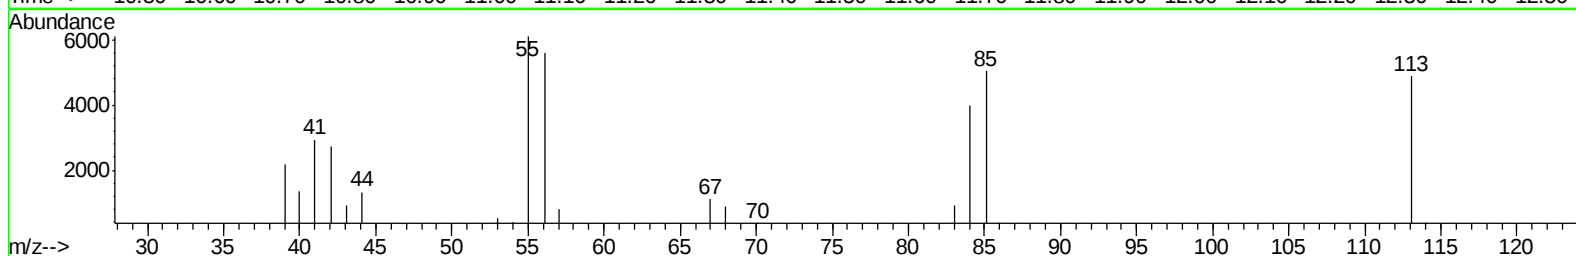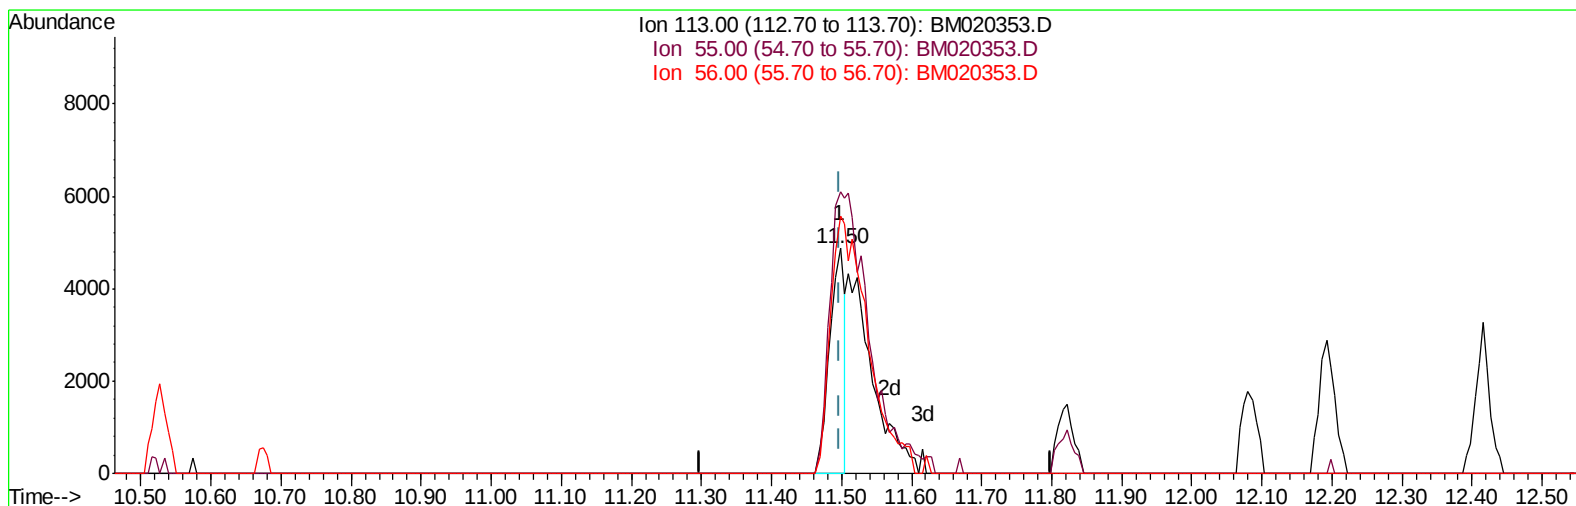

TIC: BM020353.D

(32) Caprolactam

11.498min (-0.000) 6.70ng/ul

response 7225

Ion	Exp%	Act%
113.00	100	100
55.00	130.70	125.16
56.00	110.50	114.37
0.00	0.00	0.00