
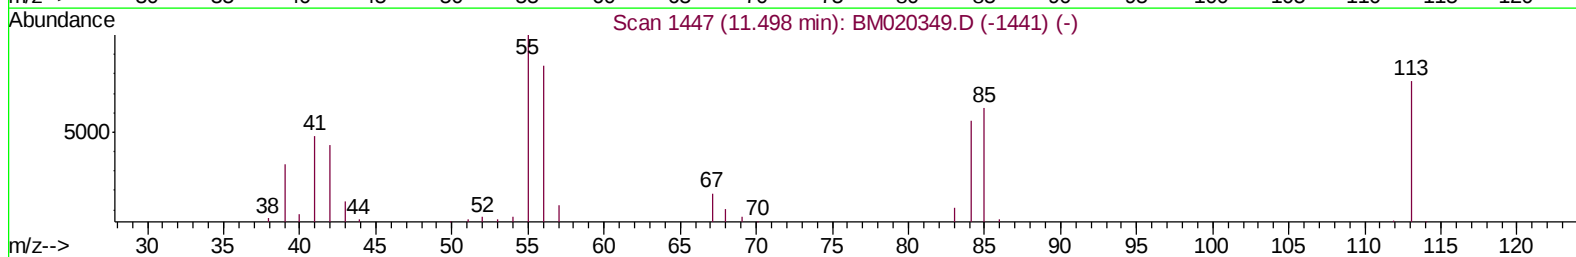
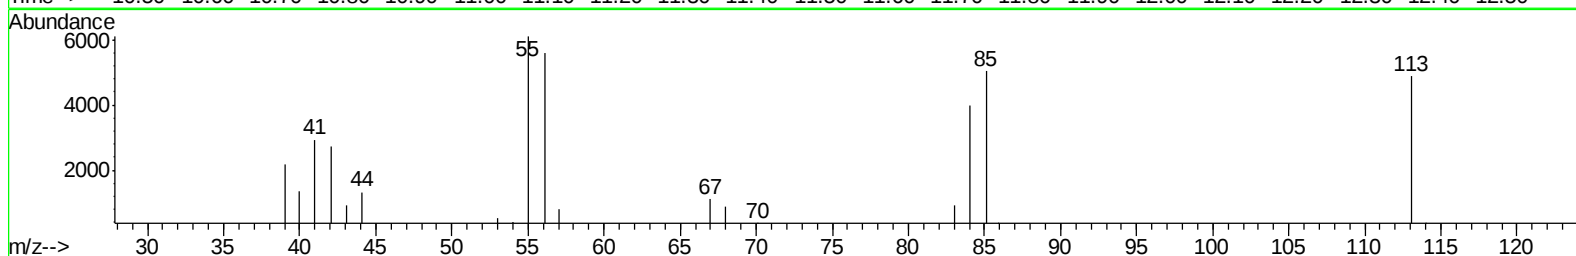


Data File : BM020353.D
Acq On : 16 May 2019 22:28
Operator : JU/SJ
Sample : SSTDICV020
Misc :
ALS Vial : 8 Sample Multiplier: 1

Quant Time: May 17 05:09:25 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051619MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 17 04:58:03 2019
Response via : Initial Calibration

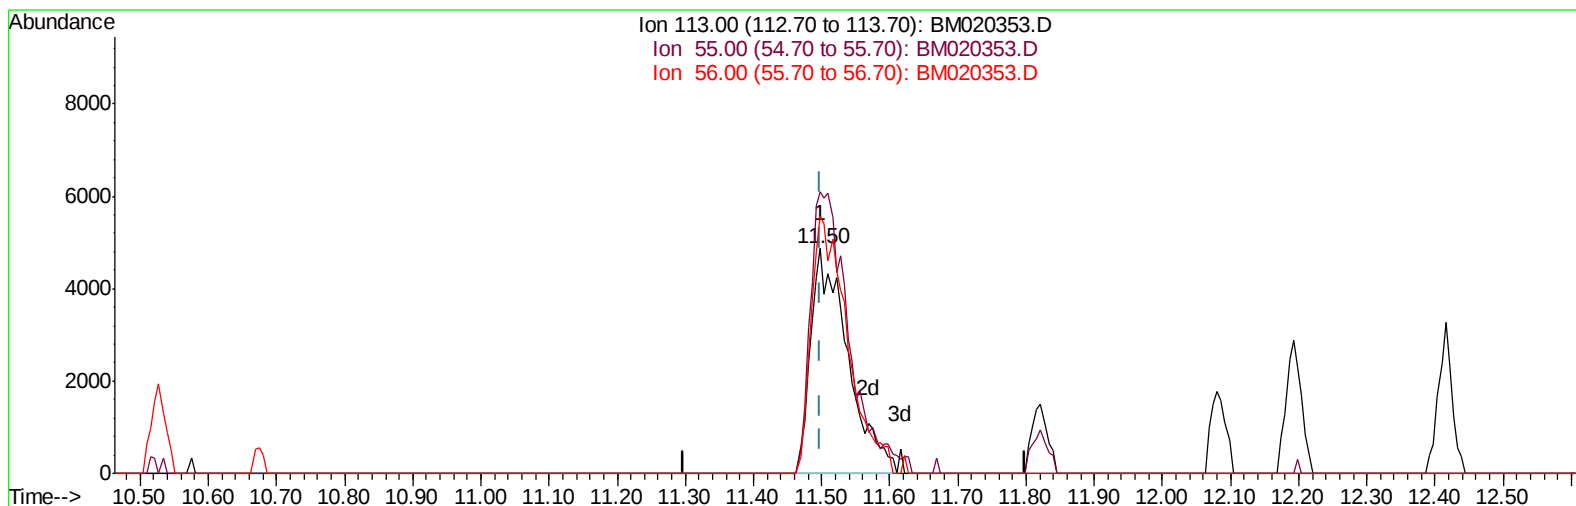

TIC: BM020353.D

(32) Caprolactam

11.498min (-0.000) 17.08ng/ul m

response 18421

Ion	Exp%	Act%
113.00	100	100
55.00	130.70	125.16
56.00	110.50	114.37
0.00	0.00	0.00