

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM051819\
 Data File : BM020417.D
 Acq On : 19 May 2019 02:17
 Operator : JU/SJ
 Sample : K2633-04
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: May 20 07:15:18 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051619MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat May 18 05:13:49 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.74	152	129635	20.00	ng/ul	0.00
18) Naphthalene-d8	10.53	136	464532	20.00	ng/ul	0.01
35) Acenaphthene-d10	14.40	164	345337	20.00	ng/ul	0.02
61) Phenanthrene-d10	17.17	188	480842	20.00	ng/ul	0.04
77) Chrysene-d12	21.35	240	503869	20.00	ng/ul	0.03
85) Perylene-d12	23.49	264	739408	20.00	ng/ul	-0.11

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.23	96	12359	3.52	ng/uL	0.00
5) Phenol-d5	6.91	99	231169	22.35	ng/ul	0.01
7) Bis-(2-Chloroethyl)ether-d	7.08	67	158895	24.17	ng/ul	0.00
9) 2-Chlorophenol-d4	7.27	132	182440	24.05	ng/ul	0.00
13) 4-Methylphenol-d8	8.45	113	98655	13.10	ng/ul	0.01
19) Nitrobenzene-d5	8.91	128	89062	29.47	ng/ul	0.01
22) 2-Nitrophenol-d4	9.63	143	99282	29.78	ng/ul	0.01
26) 2,4-Dichlorophenol-d3	10.16	165	185077	26.26	ng/ul	0.01
29) 4-Chloroaniline-d4	10.69	131	44442	6.10	ng/ul	0.02
43) Dimethylphthalate-d6	13.82	166	543073	21.86	ng/ul	0.03
46) Acenaphthylene-d8	14.11	160	636376	20.48	ng/ul	0.04
51) 4-Nitrophenol-d4	14.63	143	68262	18.92	ng/ul	0.04
57) Fluorene-d10	15.40	176	432516	19.57	ng/ul	0.03
62) 4,6-Dinitro-2-methylphenol	15.52	200	79	0.03	ng/ul	0.01
70) Anthracene-d10	17.27	188	574285	27.85	ng/ul	0.04
78) Pyrene-d10	19.56	212	663180	27.32	ng/ul	0.04
89) Benzo(a)pyrene-d12	23.49	264	718862	21.39	ng/ul	0.04

Target Compounds

					Ovalue	
6) Phenol	6.93	94	20945	1.925	ng/ul	99
17) Hexachloroethane	8.83	117	9281	2.539	ng/ul#	1
28) Naphthalene	10.59	128	1324861	62.076	ng/ul	99
32) Caprolactam	11.53	113	3203	1.637	ng/ul#	36
34) 2-Methylnaphthalene	12.25	142	22800336	1475.467	ng/ul	90
40) 1,1'-Biphenyl	13.23	154	4701523	190.170	ng/ul	100
44) Dimethylphthalate	13.87	163	149467	6.081	ng/ul	99
47) Acenaphthylene	14.15	152	13210409	450.753	ng/ul#	94
49) Acenaphthene	14.47	153	1537169	76.294	ng/ul	96
50) 2,4-Dinitrophenol	14.56	184	3593	1.352	ng/ul#	1
53) Dibenzofuran	14.80	168	1779640	58.328	ng/ul	96
54) 2,4-Dinitrotoluene	14.80	165	94353	14.371	ng/ul#	1
58) Fluorene	15.48	166	8580311	351.047	ng/ul#	95
64) N-Nitrosodiphenylamine	15.66	169	128776	10.824	ng/ul	92
69) Phenanthrene	17.30	178	3170398	138.379	ng/ul	98
71) Anthracene	17.30	178	3175124	136.240	ng/ul	99
74) Carbazole	17.57	167	63066	3.188	ng/ul#	71
76) Fluoranthene	19.23	202	8108459	280.172	ng/ul	98
79) Pyrene	19.49	202	334559	11.062	ng/ul	97
82) Benzo(a)anthracene	21.39	228	4153736	136.966	ng/ul	94
84) Chrysene	21.39	228	4153736	143.322	ng/ul	96
88) Benzo(k)fluoranthene	22.95	252	3039394	73.326	ng/ul	98
90) Benzo(a)pyrene	23.54	252	1402103	35.305	ng/ul	99

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM051819\
Data File : BM020417.D
Acq On : 19 May 2019 02:17
Operator : JU/SJ
Sample : K2633-04
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: May 20 07:15:18 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051619MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat May 18 05:13:49 2019
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
91) Indeno(1,2,3-cd)pyrene	25.71	276	132552	2.929	ng/ul	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM051819\
Data File : BM020417.D
Acq On : 19 May 2019 02:17
Operator : JU/SJ
Sample : K2633-04
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: May 20 07:15:18 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051619MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat May 18 05:13:49 2019
Response via : Initial Calibration

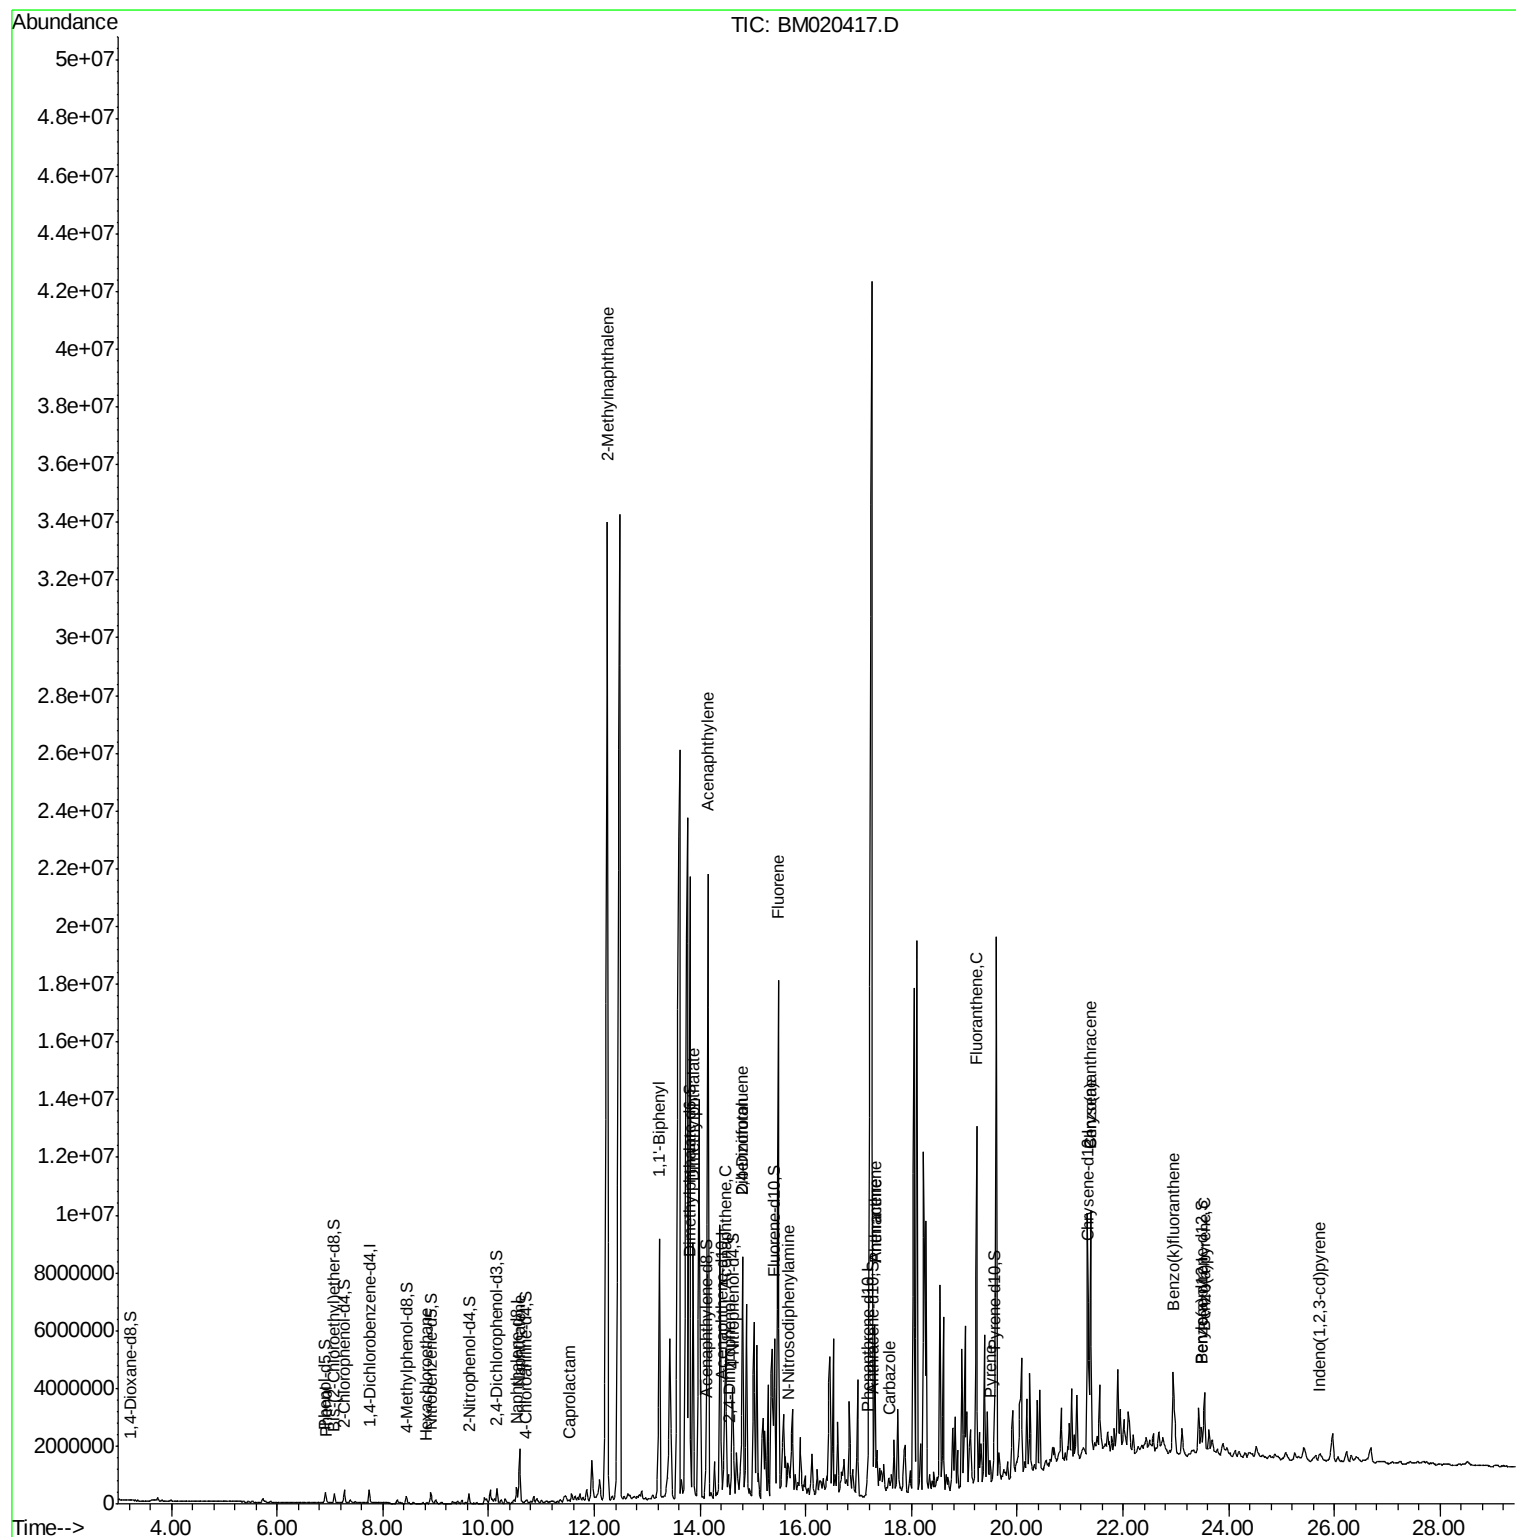

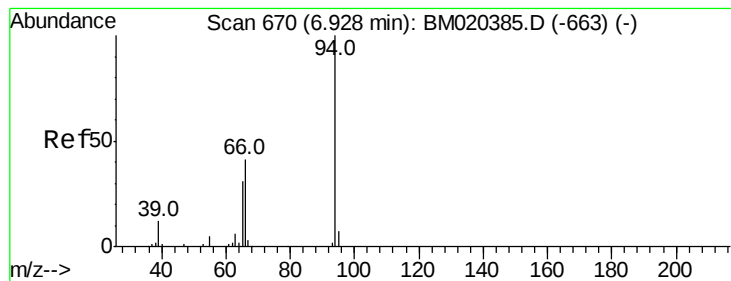

#6

Phenol

Concen: 1.925 ng/ul

RT: 6.93 min Scan# 671

Delta R.T. 0.01 min

Lab File: BM020417.D

Acq: 19 May 2019 02:17

Instrument :

BNA_M

ClientSampleId :





Tot Ion: 94 Resp: 20945

Ion Ratio Lower Upper

94 100

65 31.4 25.4 38.0

66 46.1 36.5 54.7

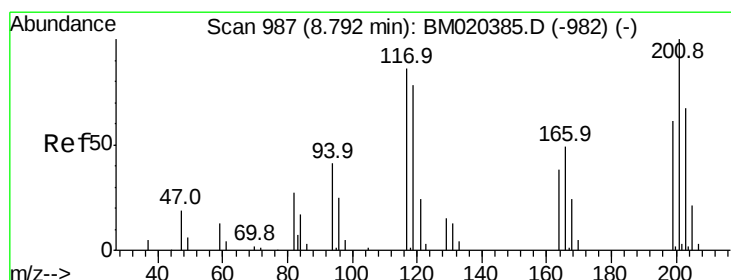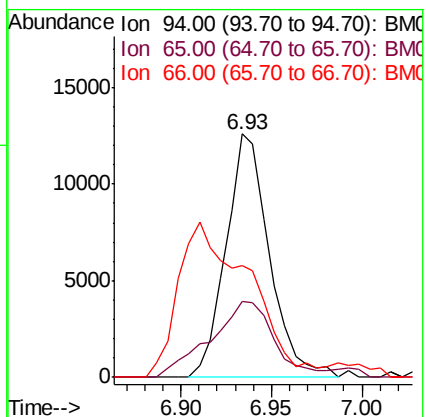

#17

Hexachloroethane

Concen: 2.539 ng/ul

RT: 8.83 min Scan# 993

Delta R.T. 0.04 min

Lab File: BM020417.D

Acq: 19 May 2019 02:17




Tgt Ion: 117 Resp: 9281


Ion Ratio Lower Upper

117 100

201 0.0 102.4 153.6#

199 0.0 63.3 94.9#

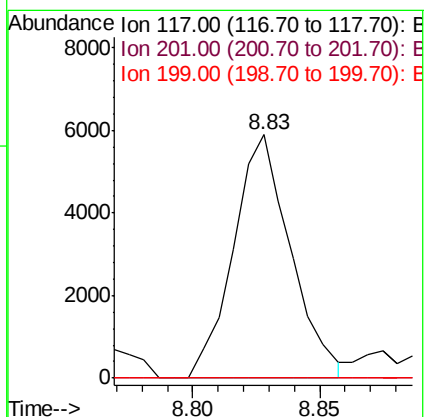

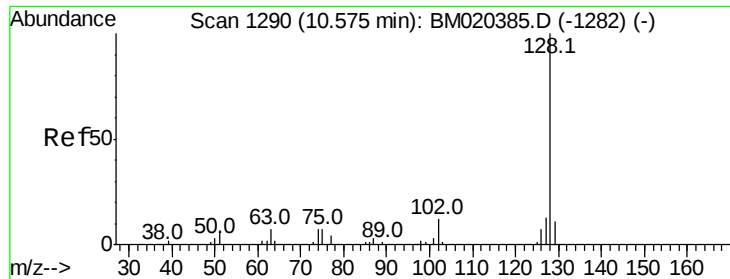

#28

Naphthalene

Concen: 62.076 ng/ul

RT: 10.59 min Scan# 1292

Delta R.T. 0.01 min

Lab File: BM020417.D

Acq: 19 May 2019 02:17

Instrument :

BNA_M

ClientSampleId :


Tot Ion:128 Resp: 1324861

Ion Ratio Lower Upper

128 100

129 11.6 8.6 13.0




127 13.2 10.6 15.8

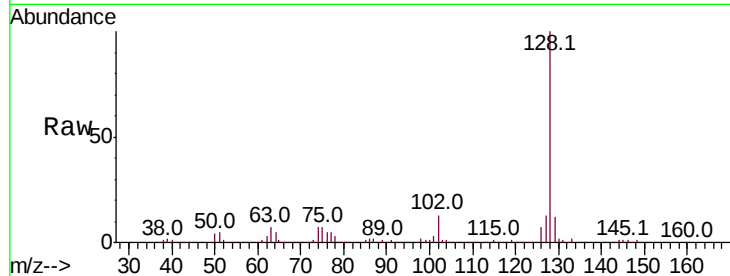

Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

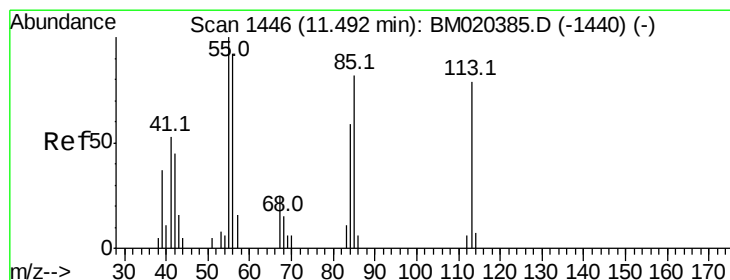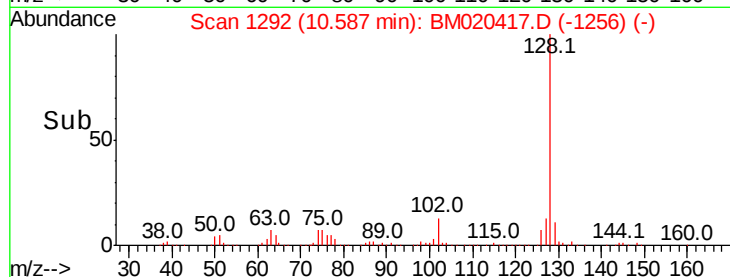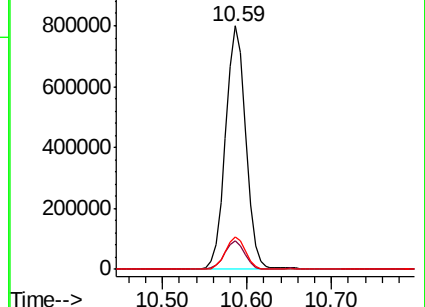

#32

Caprolactam

Concen: 1.637 ng/ul

RT: 11.53 min Scan# 1452

Delta R.T. 0.04 min

Lab File: BM020417.D

Acq: 19 May 2019 02:17


Tgt Ion:113 Resp: 3203

Ion Ratio Lower Upper

113 100

55 178.0 104.6 156.8#



56 207.6 88.4 132.6#

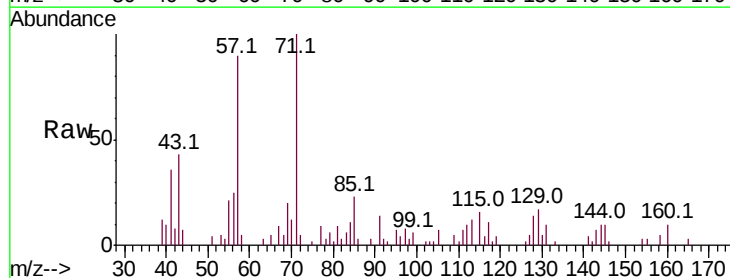


Abundance Ion 113.00 (112.70 to 113.70): E

Ion 55.00 (54.70 to 55.70): BM0

Ion 56.00 (55.70 to 56.70): BM0

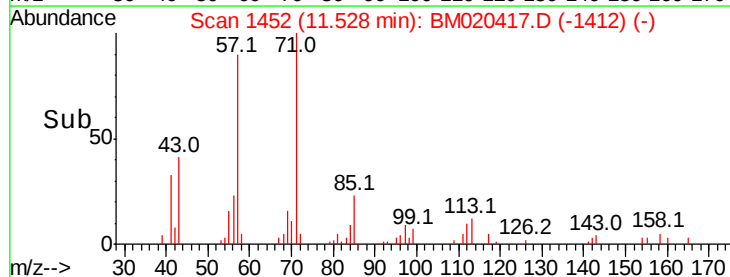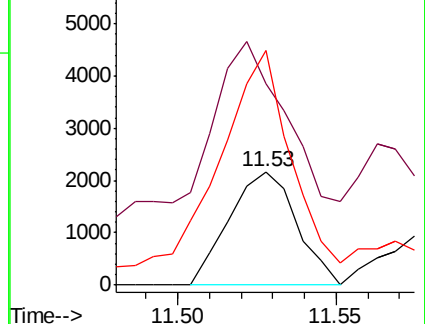







#34
 2-Methylnaphthalene
 Concen: 1475.467 ng/ul
 RT: 12.25 min Scan# 1574
 Delta R.T. 0.06 min
 Lab File: BM020417.D
 Acq: 19 May 2019 02:17

Instrument :
 BNA_M
 ClientSampled :

Tot Ion:142 Resp:22800336
 Ion Ratio Lower Upper
 142 100
 141 94.9 68.6 102.8

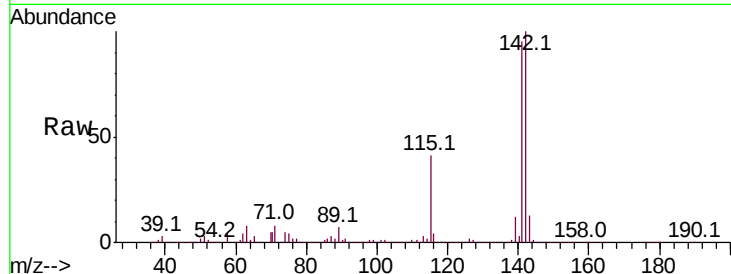


Abundance Ion 142.00 (141.70 to 142.70): E
 1e+07 Ion 141.00 (140.70 to 141.70): E

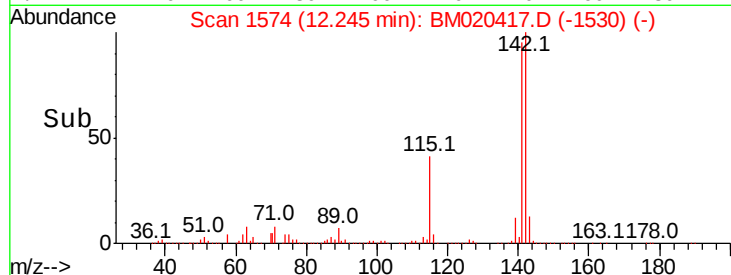
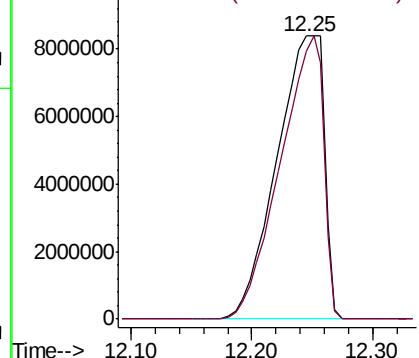



#40
 1,1'-Biphenyl
 Concen: 190.170 ng/ul
 RT: 13.23 min Scan# 1742
 Delta R.T. 0.02 min
 Lab File: BM020417.D
 Acq: 19 May 2019 02:17

Tgt Ion:154 Resp: 4701523
 Ion Ratio Lower Upper
 154 100
 153 40.4 32.2 48.4
 76 13.9 11.0 16.4

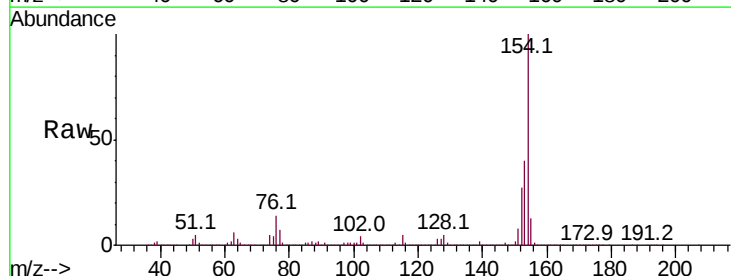

Abundance Ion 154.00 (153.70 to 154.70): E
 Ion 153.00 (152.70 to 153.70): E
 Ion 76.00 (75.70 to 76.70): BM

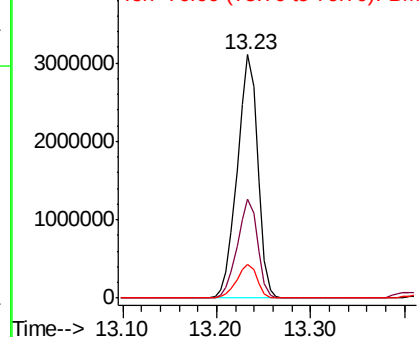



#44

Dimethylphthalate

Concen: 6.081 ng/ul

RT: 13.87 min Scan# 1850

Delta R.T. 0.03 min

Lab File: BM020417.D

Acq: 19 May 2019 02:17

Instrument :

BNA_M

ClientSampleId :


Tot Ion:163 Resp: 149467

Ion Ratio Lower Upper

163 100

194 4.6 3.3 4.9

164 10.4 8.0 12.0



Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

150000

100000

50000



0

13.85

13.87

13.90

Time-->



#47

Acenaphthylene

Concen: 450.753 ng/ul

RT: 14.15 min Scan# 1898

Delta R.T. 0.05 min

Lab File: BM020417.D

Acq: 19 May 2019 02:17


Tgt Ion:152 Resp:13210409

Ion Ratio Lower Upper

152 100

151 20.9 15.4 23.0

153 16.1 10.3 15.5#



Abundance

Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

Ion 153.00 (152.70 to 153.70): E

8000000

6000000

4000000

2000000


0


14.10

14.15

14.20

Time-->



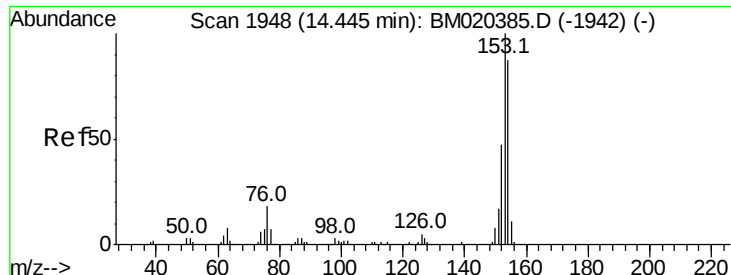

#49

Acenaphthene

Concen: 76.294 ng/ul

RT: 14.47 min Scan# 1953

Delta R.T. 0.03 min

Lab File: BM020417.D

Acq: 19 May 2019 02:17

Instrument :

BNA_M

ClientSampleId :


Tot Ion:153 Resp: 1537169

Ion Ratio Lower Upper




153 100

152 52.0 37.9 56.9

154 86.1 71.2 106.8

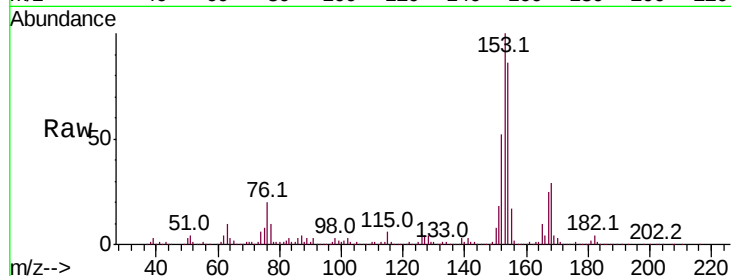

Abundance Ion 153.00 (152.70 to 153.70): E
Ion 152.00 (151.70 to 152.70): E
Ion 154.00 (153.70 to 154.70): E

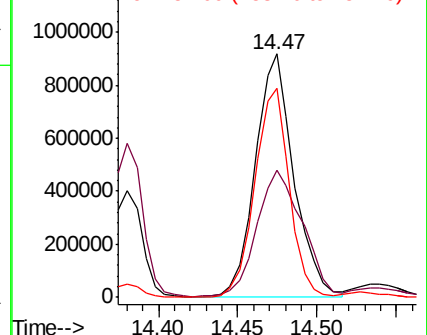

#50

2,4-Dinitrophenol

Concen: 1.352 ng/ul

RT: 14.56 min Scan# 1967

Delta R.T. 0.04 min

Lab File: BM020417.D

Acq: 19 May 2019 02:17


Tgt Ion:184 Resp: 3593

Ion Ratio Lower Upper



184 100


63 485.6 58.6 88.0#

154 228.4 47.4 71.0#



Abundance Ion 184.00 (183.70 to 184.70): E
Ion 63.00 (62.70 to 63.70): BM0
Ion 154.00 (153.70 to 154.70): E

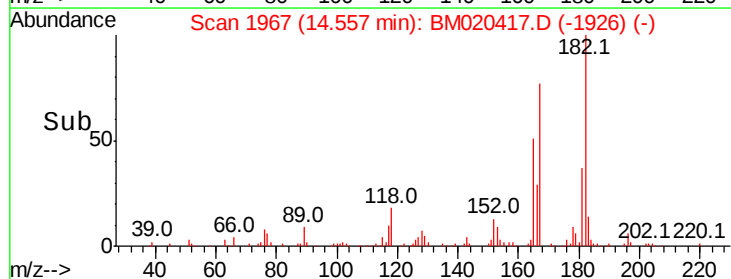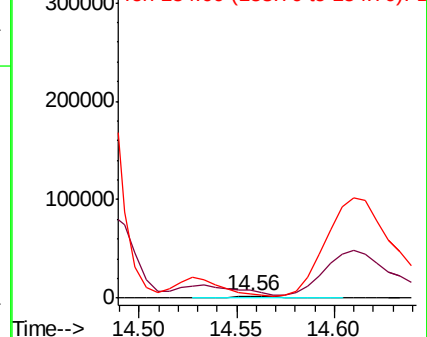



#53

Dibenzenofuran

Concen: 58.328 ng/ul

RT: 14.80 min Scan# 2009

Delta R.T. 0.02 min

Lab File: BM020417.D

Acq: 19 May 2019 02:17

Instrument :

BNA_M


ClientSampleId :

Tot Ion:168 Resp: 1779640

Ion Ratio Lower Upper




168 100

139 39.9 30.1 45.1

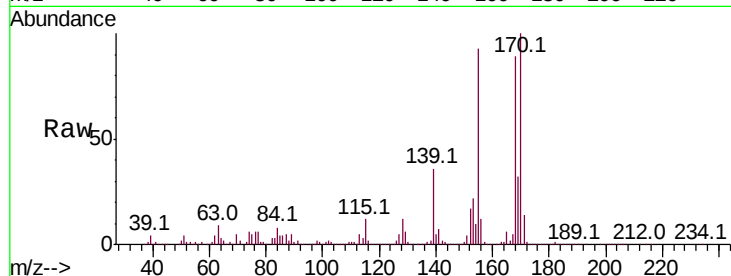

Abundance Ion 168.00 (167.70 to 168.70): E

Ion 139.00 (138.70 to 139.70): E

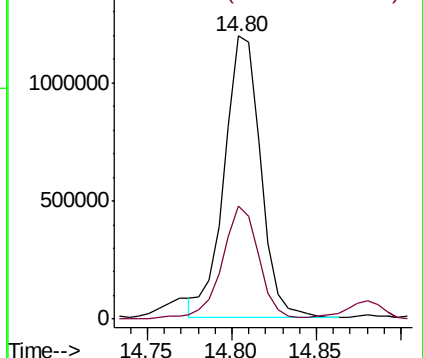

#54

2,4-Dinitrotoluene

Concen: 14.371 ng/ul

RT: 14.80 min Scan# 2009

Delta R.T. 0.04 min

Lab File: BM020417.D

Acq: 19 May 2019 02:17


Tgt Ion:165 Resp: 94353

Ion Ratio Lower Upper

165 100

63 166.6 43.2 64.8#



182 13.2 2.6 4.0#




Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BM0

Ion 182.00 (181.70 to 182.70): E

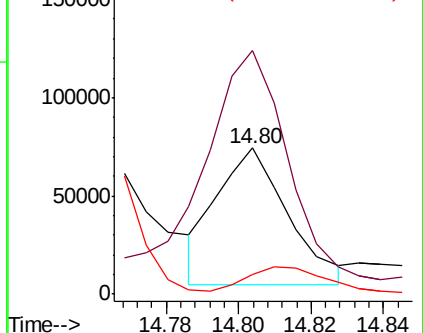

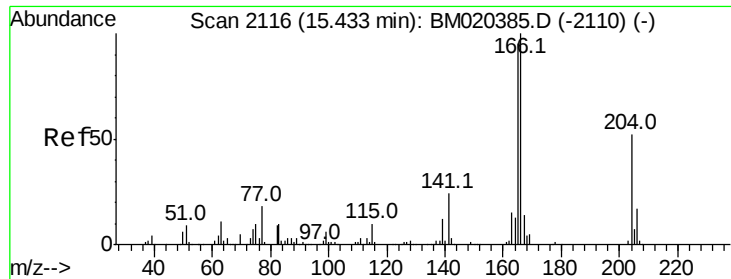

#58

Fluorene

Concen: 351.047 ng/ul

RT: 15.48 min Scan# 2124

Delta R.T. 0.05 min

Lab File: BM020417.D

Acq: 19 May 2019 02:17

Instrument :

BNA_M

ClientSampleId :


Tot Ion:166 Resp: 8580311

Ion Ratio Lower Upper

166 100

165 100.0 77.1 115.7




167 18.1 11.1 16.7#



Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

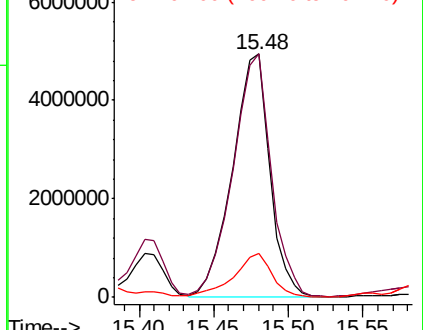

#64

N-Nitrosodiphenylamine

Concen: 10.824 ng/ul

RT: 15.66 min Scan# 2154

Delta R.T. 0.01 min

Lab File: BM020417.D

Acq: 19 May 2019 02:17


Tgt Ion:169 Resp: 128776

Ion Ratio Lower Upper

169 100

168 60.1 53.2 79.8



167 39.7 28.2 42.2




Abundance Ion 169.00 (168.70 to 169.70): E

Ion 168.00 (167.70 to 168.70): E

Ion 167.00 (166.70 to 167.70): E

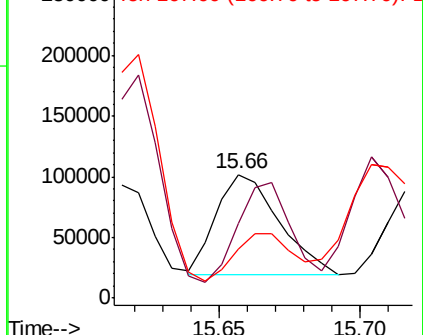

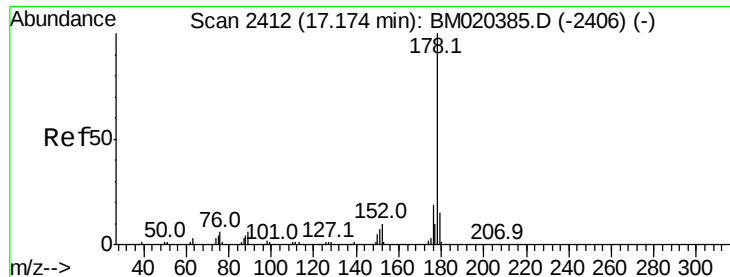

#69

Phenanthrene

Concen: 138.379 ng/ul

RT: 17.30 min Scan# 2434

Delta R.T. 0.13 min

Lab File: BM020417.D

Acq: 19 May 2019 02:17

Instrument :

BNA_M

ClientSampleId :





Tot Ion:178 Resp: 3170398

Ion Ratio Lower Upper

178 100

179 16.0 11.9 17.9

176 17.8 14.6 22.0

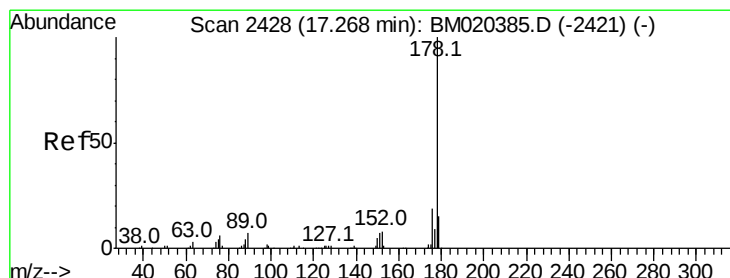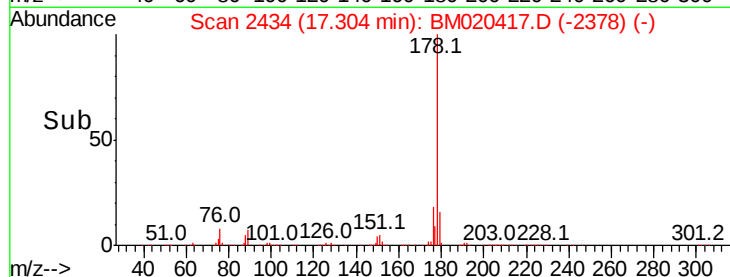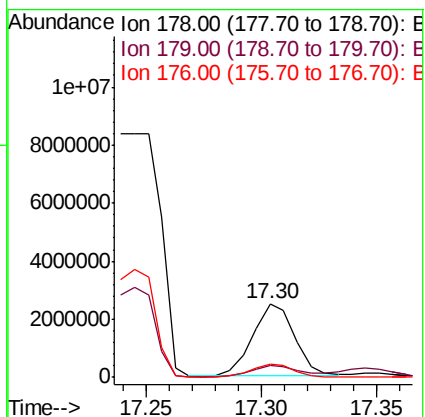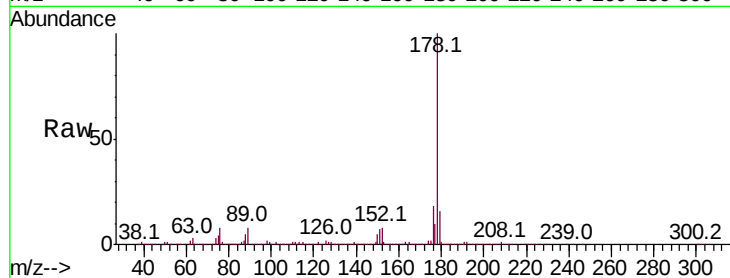

#71

Anthracene

Concen: 136.240 ng/ul

RT: 17.30 min Scan# 2434

Delta R.T. 0.04 min

Lab File: BM020417.D

Acq: 19 May 2019 02:17




Tgt Ion:178 Resp: 3175124


Ion Ratio Lower Upper

178 100

179 16.0 12.4 18.6

176 17.8 14.4 21.6

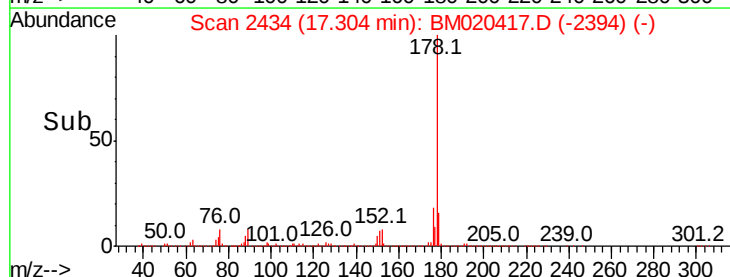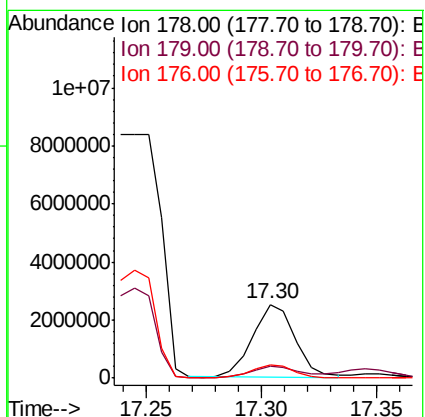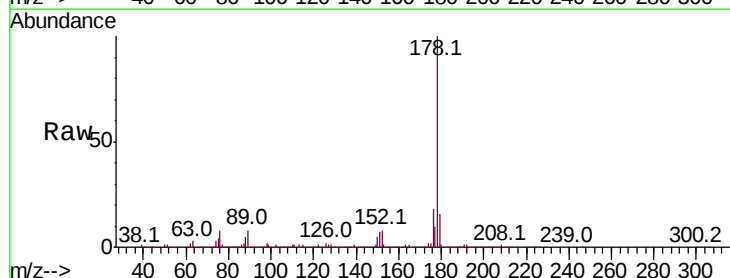

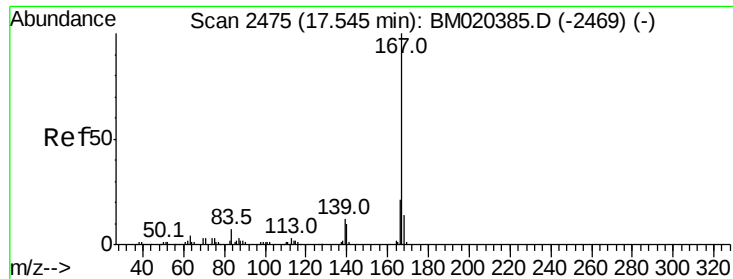

#74

Carbazole

Concen: 3.188 ng/ul

RT: 17.57 min Scan# 2479

Delta R.T. 0.02 min

Lab File: BM020417.D

Acq: 19 May 2019 02:17

Instrument :

BNA_M

ClientSampleId :





Tot Ion:167 Resp: 63066

Ion Ratio Lower Upper

167 100

166 33.8 16.6 24.8#

139 24.7 9.8 14.8#

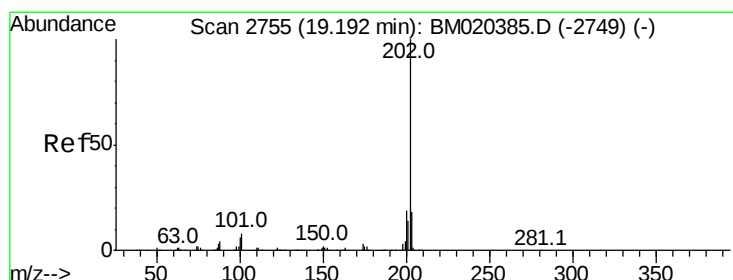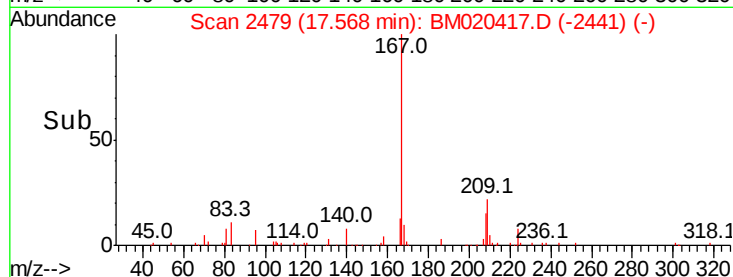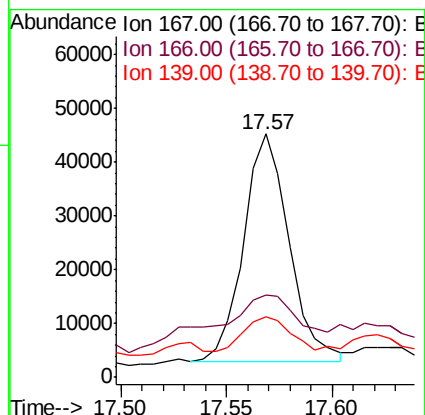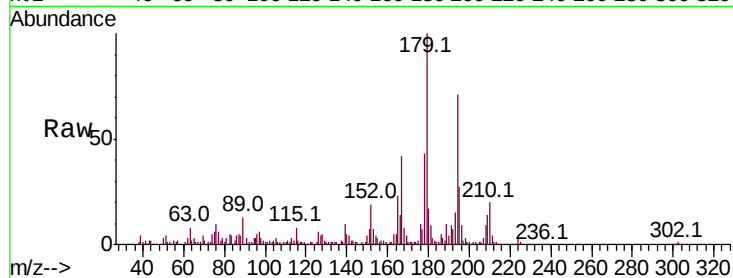

#76

Fluoranthene

Concen: 280.172 ng/ul

RT: 19.23 min Scan# 2762

Delta R.T. 0.04 min

Lab File: BM020417.D

Acq: 19 May 2019 02:17




Tgt Ion:202 Resp: 8108459


Ion Ratio Lower Upper

202 100

101 8.7 6.4 9.6

100 6.9 5.2 7.8

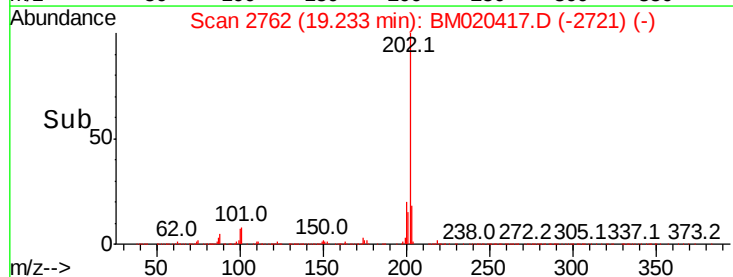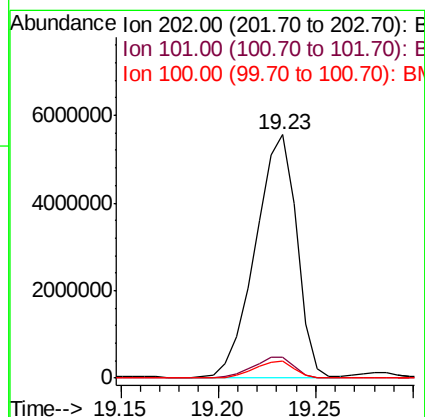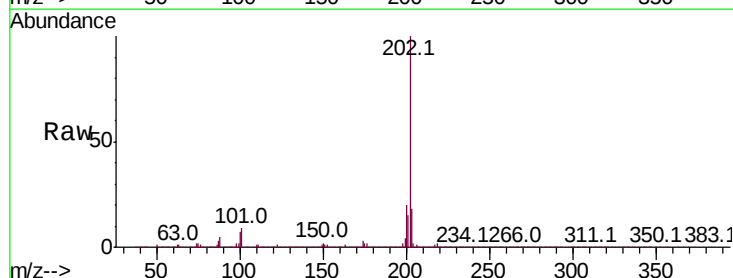



#79

Pvrene

Concen: 11.062 ng/ul

RT: 19.49 min Scan# 2806

Delta R.T. -0.06 min

Lab File: BM020417.D

Acq: 19 May 2019 02:17

Instrument :

BNA_M

ClientSampleId :


Tot Ion:202 Resp: 334559

Ion Ratio Lower Upper

202 100

101 10.2 7.1 10.7




100 6.8 5.9 8.9

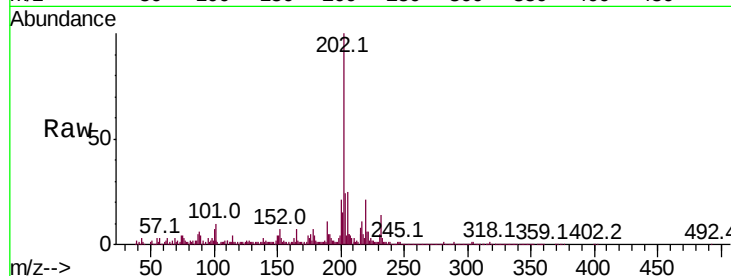

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

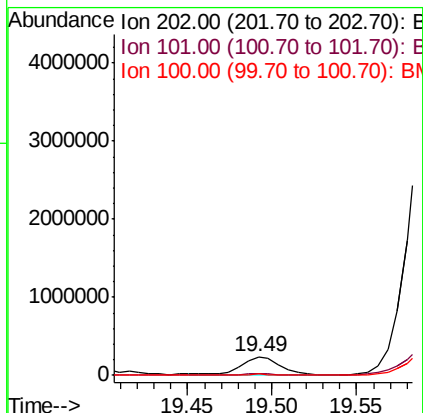

#82

Benzo(a)anthracene

Concen: 136.966 ng/ul

RT: 21.39 min Scan# 3128

Delta R.T. 0.08 min

Lab File: BM020417.D

Acq: 19 May 2019 02:17


Tgt Ion:228 Resp: 4153736

Ion Ratio Lower Upper

228 100

229 20.6 15.8 23.8



226 30.3 20.6 30.8




Abundance Ion 228.00 (227.70 to 228.70): E

Ion 229.00 (228.70 to 229.70): E

Ion 226.00 (225.70 to 226.70): E



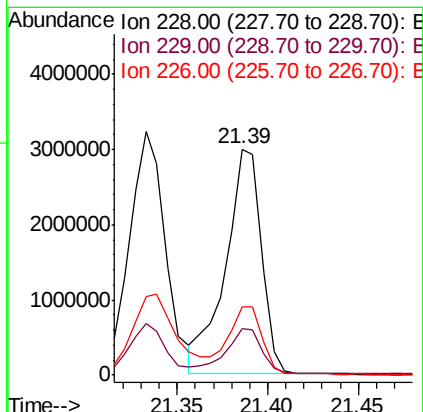



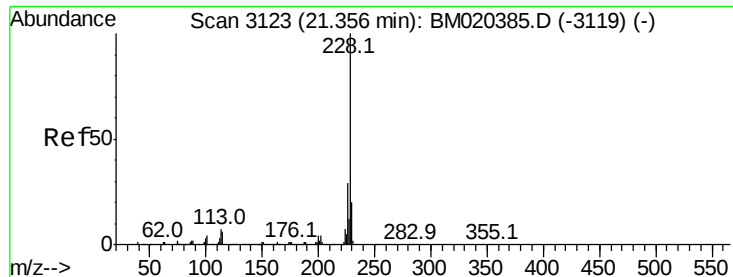

#84
Chrysene
Concen: 143.322 ng/ul
RT: 21.39 min Scan# 3128
Delta R.T. 0.03 min
Lab File: BM020417.D
Acq: 19 May 2019 02:17




Instrument :
BNA_M
ClientSampleId :


Tot Ion:228 Resp: 4153736
Ion Ratio Lower Upper
228 100
226 30.3 22.2 33.4
229 20.6 15.4 23.2

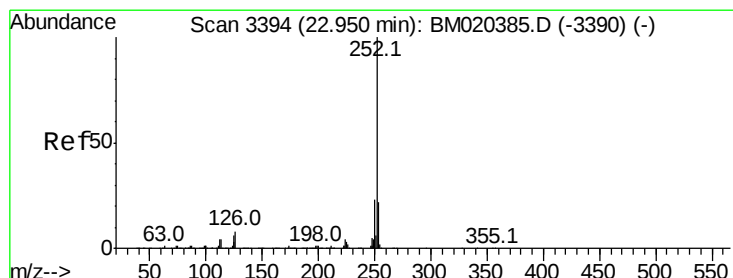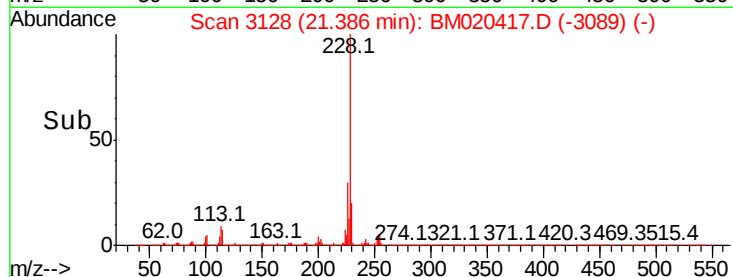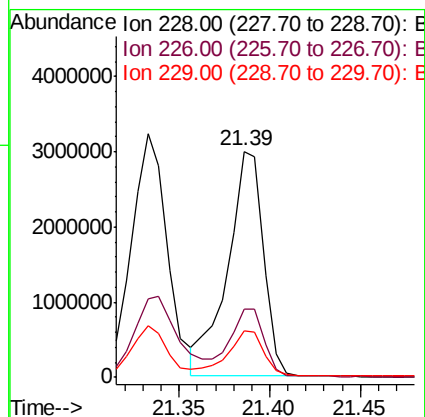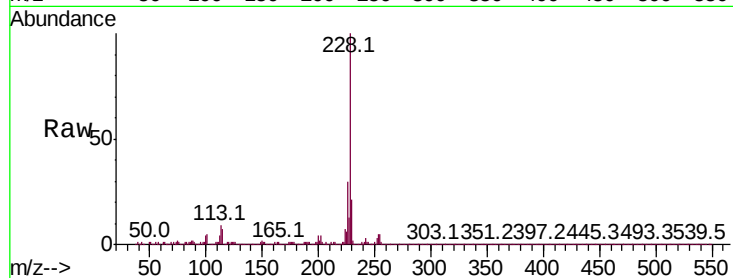

#88
Benzo(k)fluoranthene
Concen: 73.326 ng/ul
RT: 22.95 min Scan# 3394
Delta R.T. 0.00 min
Lab File: BM020417.D
Acq: 19 May 2019 02:17

Tgt Ion:252 Resp: 3039394
Ion Ratio Lower Upper
252 100
253 22.9 17.6 26.4
125 7.5 5.0 7.6

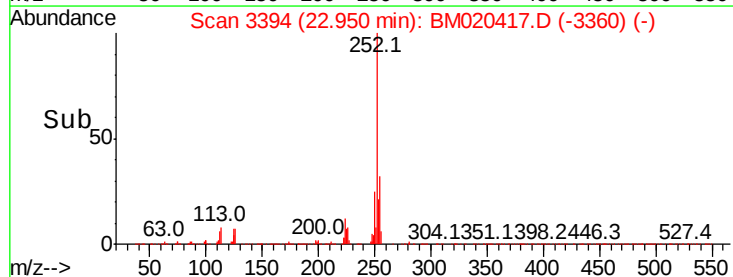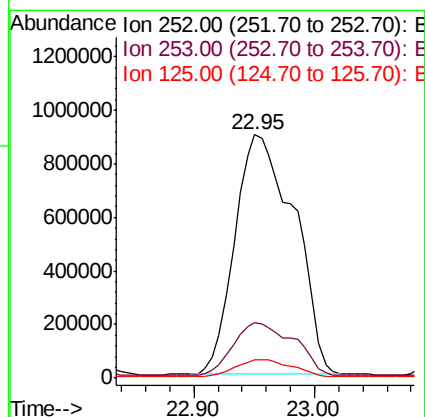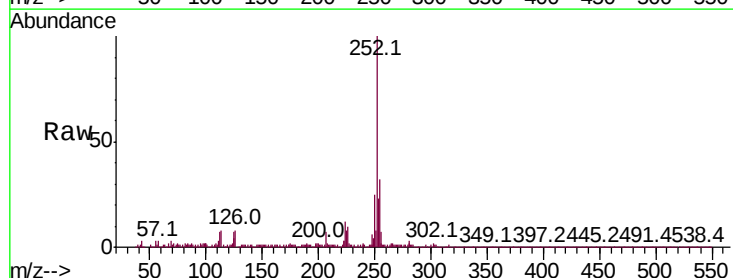

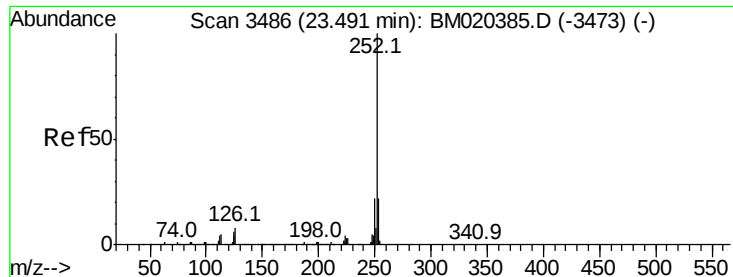

#90

Benzo(a)pyrene

Concen: 35.305 ng/ul

RT: 23.54 min Scan# 3494

Delta R.T. 0.05 min

Lab File: BM020417.D

Acq: 19 May 2019 02:17

Instrument :

BNA_M

ClientSampleId :


Tot Ion:252 Resp: 1402103

Ion Ratio Lower Upper

252 100

253 22.6 17.4 26.2




125 7.0 5.4 8.2

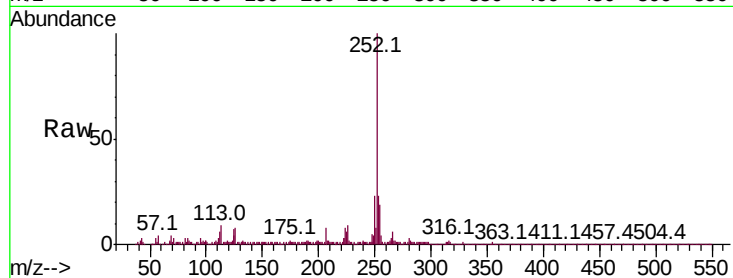

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

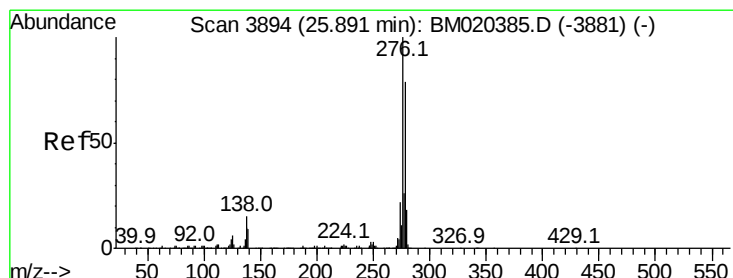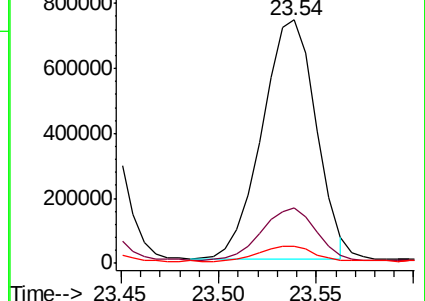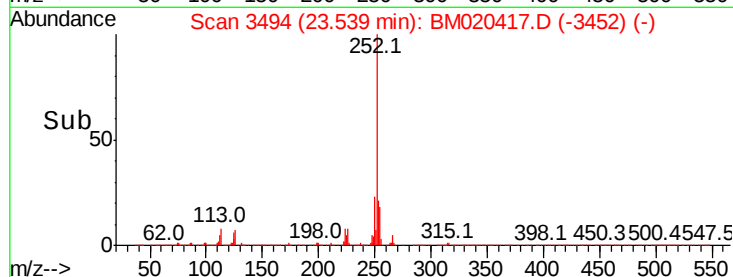

#91

Indeno(1,2,3-cd)pyrene

Concen: 2.929 ng/ul

RT: 25.71 min Scan# 3863

Delta R.T. -0.18 min

Lab File: BM020417.D

Acq: 19 May 2019 02:17


Tgt Ion:276 Resp: 132552

Ion Ratio Lower Upper

276 100

138 13.4 12.3 18.5

277 29.8 20.0 30.0

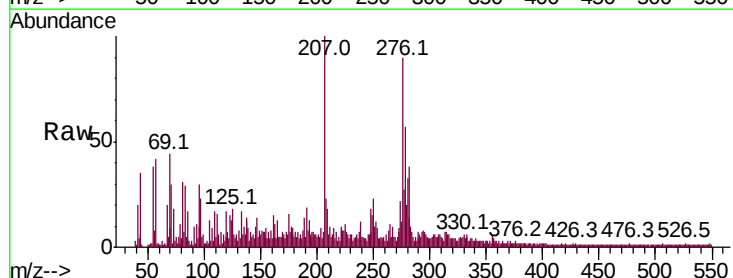

Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

