
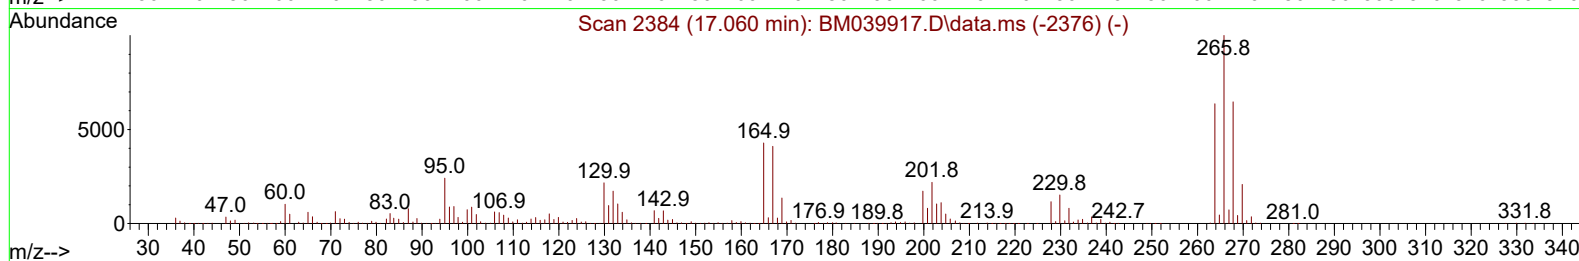
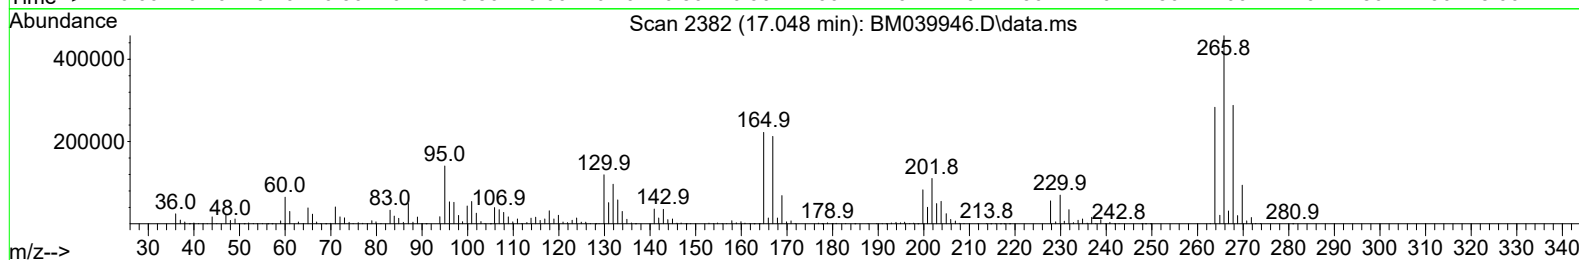


Quant Time: May 19 06:14:46 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM051223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 18 15:26:41 2023
Response via : Initial Calibration

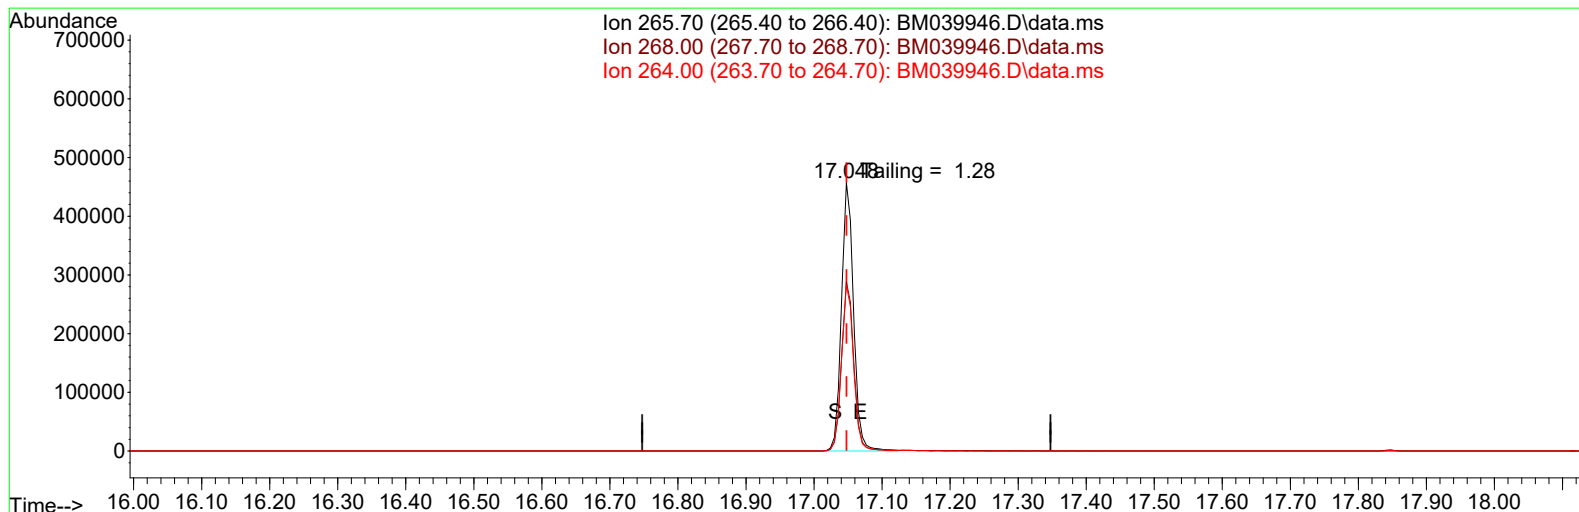

TIC: BM039946.D\data.ms

(70) Pentachlorophenol (C)




17.048min (-0.000) 0.00 ng

response **566241**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.70	63.03
264.00	63.70	61.94
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051823\
Data File : BM039946.D
Acq On : 18 May 2023 10:48
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 19 06:14:46 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM051223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 18 15:26:41 2023
Response via : Initial Calibration

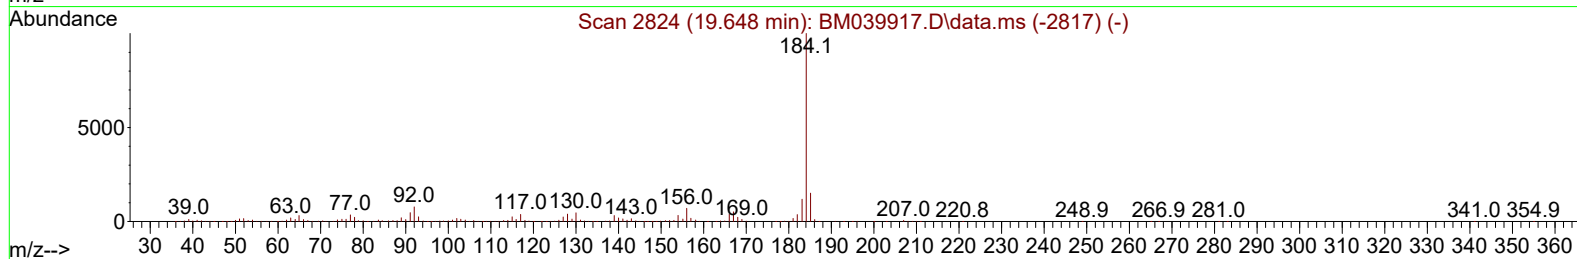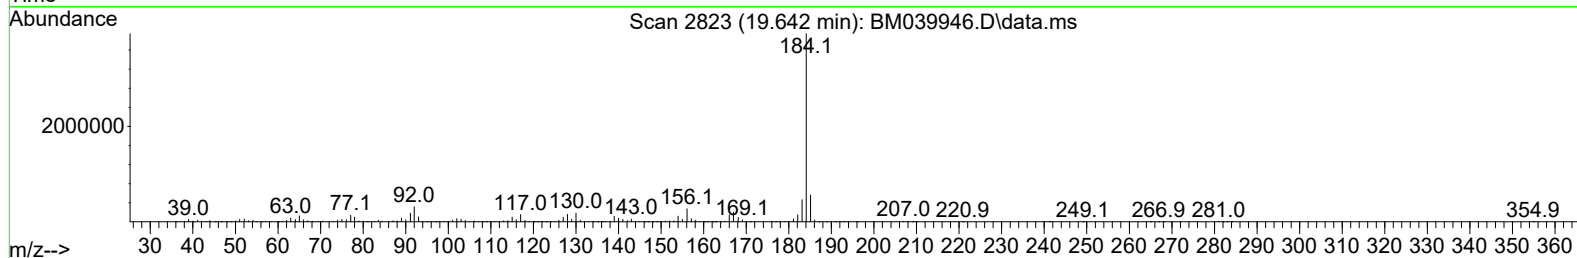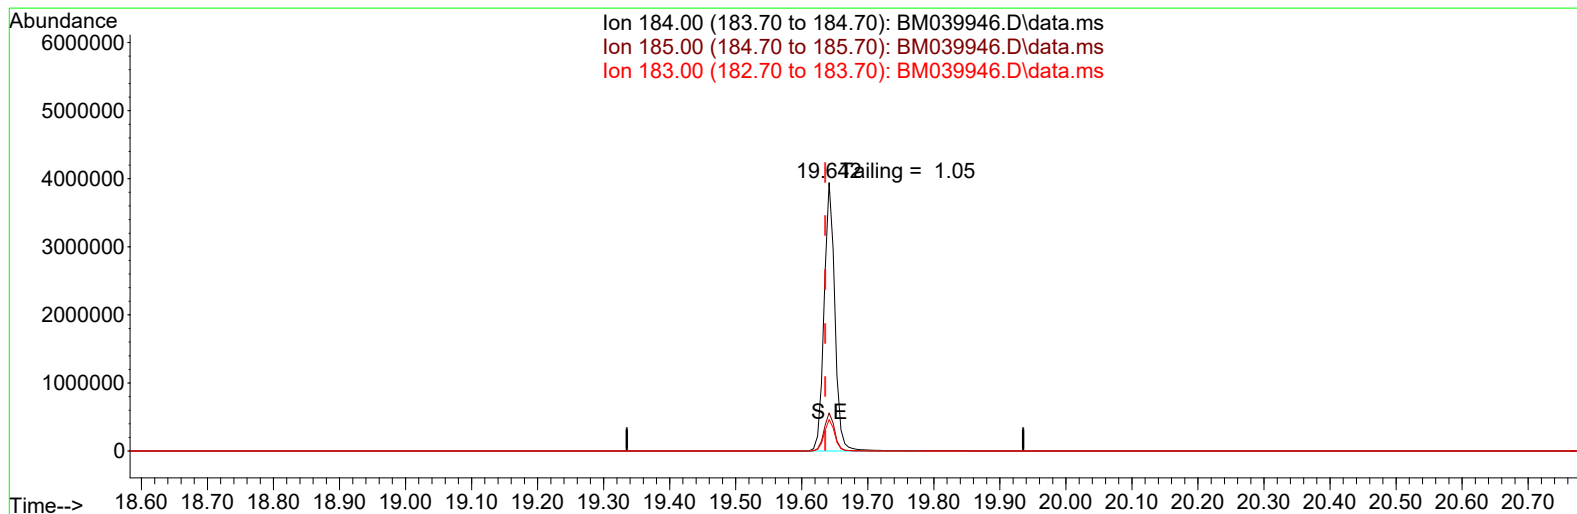

TIC: BM039946.D\data.ms

(77) Benzidine**19.642min (+ 0.006) 4092190.65 ng****response 4457716**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	14.19
183.00	11.90	11.72
0.00	0.00	0.00