


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051823\
Data File : BM039946.D
Acq On : 18 May 2023 10:48
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM051223.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu May 18 15:26:41 2023

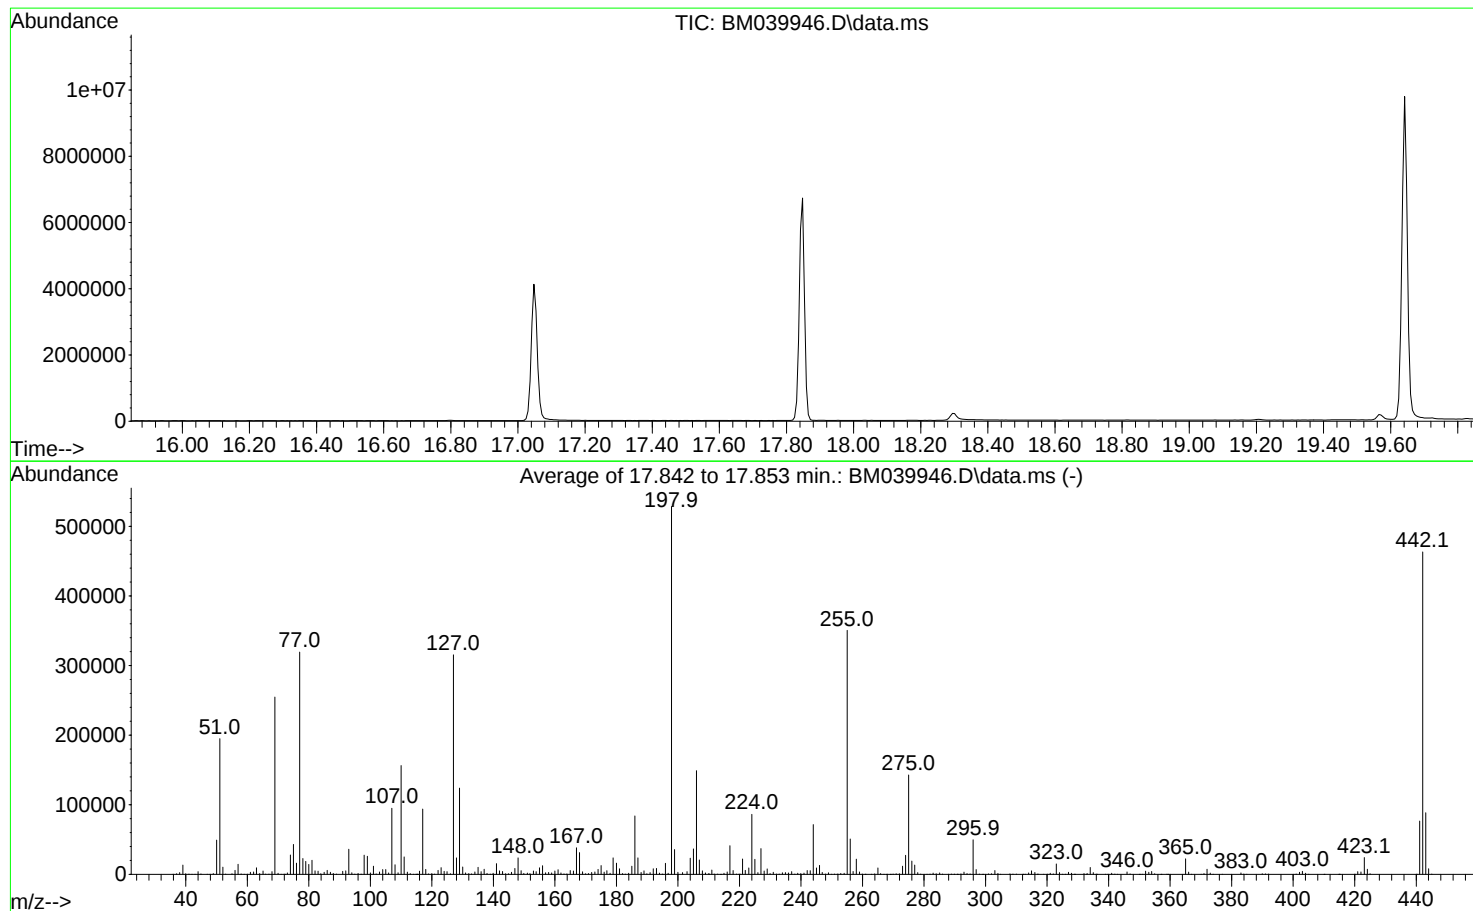

AutoFind: Scans 2517, 2518, 2519; Background Corrected with Scan 2510

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.9	195029	PASS
68	69	0.00	2	1.6	3962	PASS
69	198	0.00	100	48.2	254760	PASS
70	69	0.00	2	0.6	1557	PASS
127	198	10	80	59.7	315541	PASS
197	198	0.00	2	0.3	1547	PASS
198	198	100	100	100.0	528576	PASS
199	198	5	9	6.8	35728	PASS
275	198	10	60	27.0	142709	PASS
365	198	1	100	4.2	22408	PASS
441	198	0.01	100	14.5	76621	PASS
442	442	50	100	100.0	463317	PASS
443	442	15	24	19.1	88520	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/18/2023	BNA_M	<u>BM039946.D</u>
Compound Name	Response	Retention Time
DDT	1926197	20.877
DDD	13233	20.489
DDE	472	19.924
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
13705	1939902	0.71

Instrument :
BNA_M
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051823\
 Data File : BM039946.D
 Acq On : 18 May 2023 10:48
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: May 19 06:14:46 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM051223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu May 18 15:26:41 2023
 Response via : Initial Calibration

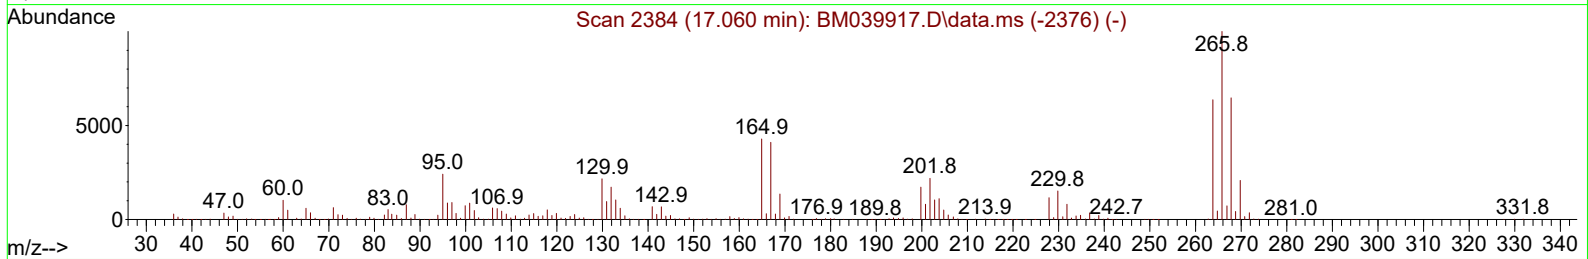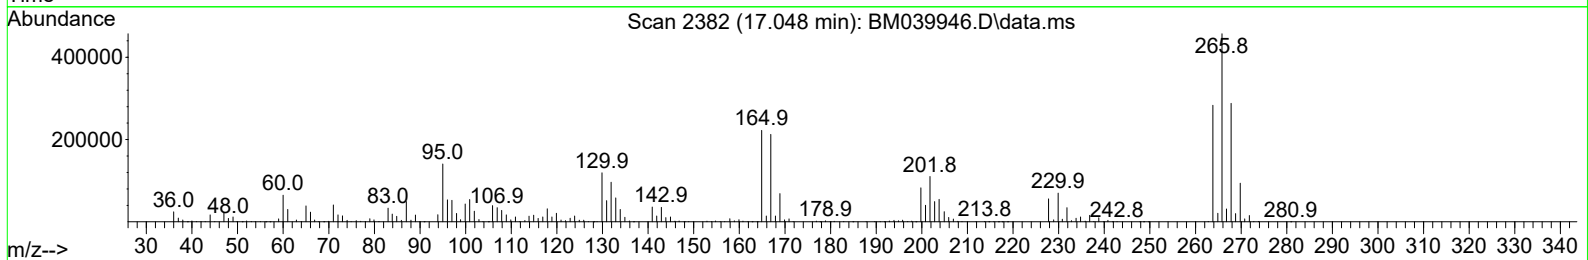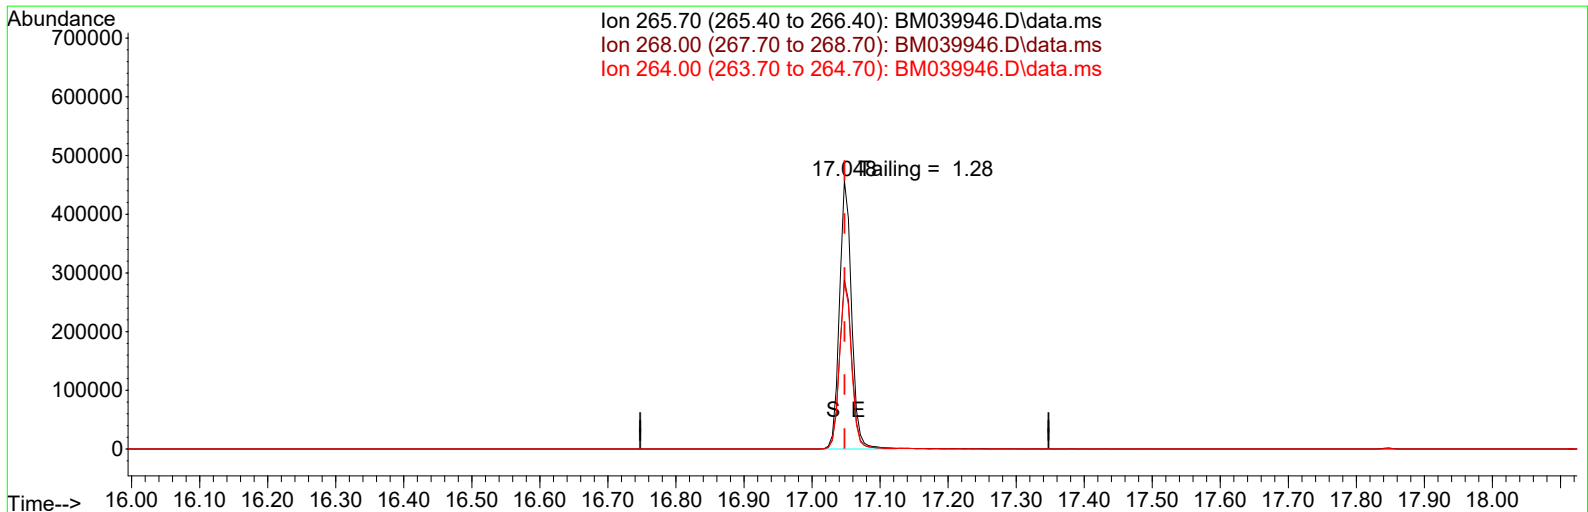

TIC: BM039946.D\data.ms

(70) Pentachlorophenol (C)

17.048min (-0.000) 0.00 ng




response 566241

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.70	63.03
264.00	63.70	61.94
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051823\
Data File : BM039946.D
Acq On : 18 May 2023 10:48
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: May 19 06:14:46 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM051223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 18 15:26:41 2023
Response via : Initial Calibration

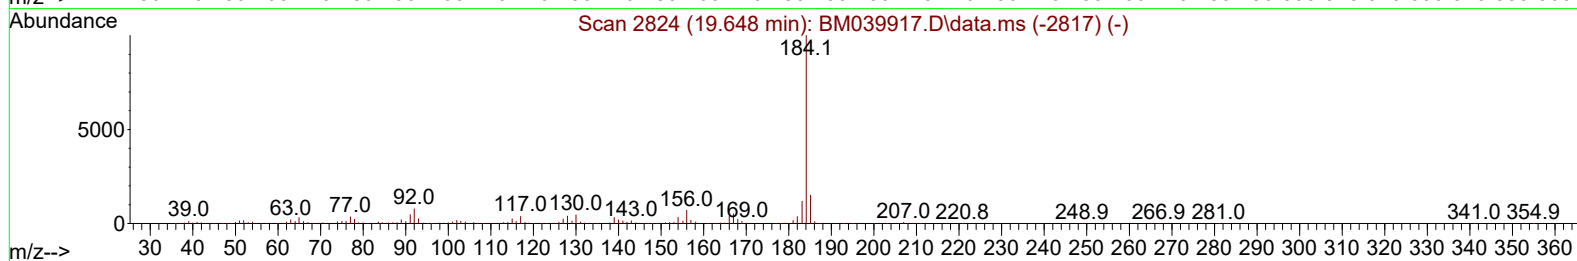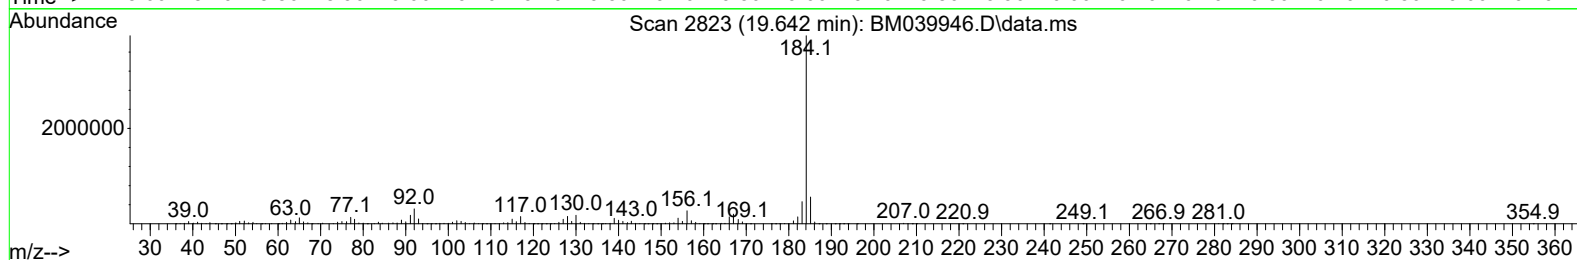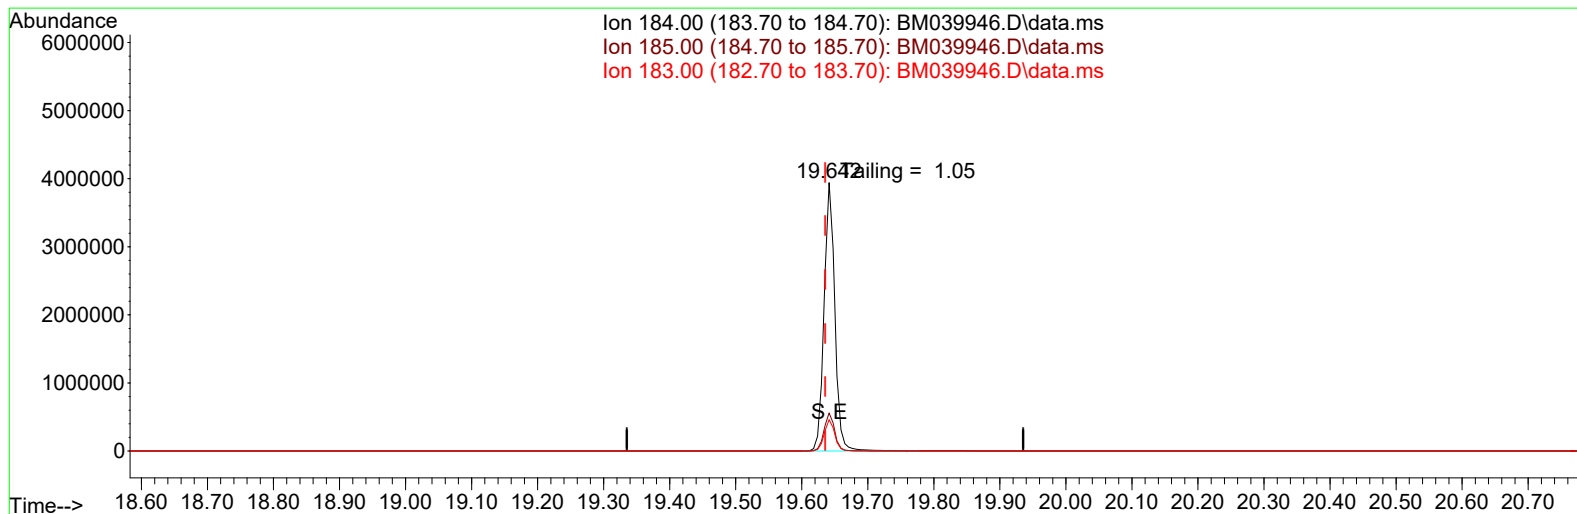

TIC: BM039946.D\data.ms

(77) Benzidine

19.642min (+ 0.006) 4092190.65 ng

response 4457716

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	14.19
183.00	11.90	11.72
0.00	0.00	0.00