

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052119\
 Data File : BM020470.D
 Acq On : 21 May 2019 21:20
 Operator : JU/SJ
 Sample : K2923-15
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4262

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051619MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.892	658	664	676	rVB	135717	255048	22.68%	2.152%
2	7.063	688	693	702	rBV	99398	173263	15.41%	1.462%
3	7.251	720	725	736	rBV	154550	258075	22.95%	2.178%
4	7.722	800	805	813	rBV	195641	315923	28.09%	2.666%
5	8.428	919	925	936	rBV	145028	252825	22.48%	2.133%
6	8.892	998	1004	1015	rVB	126892	222259	19.76%	1.876%
7	9.228	1058	1061	1065	rVB2	6748	7512	0.67%	0.063%
8	9.604	1119	1125	1134	rBV	97883	173961	15.47%	1.468%
9	9.928	1178	1180	1183	rVB2	1605	1447	0.13%	0.012%
10	10.139	1210	1216	1227	rBV	148143	270272	24.03%	2.281%
11	10.516	1273	1280	1288	rBV	241886	419494	37.30%	3.540%
12	10.669	1300	1306	1316	rBV	90703	184498	16.41%	1.557%
13	10.933	1349	1351	1353	rBV2	1302	1643	0.15%	0.014%
14	11.598	1460	1464	1466	rBV3	1646	2530	0.22%	0.021%
15	11.904	1514	1516	1521	rVB3	1071	1297	0.12%	0.011%
16	12.063	1540	1543	1547	rVB	1559	1654	0.15%	0.014%
17	12.110	1547	1551	1552	rBV2	1095	1383	0.12%	0.012%
18	12.186	1563	1564	1568	rVB	1410	1428	0.13%	0.012%
19	12.404	1595	1601	1605	rBV3	1611	2484	0.22%	0.021%
20	13.510	1786	1789	1794	rBV2	998	1546	0.14%	0.013%
21	13.692	1819	1820	1824	rVB	1328	1139	0.10%	0.010%
22	13.786	1830	1836	1840	rBV	296197	420625	37.40%	3.549%
23	13.833	1840	1844	1851	rVB	105151	150535	13.39%	1.270%
24	14.069	1877	1884	1895	rBV	345200	503599	44.78%	4.250%
25	14.145	1895	1897	1900	rVB3	1223	1334	0.12%	0.011%
26	14.251	1906	1915	1922	rBV4	5282	9602	0.85%	0.081%
27	14.374	1929	1936	1944	rBV2	378559	571572	50.83%	4.823%
28	14.433	1944	1946	1951	rVB	4583	5500	0.49%	0.046%
29	14.527	1961	1962	1968	rVB2	825	1125	0.10%	0.009%
30	14.598	1968	1974	1988	rBV3	41669	106645	9.48%	0.900%
31	14.774	2003	2004	2008	rVV2	2525	3114	0.28%	0.026%
32	15.027	2044	2047	2052	rVB2	697	1227	0.11%	0.010%
33	15.151	2065	2068	2071	rBV2	1613	2265	0.20%	0.019%
34	15.204	2075	2077	2081	rBV2	2187	1841	0.16%	0.016%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052119\
 Data File : BM020470.D
 Acq On : 21 May 2019 21:20
 Operator : JU/SJ
 Sample : K2923-15
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4262

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051619MA.M
 Title : SVOA CALIBRATION

35	15.368	2099	2105	2112	rBV	432567	635368	56.50%	5.362%
36	15.421	2112	2114	2118	rVB2	5509	7532	0.67%	0.064%
37	15.510	2124	2129	2138	rBV	86867	125226	11.14%	1.057%
38	15.604	2141	2145	2150	rBV3	3006	4824	0.43%	0.041%
39	15.721	2162	2165	2167	rVV	1472	1419	0.13%	0.012%
40	15.874	2187	2191	2193	rBV2	1813	2395	0.21%	0.020%
41	16.086	2223	2227	2228	rBV2	2276	2491	0.22%	0.021%
42	16.486	2292	2295	2297	rBV2	1321	1472	0.13%	0.012%
43	16.786	2344	2346	2353	rBV3	1449	2166	0.19%	0.018%
44	16.862	2356	2359	2363	rVB2	2177	2884	0.26%	0.024%
45	16.915	2363	2368	2370	rBV3	1335	2197	0.20%	0.019%
46	16.945	2370	2373	2377	rVB2	1717	1866	0.17%	0.016%
47	17.127	2398	2404	2408	rVV2	519938	733859	65.26%	6.193%
48	17.168	2408	2411	2416	rVV	81985	110738	9.85%	0.934%
49	17.227	2416	2421	2439	rVV	487203	753897	67.04%	6.362%
50	17.474	2461	2463	2465	rBV2	1190	1435	0.13%	0.012%
51	17.545	2472	2475	2479	rBV2	2304	3758	0.33%	0.032%
52	17.604	2483	2485	2488	rVB3	3235	2699	0.24%	0.023%
53	17.639	2488	2491	2492	rBV	1254	1351	0.12%	0.011%
54	17.815	2517	2521	2524	rBV4	1959	3575	0.32%	0.030%
55	17.862	2524	2529	2530	rVV2	1391	1623	0.14%	0.014%
56	17.886	2530	2533	2535	rVB2	1066	1366	0.12%	0.012%
57	17.974	2546	2548	2549	rBV2	1982	1601	0.14%	0.014%
58	18.004	2549	2553	2558	rVV	41873	65065	5.79%	0.549%
59	18.051	2558	2561	2565	rVB3	10411	17063	1.52%	0.144%
60	18.133	2571	2575	2577	rBV3	3402	3342	0.30%	0.028%
61	18.151	2577	2578	2581	rVB3	3083	1955	0.17%	0.016%
62	18.204	2581	2587	2590	rBV3	12939	25457	2.26%	0.215%
63	18.239	2590	2593	2600	rVB3	8423	13073	1.16%	0.110%
64	18.292	2600	2602	2608	rBV4	3679	6115	0.54%	0.052%
65	18.356	2612	2613	2616	rBV2	1813	1734	0.15%	0.015%
66	18.386	2616	2618	2622	rVB3	2564	2420	0.22%	0.020%
67	18.427	2622	2625	2627	rBV2	2194	2238	0.20%	0.019%
68	18.480	2632	2634	2635	rBV2	1489	1441	0.13%	0.012%
69	18.509	2635	2639	2644	rVB3	5823	9437	0.84%	0.080%
70	18.556	2644	2647	2652	rBV5	6551	11453	1.02%	0.097%
71	18.615	2655	2657	2660	rBV4	1492	1837	0.16%	0.016%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052119\
 Data File : BM020470.D
 Acq On : 21 May 2019 21:20
 Operator : JU/SJ
 Sample : K2923-15
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4262

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051619MA.M
 Title : SVOA CALIBRATION

72	18.715	2672	2674	2677	rVB3	2121	1908	0.17%	0.016%
73	18.751	2677	2680	2683	rBV4	3482	5120	0.46%	0.043%
74	18.803	2686	2689	2690	rBV3	3124	2272	0.20%	0.019%
75	18.921	2705	2709	2716	rBV7	7519	16001	1.42%	0.135%
76	18.968	2716	2717	2719	rVV2	2407	1975	0.18%	0.017%
77	18.992	2719	2721	2723	rVB3	2686	2289	0.20%	0.019%
78	19.051	2729	2731	2732	rBV2	2653	1404	0.12%	0.012%
79	19.080	2732	2736	2739	rVV5	5044	5746	0.51%	0.048%
80	19.162	2743	2750	2751	rBV3	9457	14911	1.33%	0.126%
81	19.192	2751	2755	2763	rVB	130214	179872	16.00%	1.518%
82	19.251	2763	2765	2767	rBV3	4517	3168	0.28%	0.027%
83	19.292	2769	2772	2777	rVV6	13386	18647	1.66%	0.157%
84	19.345	2777	2781	2784	rVV5	3664	4885	0.43%	0.041%
85	19.527	2806	2812	2816	rBV	795007	1124551	100.00%	9.489%
86	19.627	2826	2829	2833	rVB5	8419	11008	0.98%	0.093%
87	19.739	2846	2848	2850	rBV2	4795	3970	0.35%	0.034%
88	19.874	2869	2871	2872	rBV2	5252	4228	0.38%	0.036%
89	20.050	2898	2901	2905	rVB5	23420	31333	2.79%	0.264%
90	20.150	2915	2918	2923	rBV3	15457	21159	1.88%	0.179%
91	20.621	2994	2998	3002	rVB	55316	63538	5.65%	0.536%
92	20.962	3051	3056	3060	rBV5	39611	70348	6.26%	0.594%
93	21.015	3061	3065	3070	rBV6	67168	101295	9.01%	0.855%
94	21.321	3111	3117	3121	rBV	772650	1107266	98.46%	9.344%
95	23.444	3472	3478	3484	rBV2	602092	1086489	96.62%	9.168%
96	23.591	3497	3503	3519	rVB2	534159	1070103	95.16%	9.030%


Sum of corrected areas: 11850523

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052119\
Data File : BM020470.D
Acq On : 21 May 2019 21:20
Operator : JU/SJ
Sample : K2923-15
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4262

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051619MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

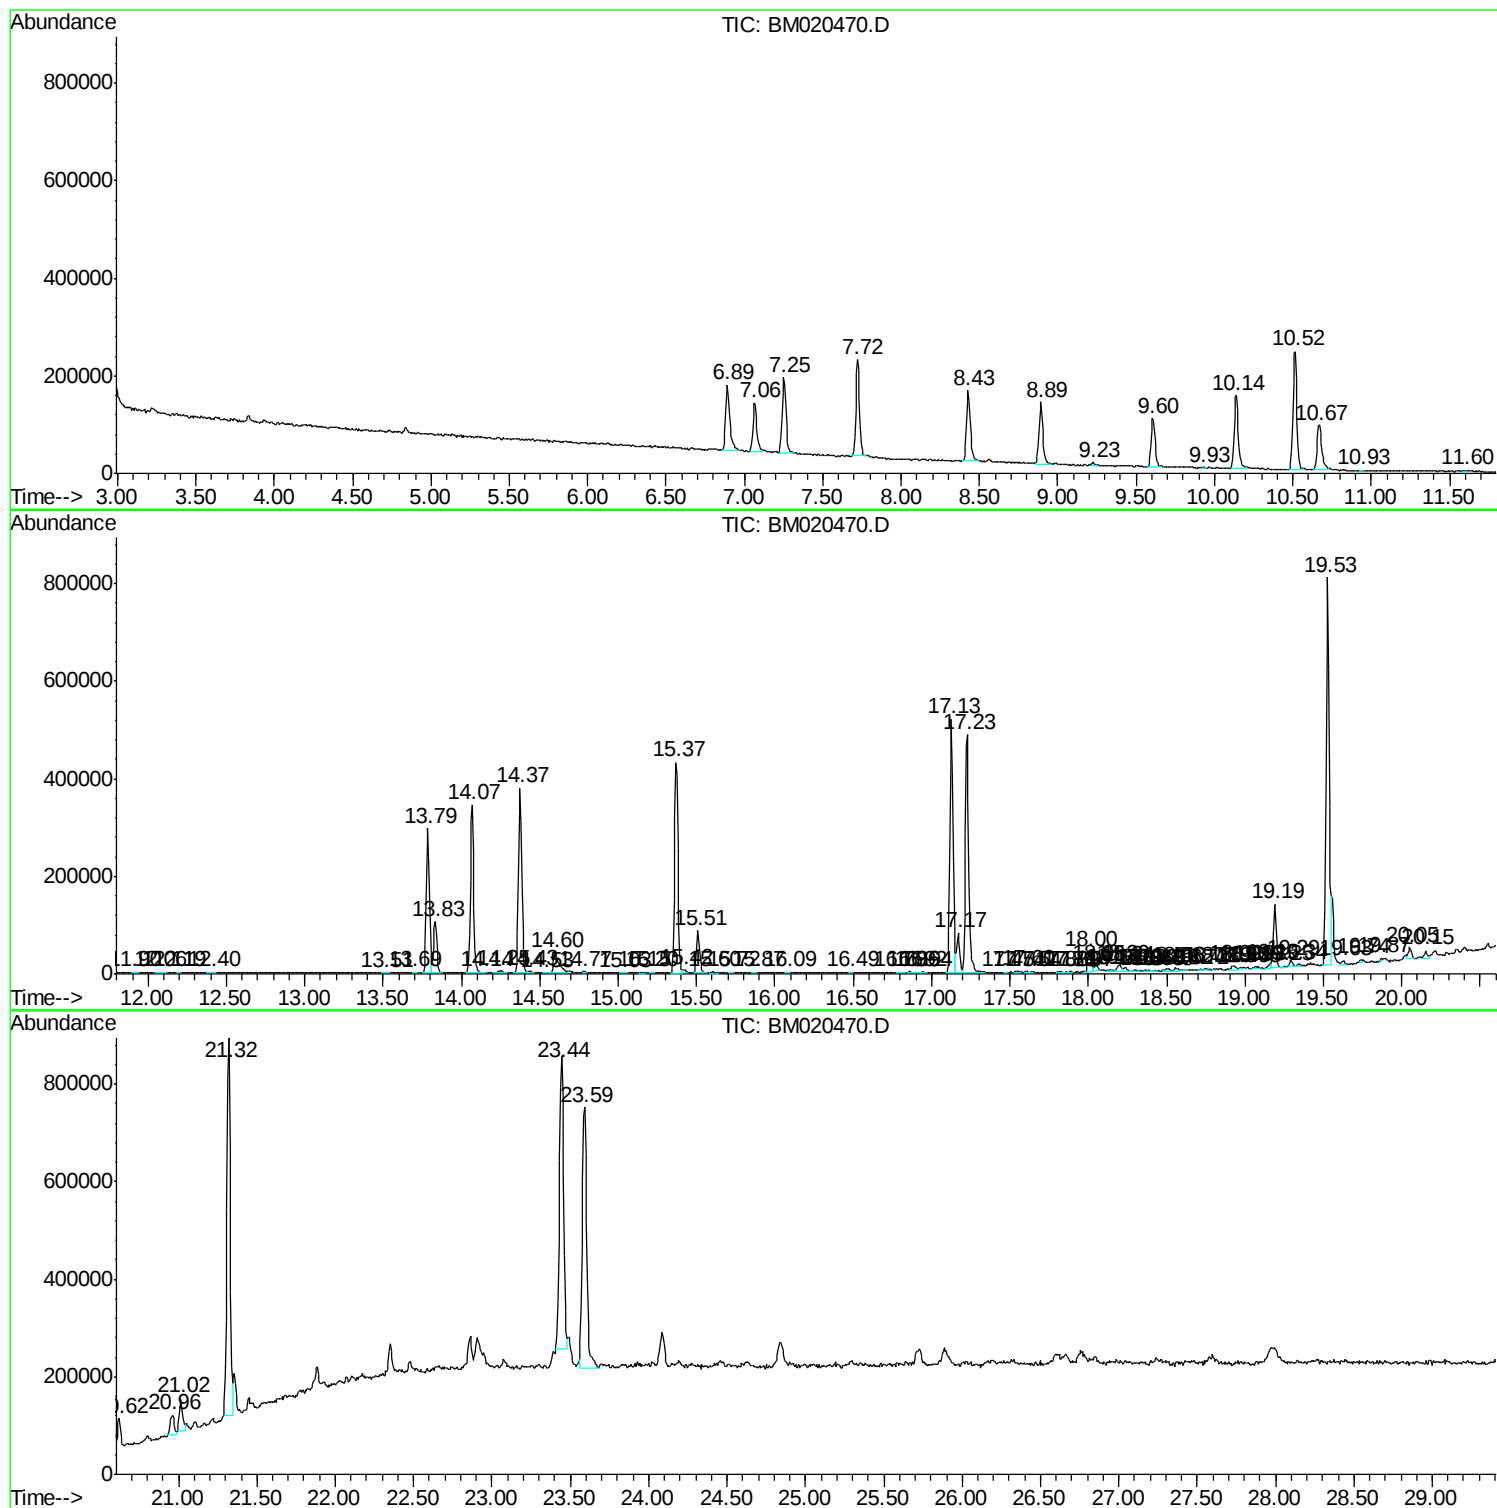

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM052119\
Data File : BM020470.D
Acq On : 21 May 2019 21:20
Operator : JU/SJ
Sample : K2923-15
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4262

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051619MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM052119\
Data File : BM020470.D
Acq On : 21 May 2019 21:20
Operator : JU/SJ
Sample : K2923-15
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4262

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051619MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc