

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052119\
 Data File : BM020486.D
 Acq On : 22 May 2019 07:06
 Operator : JU/SJ
 Sample : K2923-10DL 5X
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4257DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051619MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.910	663	667	674	rVB2	16311	29261	3.00%	0.889%
2	7.263	723	727	734	rVB3	21683	38909	4.00%	1.182%
3	7.722	800	805	813	rVB	234473	390272	40.08%	11.854%
4	8.439	923	927	935	rBV2	17415	32059	3.29%	0.974%
5	8.904	1001	1006	1010	rBV2	12461	20750	2.13%	0.630%
6	9.610	1122	1126	1133	rVB4	11891	22139	2.27%	0.672%
7	10.151	1213	1218	1228	rBV5	17475	33201	3.41%	1.008%
8	10.280	1238	1240	1242	rBV2	1416	1066	0.11%	0.032%
9	10.516	1274	1280	1291	rVB	311294	520179	53.41%	15.800%
10	13.074	1711	1715	1720	rBV2	871	1413	0.15%	0.043%
11	13.580	1797	1801	1804	rVB2	715	1102	0.11%	0.033%
12	13.786	1829	1836	1841	rBV	44461	62849	6.45%	1.909%
13	13.833	1841	1844	1851	rVB	19648	27233	2.80%	0.827%
14	14.074	1878	1885	1890	rBV	50477	77950	8.00%	2.368%
15	14.380	1930	1937	1945	rBV2	449143	709194	72.82%	21.541%
16	14.668	1983	1986	1989	rBV2	2763	3565	0.37%	0.108%
17	14.798	2007	2008	2010	rVB	2349	1378	0.14%	0.042%
18	14.857	2015	2018	2019	rBV2	1214	1304	0.13%	0.040%
19	14.915	2027	2028	2032	rVB2	1253	1283	0.13%	0.039%
20	15.039	2048	2049	2051	rBV2	1316	1088	0.11%	0.033%
21	15.315	2095	2096	2100	rBV2	951	1364	0.14%	0.041%
22	15.380	2101	2107	2112	rBV	68393	102334	10.51%	3.108%
23	15.662	2153	2155	2160	rVB2	798	1156	0.12%	0.035%
24	15.862	2186	2189	2192	rBV2	1013	1399	0.14%	0.042%
25	15.898	2192	2195	2200	rBV4	1407	2258	0.23%	0.069%
26	16.033	2215	2218	2219	rVB2	1620	1523	0.16%	0.046%
27	16.068	2222	2224	2226	rVV2	1341	1249	0.13%	0.038%
28	16.121	2230	2233	2237	rVV3	1154	1297	0.13%	0.039%
29	16.168	2240	2241	2244	rVB	1850	1135	0.12%	0.034%
30	16.221	2248	2250	2252	rBV	1840	1410	0.14%	0.043%
31	16.262	2254	2257	2258	rBV	1349	1206	0.12%	0.037%
32	16.380	2274	2277	2279	rBV3	1764	1541	0.16%	0.047%
33	16.427	2283	2285	2287	rVB2	2186	1556	0.16%	0.047%
34	16.445	2287	2288	2291	rVB2	1637	1396	0.14%	0.042%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052119\
 Data File : BM020486.D
 Acq On : 22 May 2019 07:06
 Operator : JU/SJ
 Sample : K2923-10DL 5X
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4257DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051619MA.M
 Title : SVOA CALIBRATION

35	16.474	2291	2293	2295	rBV3	1946	1880	0.19%	0.057%
36	16.504	2295	2298	2299	rBV2	1793	1510	0.16%	0.046%
37	16.515	2299	2300	2305	rBV3	1682	2298	0.24%	0.070%
38	16.651	2321	2323	2325	rVB2	2761	1790	0.18%	0.054%
39	16.739	2335	2338	2339	rBV3	2058	1683	0.17%	0.051%
40	16.768	2341	2343	2346	rBV4	2414	2533	0.26%	0.077%
41	16.815	2346	2351	2355	rVB5	3092	5996	0.62%	0.182%
42	16.862	2355	2359	2361	rBV5	3925	5396	0.55%	0.164%
43	16.904	2363	2366	2368	rBV4	2769	3272	0.34%	0.099%
44	16.974	2376	2378	2379	rBV3	1932	1172	0.12%	0.036%
45	17.009	2382	2384	2387	rBV4	2666	2424	0.25%	0.074%
46	17.051	2387	2391	2393	rVB4	1871	2429	0.25%	0.074%
47	17.151	2401	2408	2420	rBV	539243	973848	100.00%	29.580%
48	17.251	2420	2425	2436	rVV2	72066	148055	15.20%	4.497%
49	17.321	2436	2437	2439	rVV2	3244	2441	0.25%	0.074%
50	17.345	2439	2441	2445	rVB5	2678	3043	0.31%	0.092%
51	17.503	2466	2468	2471	rBV4	2294	2348	0.24%	0.071%
52	17.615	2485	2487	2488	rVB2	4099	2045	0.21%	0.062%
53	17.698	2498	2501	2503	rBV4	3851	4209	0.43%	0.128%
54	17.786	2514	2516	2517	rBV2	3066	1790	0.18%	0.054%
55	17.803	2517	2519	2522	rVB4	4382	3196	0.33%	0.097%
56	17.921	2537	2539	2540	rVB2	4342	2617	0.27%	0.079%
57	18.233	2590	2592	2595	rBV3	7184	7729	0.79%	0.235%
58	18.745	2677	2679	2680	rBV2	12332	11535	1.18%	0.350%


Sum of corrected areas: 3292258

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052119\
Data File : BM020486.D
Acq On : 22 May 2019 07:06
Operator : JU/SJ
Sample : K2923-10DL 5X
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4257DL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051619MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

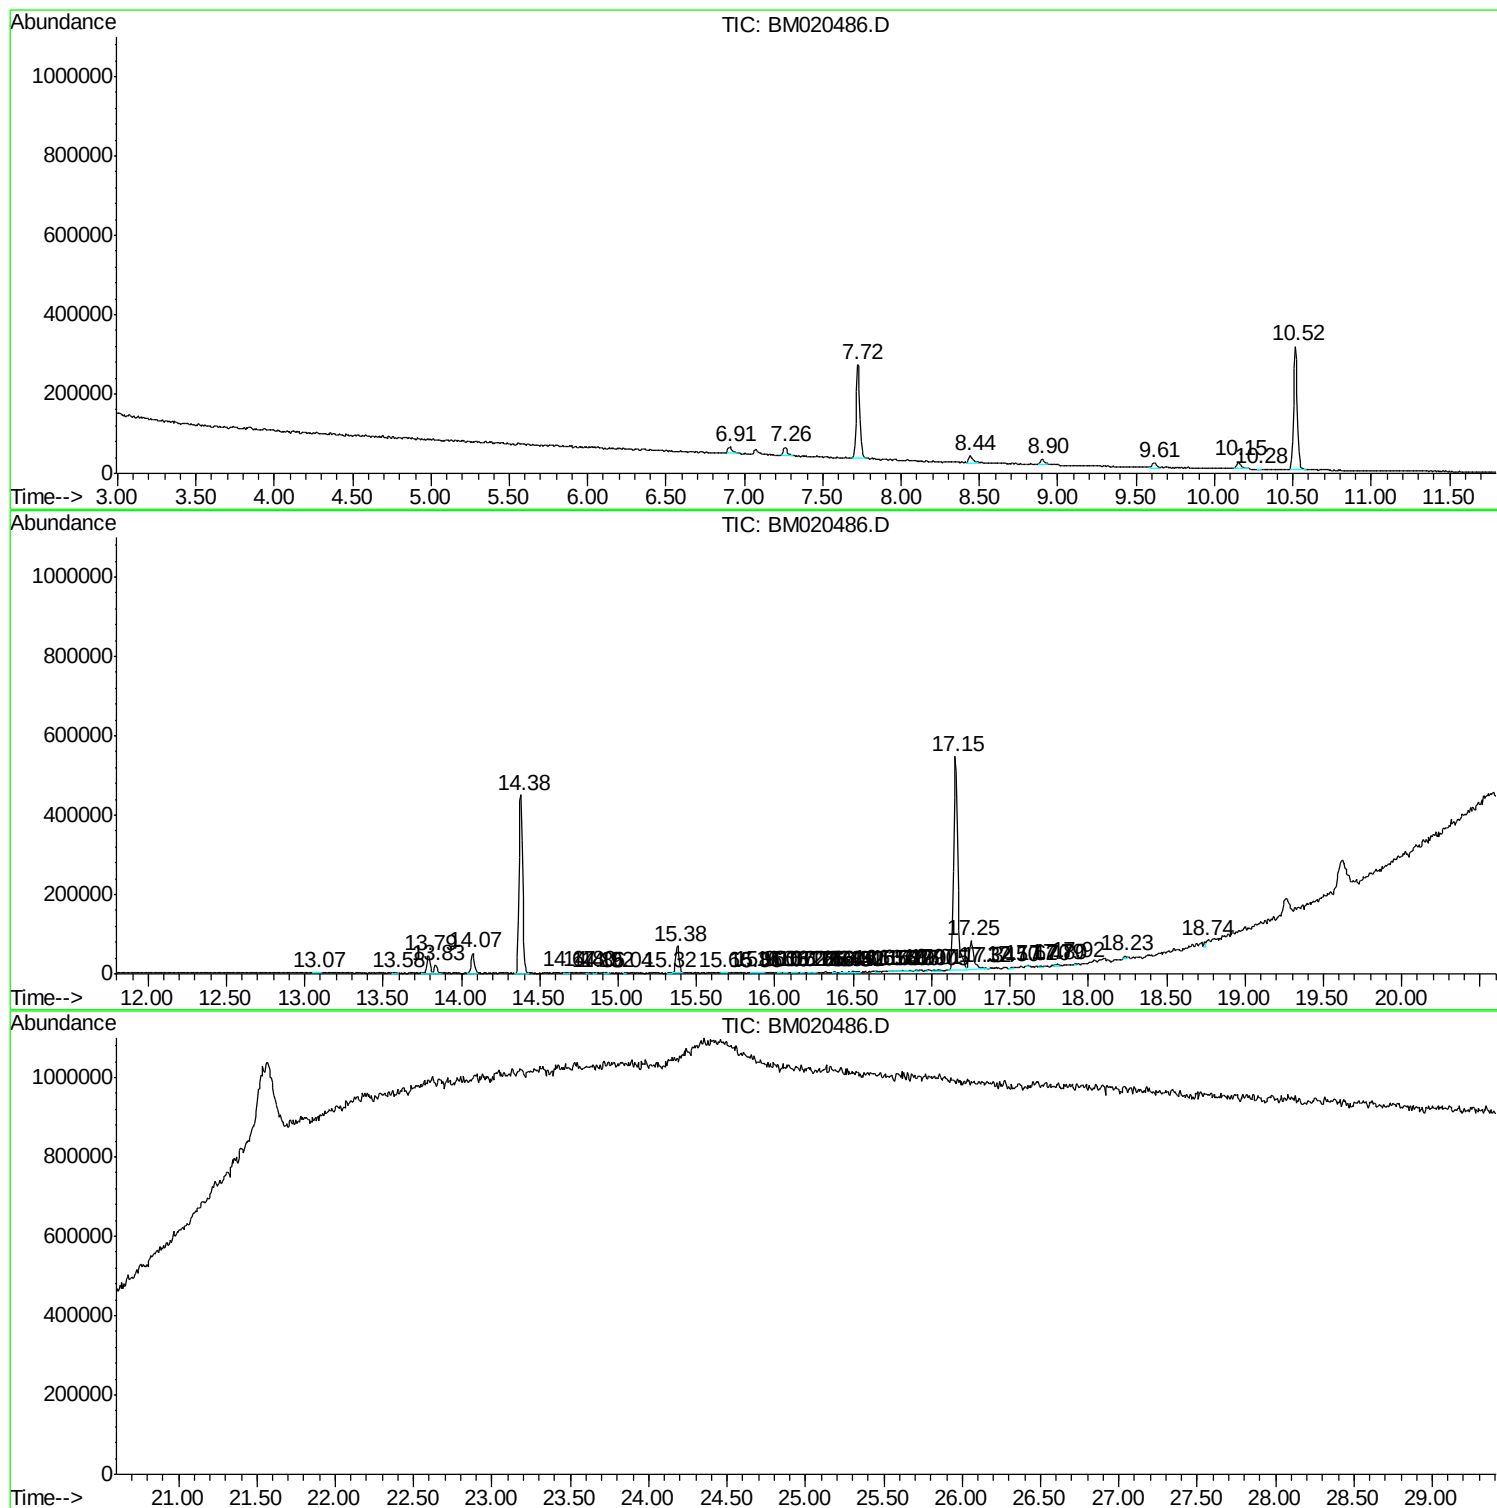

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM052119\
Data File : BM020486.D
Acq On : 22 May 2019 07:06
Operator : JU/SJ
Sample : K2923-10DL 5X
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4257DL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051619MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM052119\
Data File : BM020486.D
Acq On : 22 May 2019 07:06
Operator : JU/SJ
Sample : K2923-10DL 5X
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4257DL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051619MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc