

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052119\
 Data File : BM020491.D
 Acq On : 22 May 2019 10:08
 Operator : JU/SJ
 Sample : K2923-22
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A42F3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051619MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.911	661	667	680	rBV	97809	228764	7.68%	1.872%
2	7.069	689	694	705	rBV	87587	160620	5.39%	1.314%
3	7.263	721	727	738	rBV	127655	237429	7.97%	1.942%
4	7.728	800	806	822	rVB	247694	451825	15.17%	3.697%
5	8.440	922	927	937	rBV2	118195	258821	8.69%	2.118%
6	8.899	999	1005	1016	rVB	112545	218491	7.33%	1.788%
7	9.616	1121	1127	1137	rVB	97104	189602	6.36%	1.551%
8	10.157	1212	1219	1240	rBV	132774	317637	10.66%	2.599%
9	10.522	1274	1281	1288	rBV	310263	565601	18.98%	4.627%
10	10.681	1302	1308	1318	rBV3	26407	57298	1.92%	0.469%
11	12.110	1549	1551	1556	rVB3	2109	3457	0.12%	0.028%
12	12.187	1559	1564	1571	rVB2	5634	10581	0.36%	0.087%
13	12.410	1598	1602	1607	rVB	8406	11924	0.40%	0.098%
14	13.545	1789	1795	1796	rBV3	6363	10086	0.34%	0.083%
15	13.698	1815	1821	1826	rBV3	16992	30802	1.03%	0.252%
16	13.751	1826	1830	1832	rVV	11006	12550	0.42%	0.103%
17	13.792	1832	1837	1842	rVV	303438	479993	16.11%	3.927%
18	13.839	1842	1845	1857	rVB	122734	185150	6.21%	1.515%
19	13.934	1857	1861	1865	rBV2	9037	14733	0.49%	0.121%
20	14.081	1879	1886	1904	rBV2	342624	702491	23.58%	5.747%
21	14.251	1910	1915	1920	rVB4	3553	5746	0.19%	0.047%
22	14.387	1929	1938	1946	rBV2	449262	781265	26.22%	6.392%
23	14.451	1946	1949	1955	rVB2	14603	24123	0.81%	0.197%
24	14.534	1959	1963	1968	rBV2	1821	4259	0.14%	0.035%
25	14.675	1983	1987	1989	rBV3	2173	3037	0.10%	0.025%
26	14.787	2000	2006	2011	rBV3	39689	71318	2.39%	0.583%
27	14.863	2014	2019	2024	rBV6	18736	40639	1.36%	0.332%
28	14.998	2038	2042	2048	rVB5	15467	28032	0.94%	0.229%
29	15.057	2048	2052	2057	rVB2	9736	13582	0.46%	0.111%
30	15.157	2065	2069	2071	rBV4	7380	10813	0.36%	0.088%
31	15.210	2076	2078	2083	rVB3	8636	11231	0.38%	0.092%
32	15.269	2083	2088	2093	rBV2	6198	11672	0.39%	0.095%
33	15.316	2093	2096	2099	rVB3	3372	3368	0.11%	0.028%
34	15.392	2099	2109	2115	rBV	404276	774653	26.00%	6.338%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052119\
Data File : BM020491.D
Acq On : 22 May 2019 10:08
Operator : JU/SJ
Sample : K2923-22
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A42F3

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051619MA.M
Title : SVOA CALIBRATION

35	15.445	2115	2118	2128	rVB	67729	133443	4.48%	1.092%
36	15.534	2130	2133	2135	rBV3	4021	4177	0.14%	0.034%
37	15.610	2143	2146	2147	rBV3	5285	5073	0.17%	0.042%
38	15.663	2150	2155	2157	rBV4	5616	8710	0.29%	0.071%
39	15.739	2163	2168	2176	rBV2	27346	47710	1.60%	0.390%
40	15.898	2185	2195	2204	rBV2	32778	88634	2.97%	0.725%
41	15.975	2206	2208	2209	rBV2	5085	3799	0.13%	0.031%
42	16.086	2219	2227	2228	rBV5	7407	11153	0.37%	0.091%
43	16.257	2253	2256	2258	rBV3	3530	4152	0.14%	0.034%
44	16.333	2267	2269	2272	rBV3	4133	4331	0.15%	0.035%
45	16.463	2280	2291	2298	rBV5	27539	76211	2.56%	0.624%
46	16.516	2298	2300	2302	rBV2	6737	6411	0.22%	0.052%
47	16.569	2307	2309	2312	rVB4	3428	3548	0.12%	0.029%
48	16.616	2314	2317	2321	rBV5	7513	12839	0.43%	0.105%
49	16.692	2325	2330	2334	rBV4	17193	34600	1.16%	0.283%
50	16.863	2350	2359	2373	rBV5	43213	187974	6.31%	1.538%
51	16.998	2375	2382	2392	rVV	41260	105258	3.53%	0.861%
52	17.233	2405	2422	2428	rBV2	768515	2979316	100.00%	24.375%
53	17.292	2429	2432	2449	rVB3	334752	1107185	37.16%	9.058%
54	17.657	2482	2494	2495	rBV10	42100	115876	3.89%	0.948%
55	18.092	2560	2568	2571	rBV2	93201	243299	8.17%	1.991%
56	18.298	2596	2603	2606	rBV4	93287	235813	7.92%	1.929%
57	19.345	2771	2781	2782	rBV2	372331	871840	29.26%	7.133%


Sum of corrected areas: 12222945

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052119\
Data File : BM020491.D
Acq On : 22 May 2019 10:08
Operator : JU/SJ
Sample : K2923-22
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A42F3

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051619MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

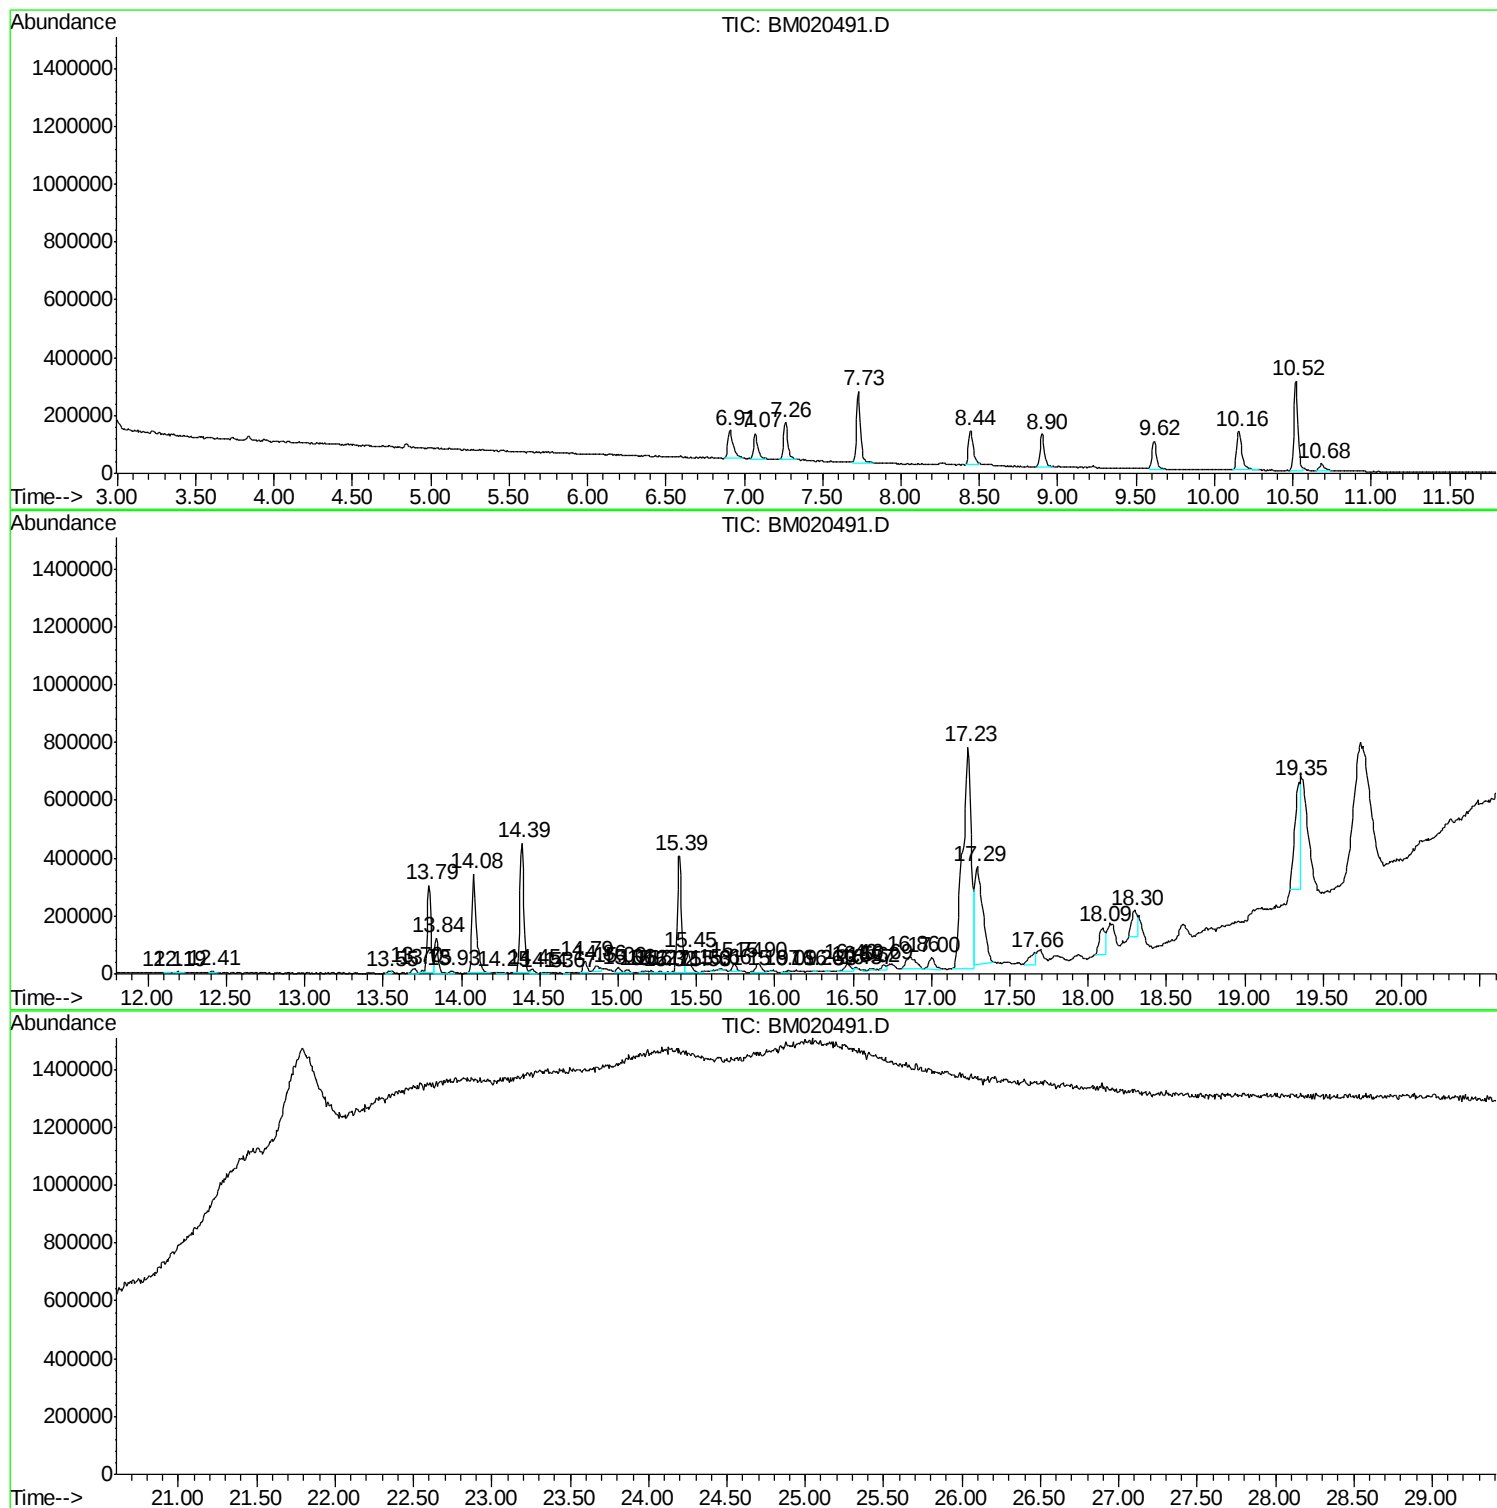

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM052119\
Data File : BM020491.D
Acq On : 22 May 2019 10:08
Operator : JU/SJ
Sample : K2923-22
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A42F3

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051619MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM052119\
Data File : BM020491.D
Acq On : 22 May 2019 10:08
Operator : JU/SJ
Sample : K2923-22
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A42F3

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051619MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc