

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052219\
 Data File : BM020497.D
 Acq On : 22 May 2019 18:33
 Operator : JU/SJ
 Sample : PB119912BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK12

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051619MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.857	652	658	668	rVB	186461	322578	24.51%	2.534%
2	7.022	681	686	693	rVB	139098	223224	16.96%	1.754%
3	7.210	712	718	725	rVB	205885	333218	25.32%	2.618%
4	7.675	792	797	805	rVB	193463	319245	24.26%	2.508%
5	8.392	913	919	930	rBV	218738	374944	28.49%	2.945%
6	8.851	991	997	1007	rVB	173611	299115	22.73%	2.350%
7	9.563	1112	1118	1130	rVB	152169	261695	19.88%	2.056%
8	10.098	1203	1209	1223	rBV	231075	397671	30.22%	3.124%
9	10.469	1264	1272	1281	rBV	251066	432560	32.87%	3.398%
10	10.622	1292	1298	1309	rBV	183834	338380	25.71%	2.658%
11	12.075	1541	1545	1550	rVB3	3082	4433	0.34%	0.035%
12	13.751	1824	1830	1841	rBV	453924	590028	44.83%	4.635%
13	14.033	1871	1878	1885	rBV	462851	684575	52.01%	5.378%
14	14.210	1900	1908	1919	rBV3	13181	34005	2.58%	0.267%
15	14.339	1924	1930	1940	rBV2	410793	603467	45.85%	4.741%
16	14.574	1964	1970	1986	rBV	107977	224473	17.06%	1.763%
17	14.686	1988	1989	1994	rVV3	3815	5344	0.41%	0.042%
18	14.721	1994	1995	1998	rVV	2594	2214	0.17%	0.017%
19	14.763	1998	2002	2004	rVV2	1595	2620	0.20%	0.021%
20	15.121	2062	2063	2068	rVB2	1718	1603	0.12%	0.013%
21	15.339	2093	2100	2110	rBV	590793	857675	65.17%	6.738%
22	15.404	2110	2111	2114	rVB	2187	1935	0.15%	0.015%
23	15.480	2120	2124	2132	rBV	138441	195261	14.84%	1.534%
24	15.568	2137	2139	2143	rBV	3112	4180	0.32%	0.033%
25	16.115	2228	2232	2234	rVB	1820	1897	0.14%	0.015%
26	16.210	2245	2248	2250	rBV3	1191	1341	0.10%	0.011%
27	16.321	2264	2267	2269	rBV	1637	1481	0.11%	0.012%
28	16.886	2359	2363	2365	rVV3	1974	1771	0.13%	0.014%
29	17.092	2392	2398	2409	rBV2	545173	769328	58.45%	6.044%
30	17.192	2409	2415	2425	rVV	703220	958726	72.84%	7.532%
31	17.286	2428	2431	2434	rVB2	1444	1627	0.12%	0.013%
32	17.545	2472	2475	2478	rBV3	1972	2731	0.21%	0.021%
33	17.698	2498	2501	2505	rVB3	1317	1446	0.11%	0.011%
34	17.974	2544	2548	2552	rBV3	3583	5744	0.44%	0.045%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052219\
 Data File : BM020497.D
 Acq On : 22 May 2019 18:33
 Operator : JU/SJ
 Sample : PB119912BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK12

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051619MA.M
 Title : SVOA CALIBRATION

35	18.051	2558	2561	2563	rBV2	2637	2324	0.18%	0.018%
36	18.315	2605	2606	2610	rBV3	1824	2499	0.19%	0.020%
37	18.498	2634	2637	2640	rBV3	1842	2941	0.22%	0.023%
38	18.533	2640	2643	2646	rVV4	2121	2826	0.21%	0.022%
39	18.580	2649	2651	2654	rVB3	2612	1665	0.13%	0.013%
40	18.627	2655	2659	2660	rBV3	2397	2523	0.19%	0.020%
41	18.851	2694	2697	2698	rBV3	2096	2588	0.20%	0.020%
42	18.868	2698	2700	2702	rVB2	2306	2284	0.17%	0.018%
43	18.921	2707	2709	2715	rVV4	2254	3663	0.28%	0.029%
44	18.968	2715	2717	2718	rBV3	1735	1472	0.11%	0.012%
45	19.062	2731	2733	2735	rBV3	2380	2890	0.22%	0.023%
46	19.103	2739	2740	2741	rBV2	2331	1475	0.11%	0.012%
47	19.133	2741	2745	2749	rVV4	6592	8970	0.68%	0.070%
48	19.386	2784	2788	2789	rBV4	5810	6679	0.51%	0.052%
49	19.498	2800	2807	2814	rBV	877395	1244557	94.56%	9.777%
50	21.286	3107	3111	3118	rBV	683152	953512	72.45%	7.491%
51	23.397	3464	3470	3478	rVB	696192	1316136	100.00%	10.339%
52	23.538	3489	3494	3501	rVB	501788	909992	69.14%	7.149%


Sum of corrected areas: 12729531

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052219\
Data File : BM020497.D
Acq On : 22 May 2019 18:33
Operator : JU/SJ
Sample : PB119912BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK12

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051619MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

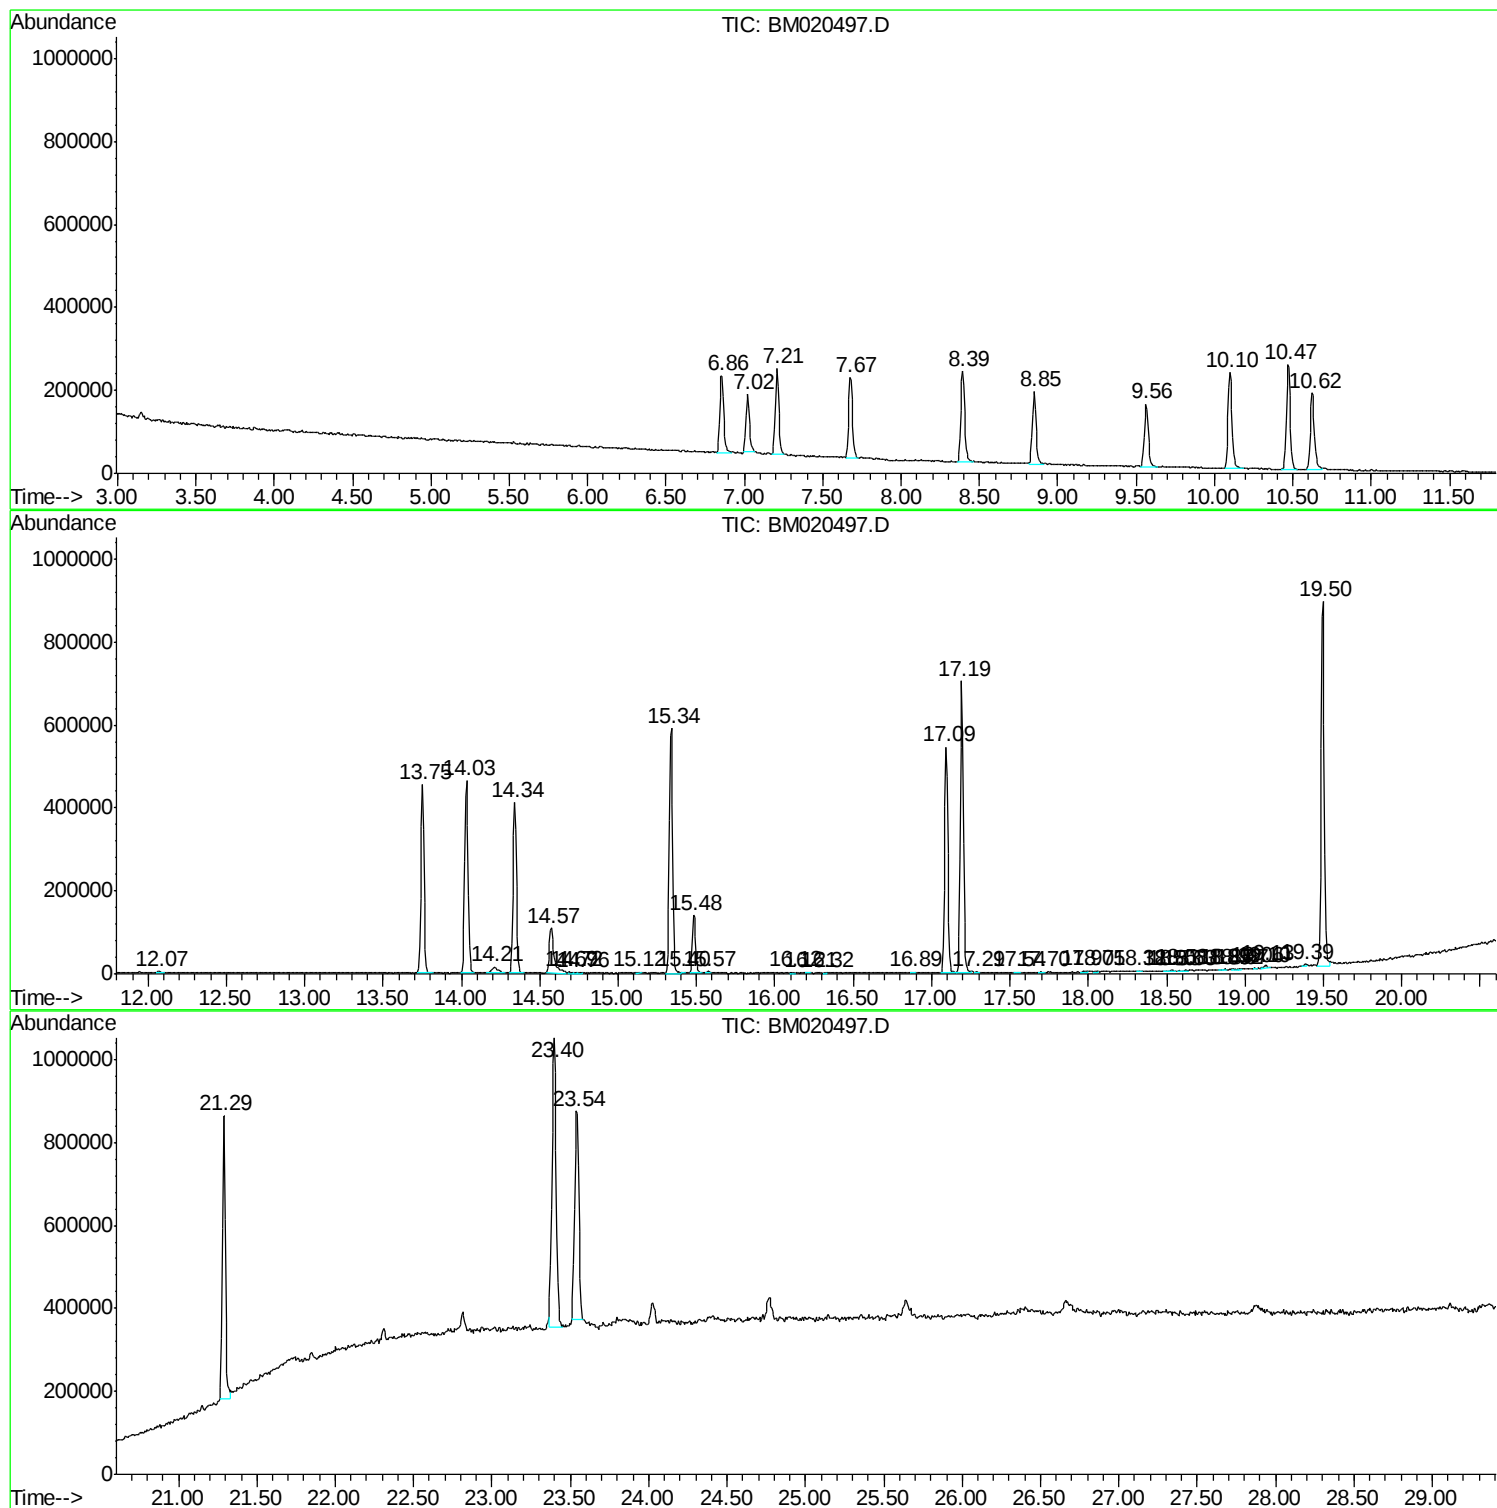

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM052219\
Data File : BM020497.D
Acq On : 22 May 2019 18:33
Operator : JU/SJ
Sample : PB119912BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK12

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051619MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM052219\
Data File : BM020497.D
Acq On : 22 May 2019 18:33
Operator : JU/SJ
Sample : PB119912BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK12

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051619MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc