
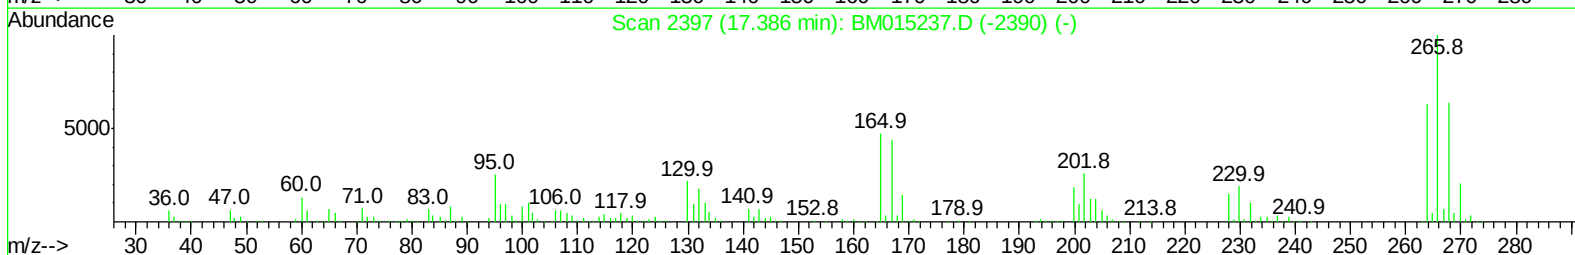
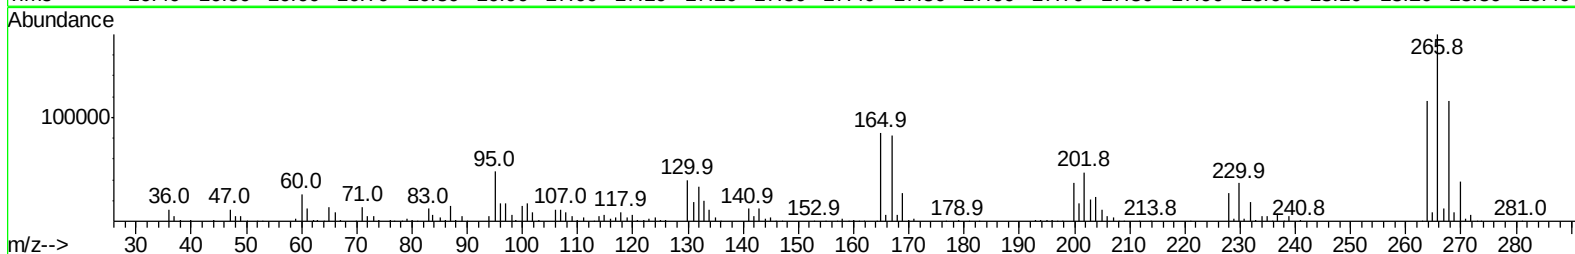


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA M\DATA\BM052318\
Data File : BM015273.D
Acq On : 23 May 2018 13:24
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 24 03:18:00 2018
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM052218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 22 15:47:28 2018
Response via : Initial Calibration

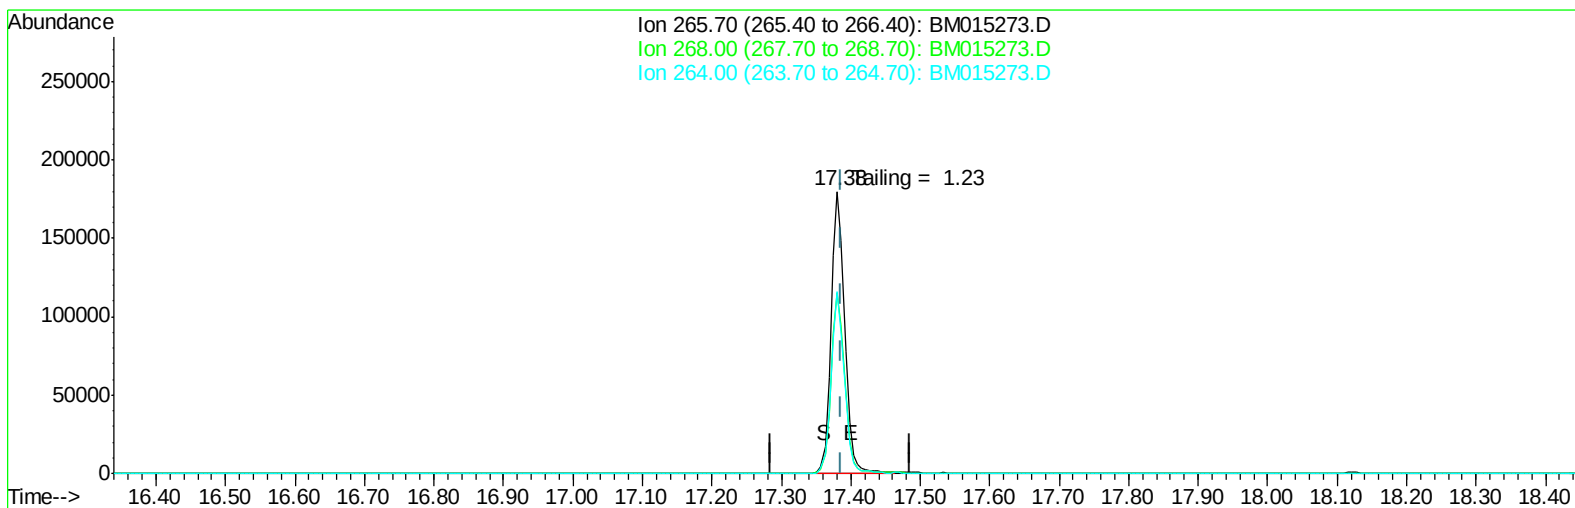

TIC: BM015273.D

(69) Pentachlorophenol (C)




17.380min (-0.006) 43102.92ng

response 243259

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	64.30
264.00	61.20	64.67
0.00	0.00	0.00

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA M\DATA\BM052318\
Data File : BM015273.D
Acq On : 23 May 2018 13:24
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 24 03:18:00 2018
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM052218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 22 15:47:28 2018
Response via : Initial Calibration

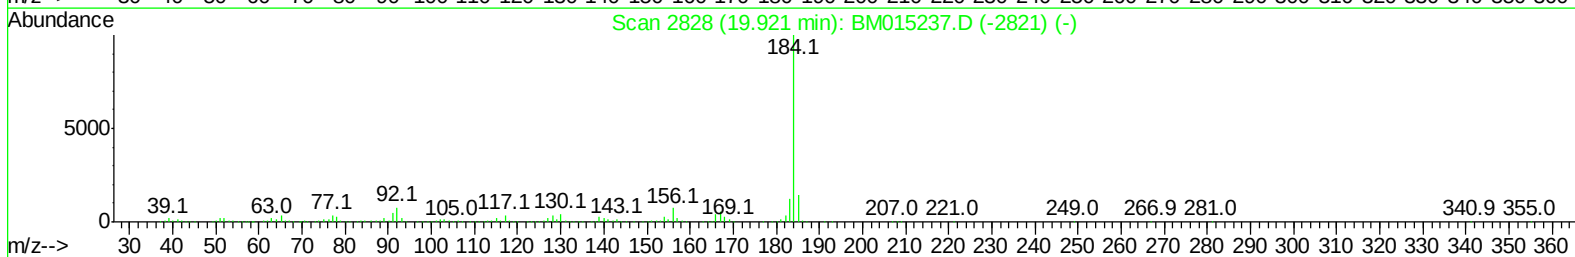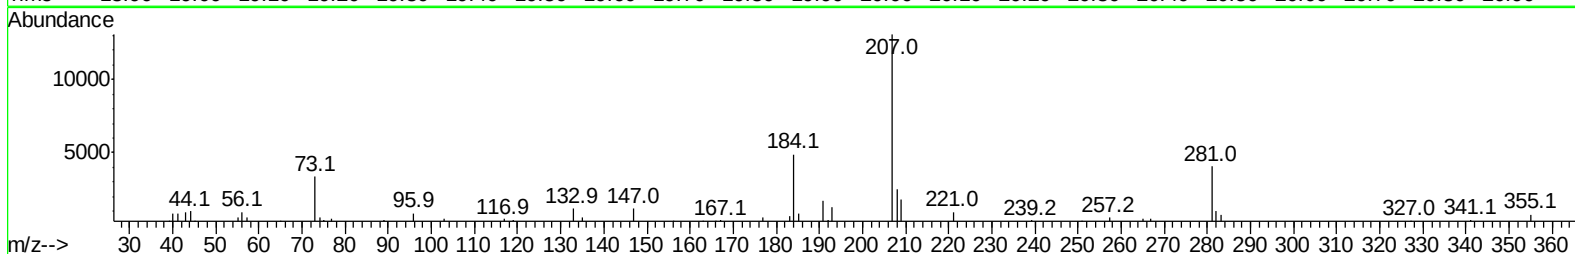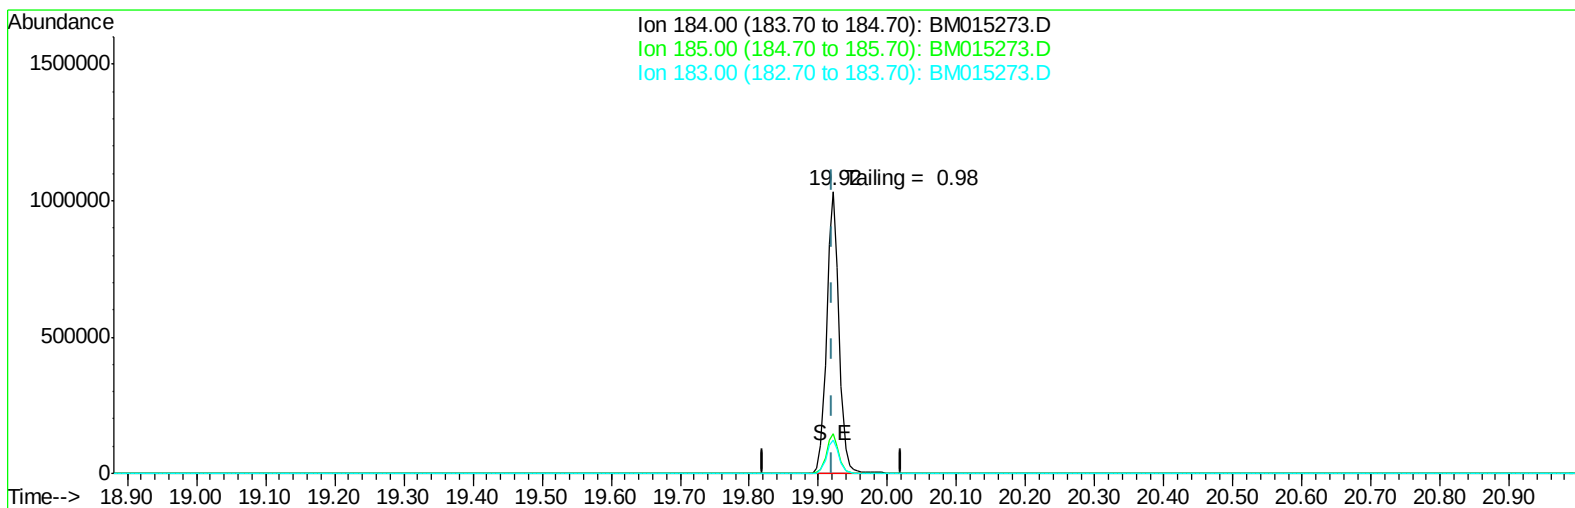

TIC: BM015273.D

(76) Benzidine

19.921min (+0.000) 18679.97ng

response 1280676

Ion	Exp%	Act%
184.00	100	100
185.00	14.10	14.25
183.00	11.10	12.06
0.00	0.00	0.00