


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA M\Data\BM052318\
 Data File : BM015273.D
 Acq On : 23 May 2018 13:24
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM052218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue May 22 15:47:28 2018

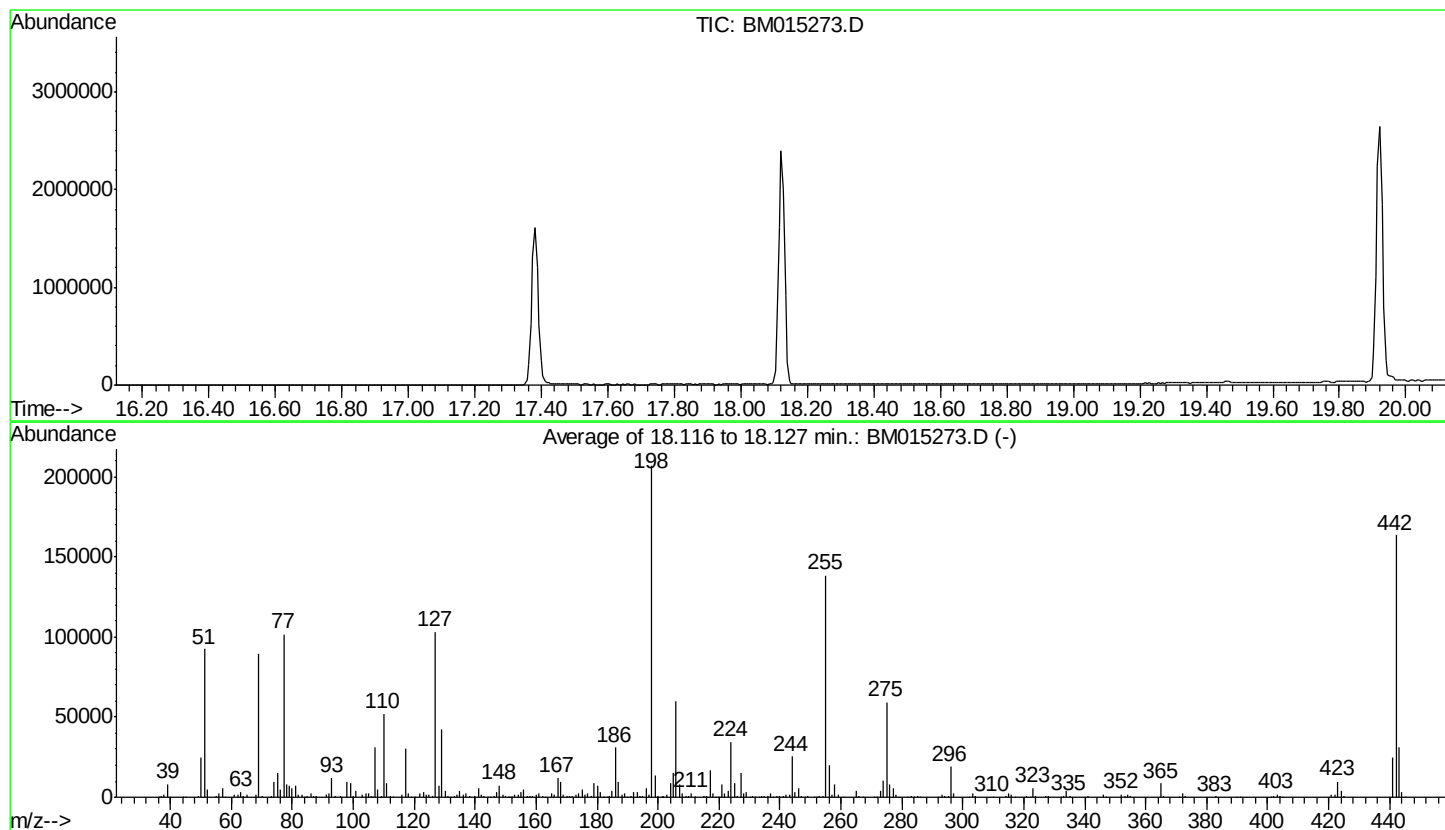

AutoFind: Scans 2521, 2522, 2523; Background Corrected with Scan 2515

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.7	92445	PASS
68	69	0.00	2	1.9	1656	PASS
69	198	0.00	100	43.1	89176	PASS
70	69	0.00	2	0.5	456	PASS
127	198	10	80	49.9	103210	PASS
197	198	0.00	2	0.6	1318	PASS
198	198	100	100	100.0	206997	PASS
199	198	5	9	6.6	13625	PASS
275	198	10	60	28.7	59418	PASS
365	198	1	100	4.1	8431	PASS
441	443	0.01	100	78.9	24827	PASS
442	198	50	100	79.0	163440	PASS
443	442	15	24	19.3	31472	PASS