


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052319\
 Data File : BM020522.D
 Acq On : 23 May 2019 18:57
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM043019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu May 23 13:59:00 2019

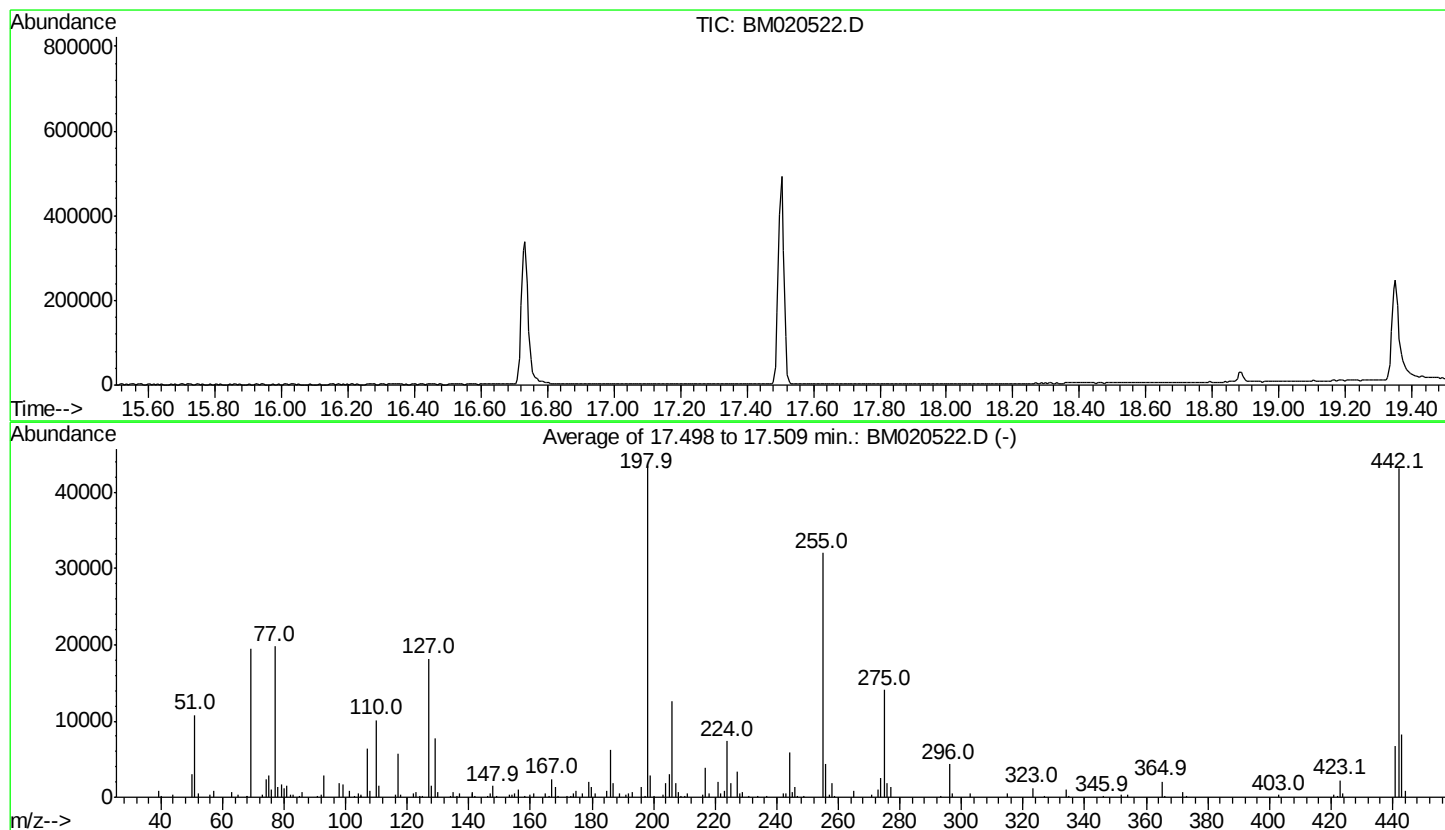

AutoFind: Scans 2467, 2468, 2469; Background Corrected with Scan 2461

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	24.8	10799	PASS
68	69	0.00	2	1.0	185	PASS
69	198	0.00	100	44.7	19467	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	41.8	18183	PASS
197	198	0.00	2	0.6	252	PASS
198	198	100	100	100.0	43525	PASS
199	198	5	9	6.7	2914	PASS
275	198	10	60	32.3	14076	PASS
365	198	1	100	4.8	2078	PASS
441	198	0.01	100	15.4	6708	PASS
442	198	50	100	99.3	43213	PASS
443	442	15	24	19.2	8276	PASS