



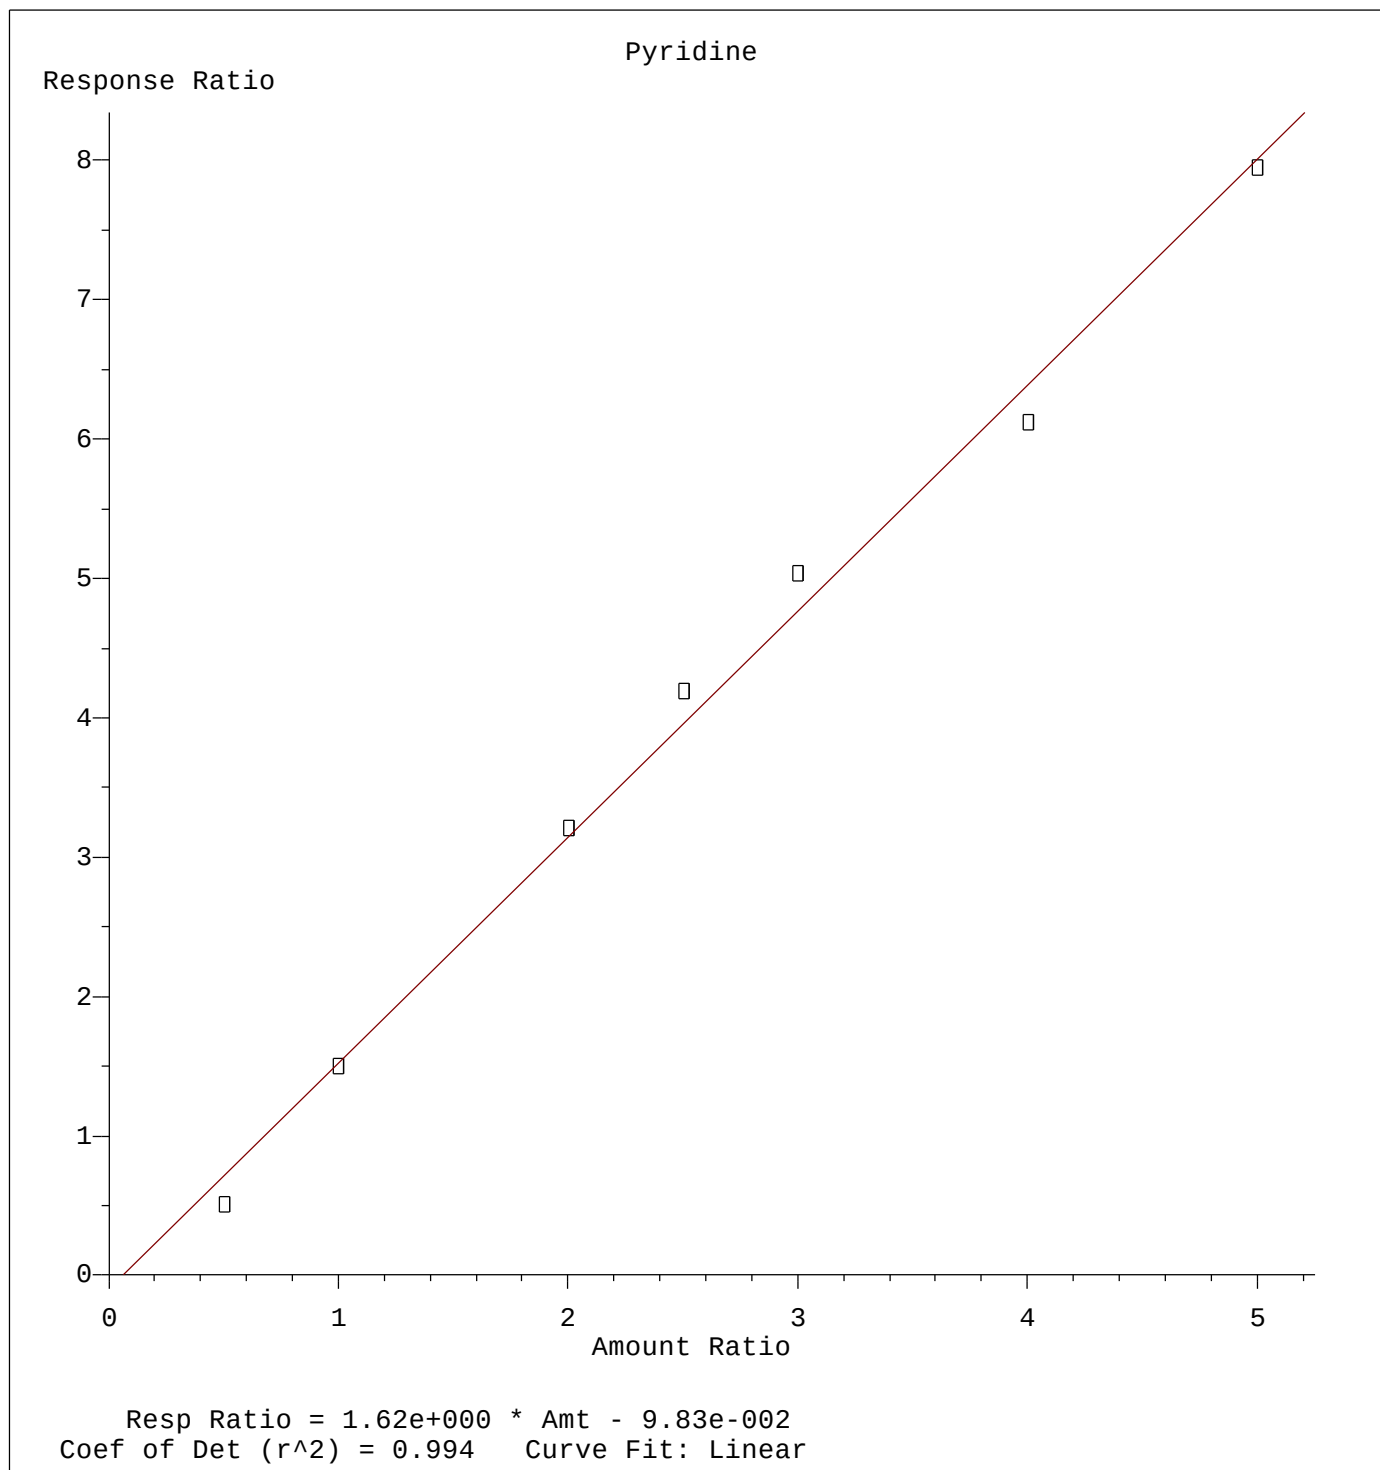


Method Name: Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM052419.M
Calibration Table Last Updated: Fri May 24 16:07:05 2019

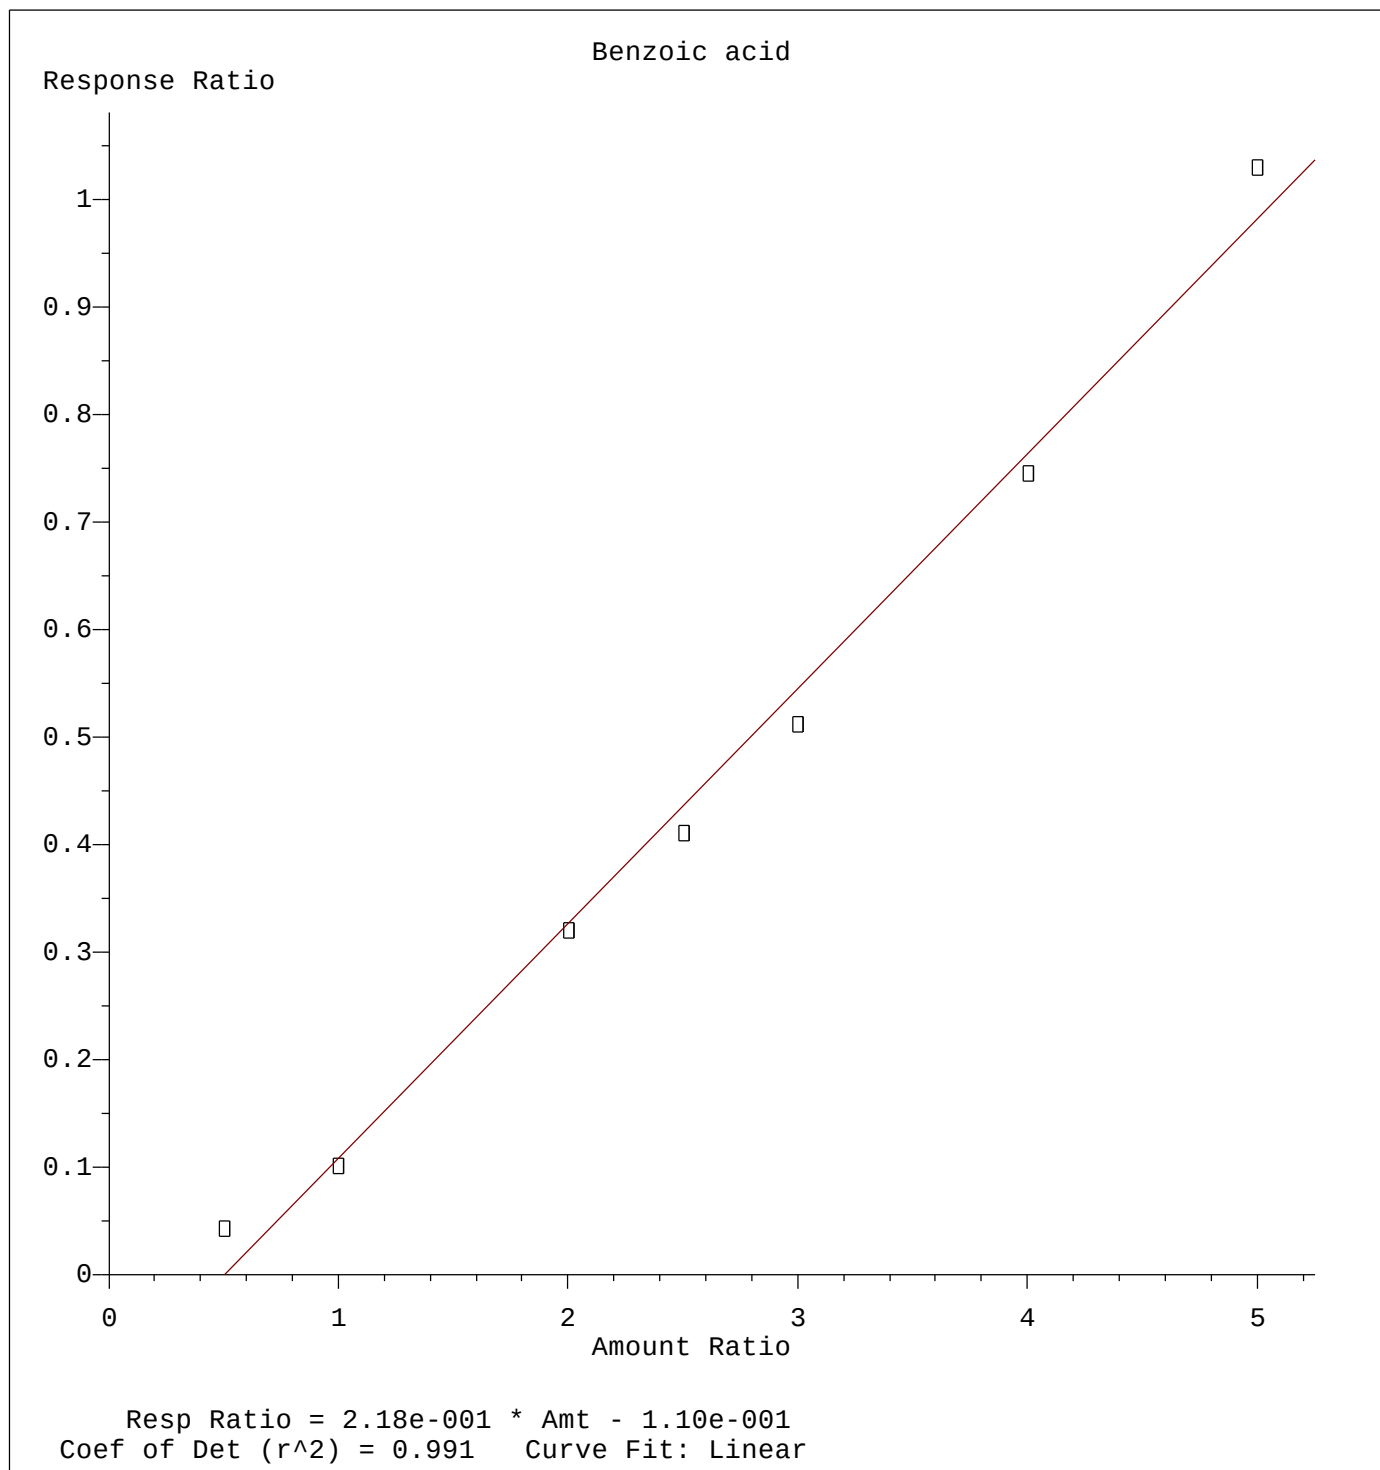

Method Name: Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM052419.M
Calibration Table Last Updated: Fri May 24 16:07:05 2019


Hexachlorocyclopentadiene

Response Ratio

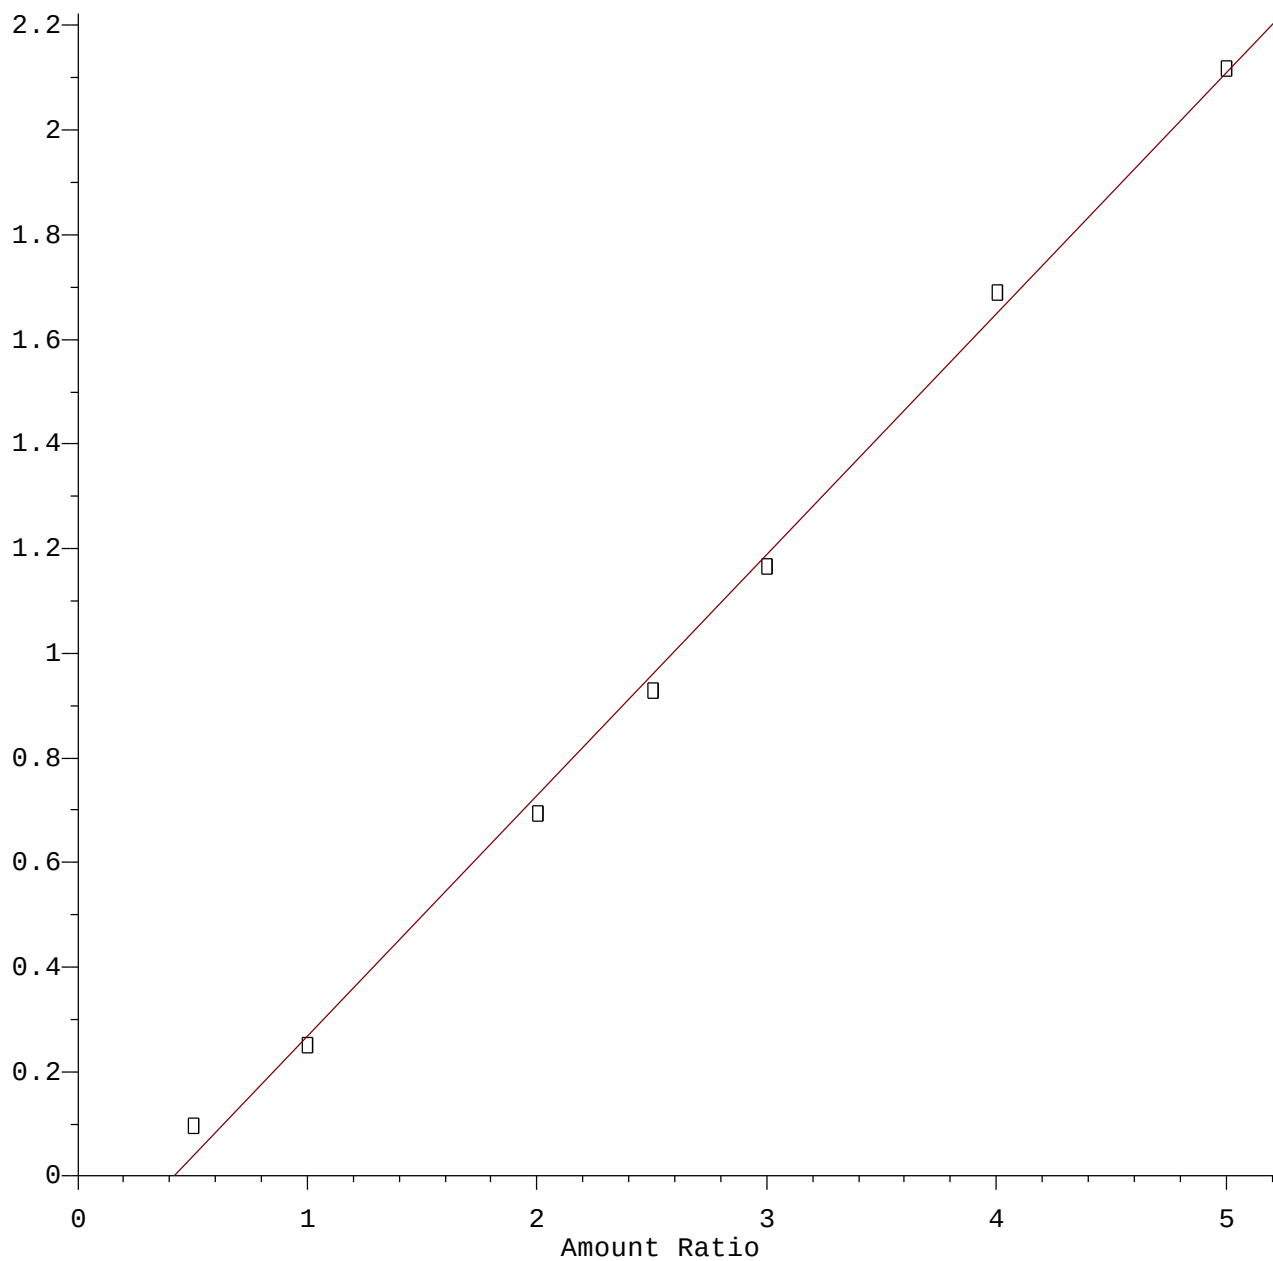

Resp Ratio = $4.60 \times 10^{-1} \times \text{Amt} - 1.91 \times 10^{-1}$
Coef of Det (r^2) = 0.997 Curve Fit: Linear


Method Name: Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM052419.M
Calibration Table Last Updated: Fri May 24 16:07:05 2019

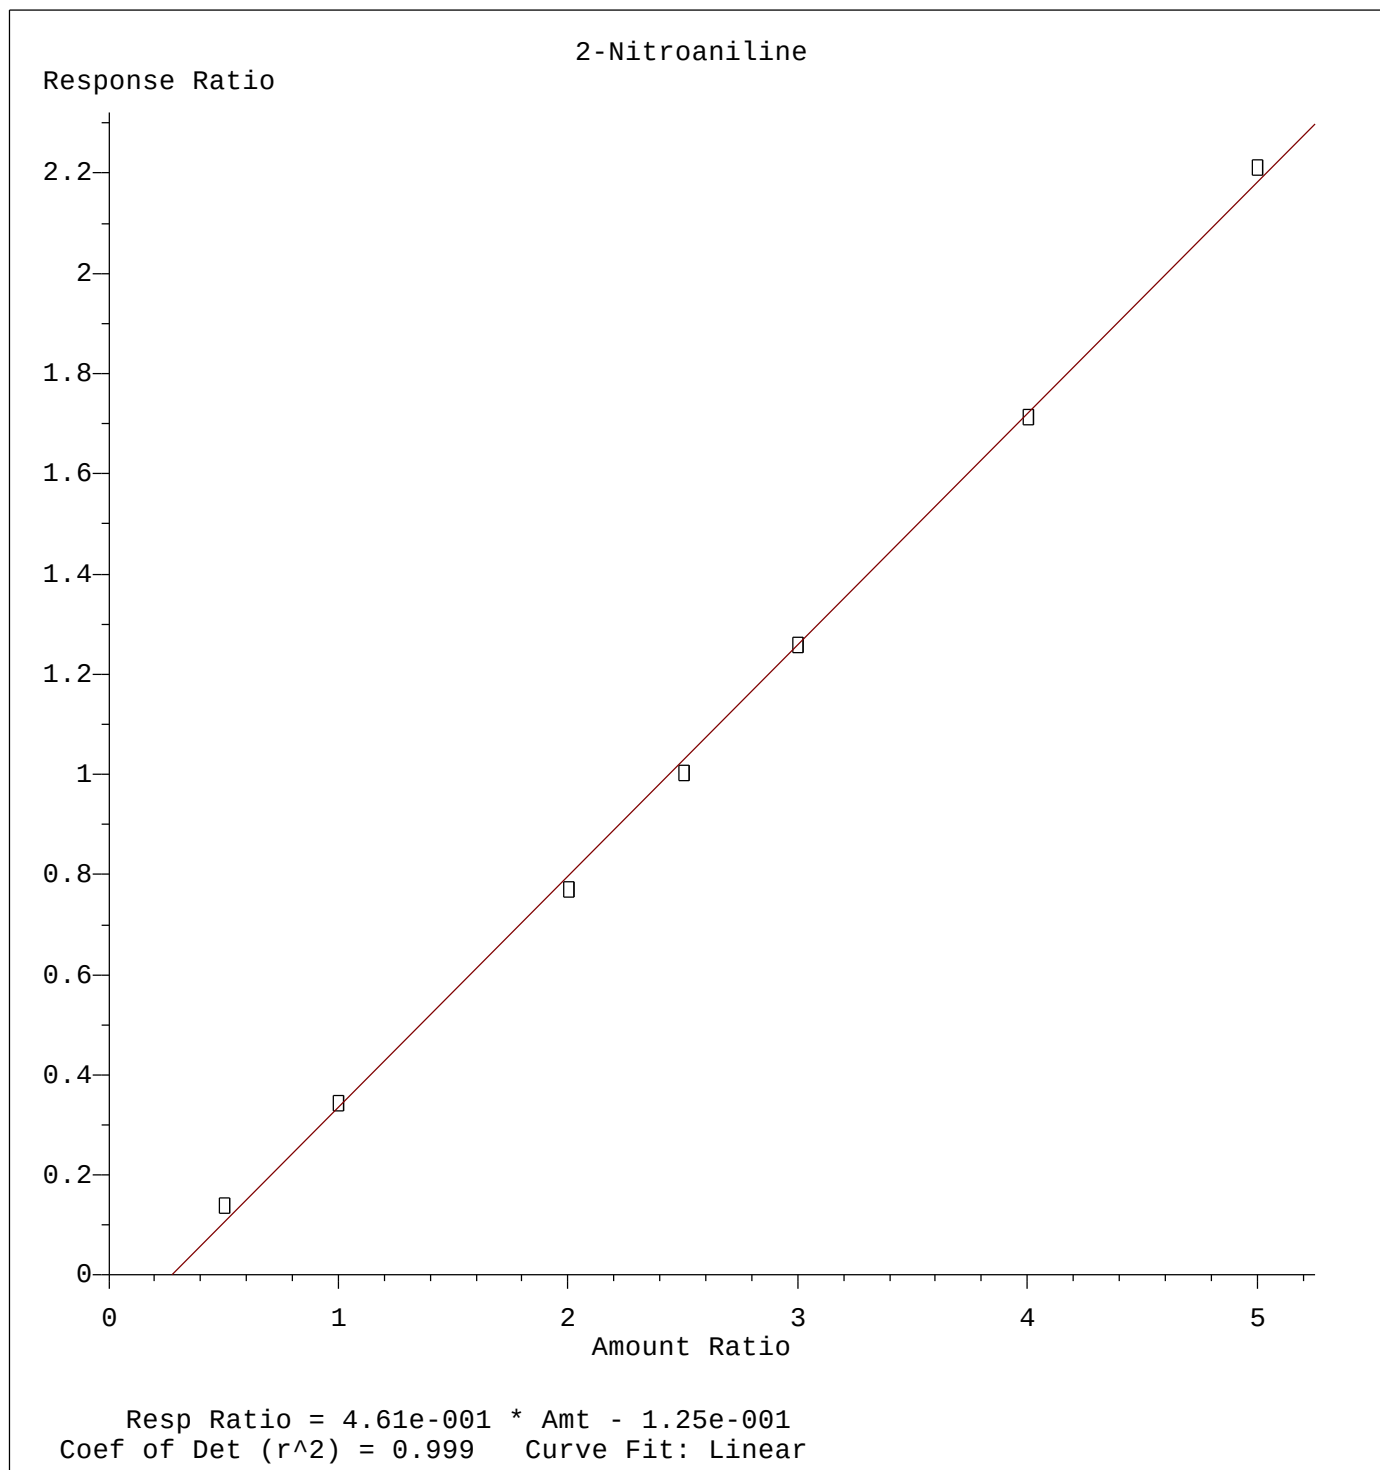

Method Name: Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM052419.M
Calibration Table Last Updated: Fri May 24 16:07:05 2019

3-Nitroaniline

Response Ratio

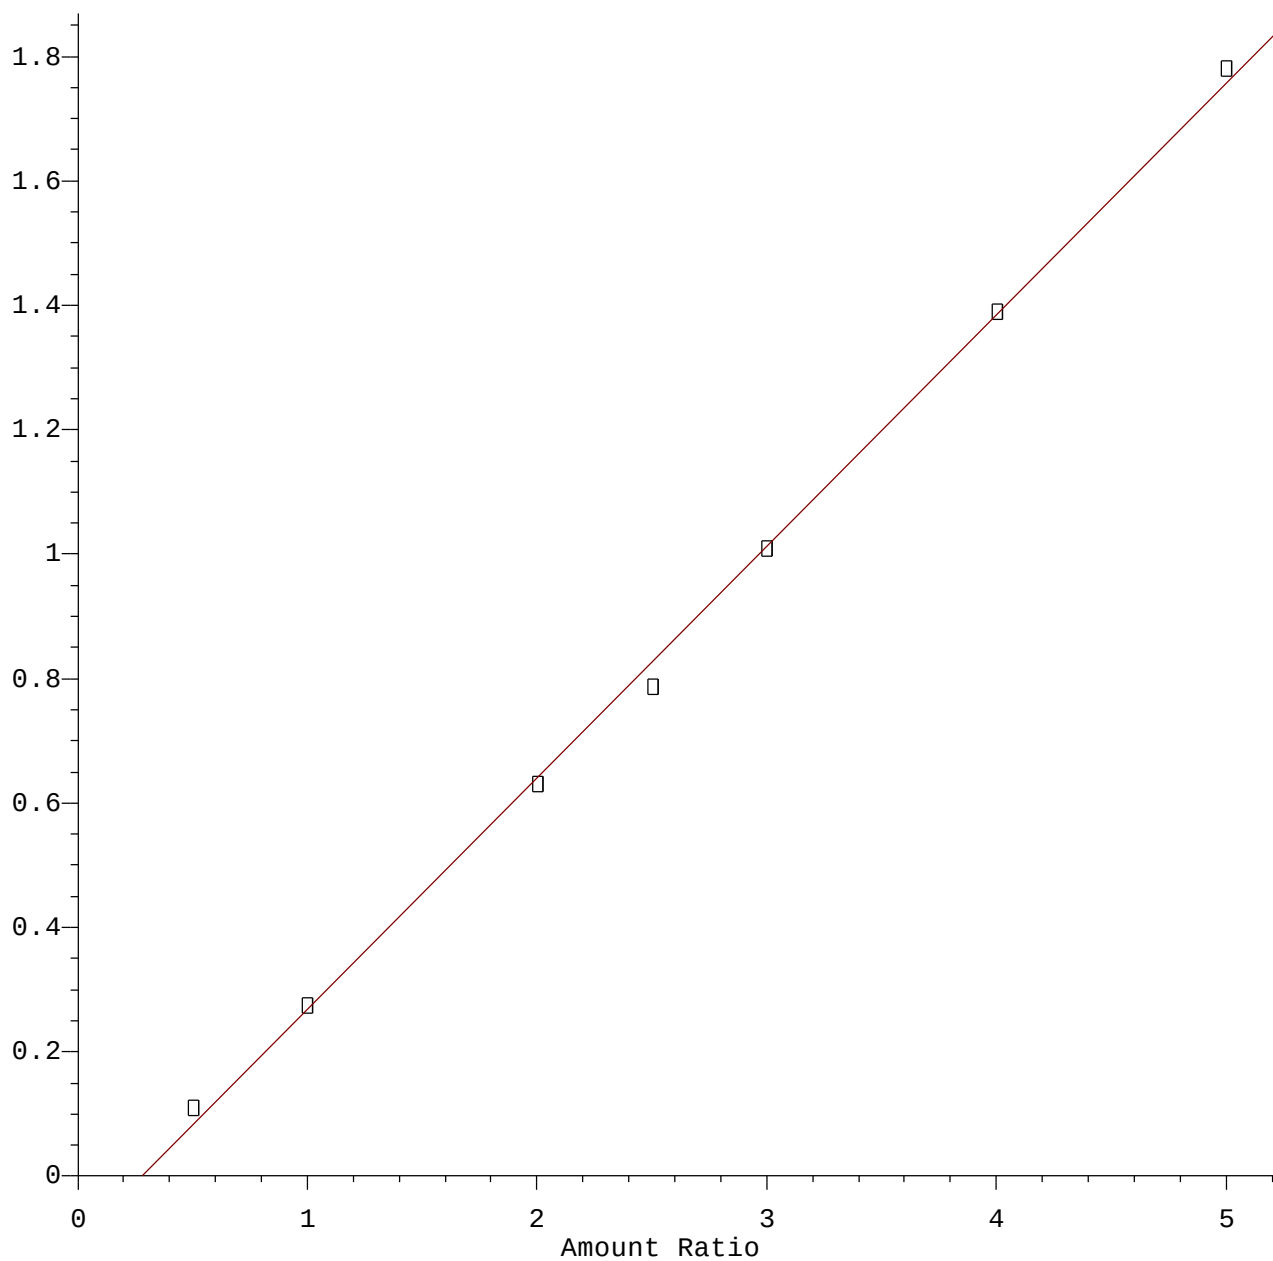


Resp Ratio = $3.72 \times 10^{-1} \times \text{Amt} - 1.04 \times 10^{-1}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM052419.M
Calibration Table Last Updated: Fri May 24 16:07:05 2019


2,4-Dinitrophenol

Response Ratio

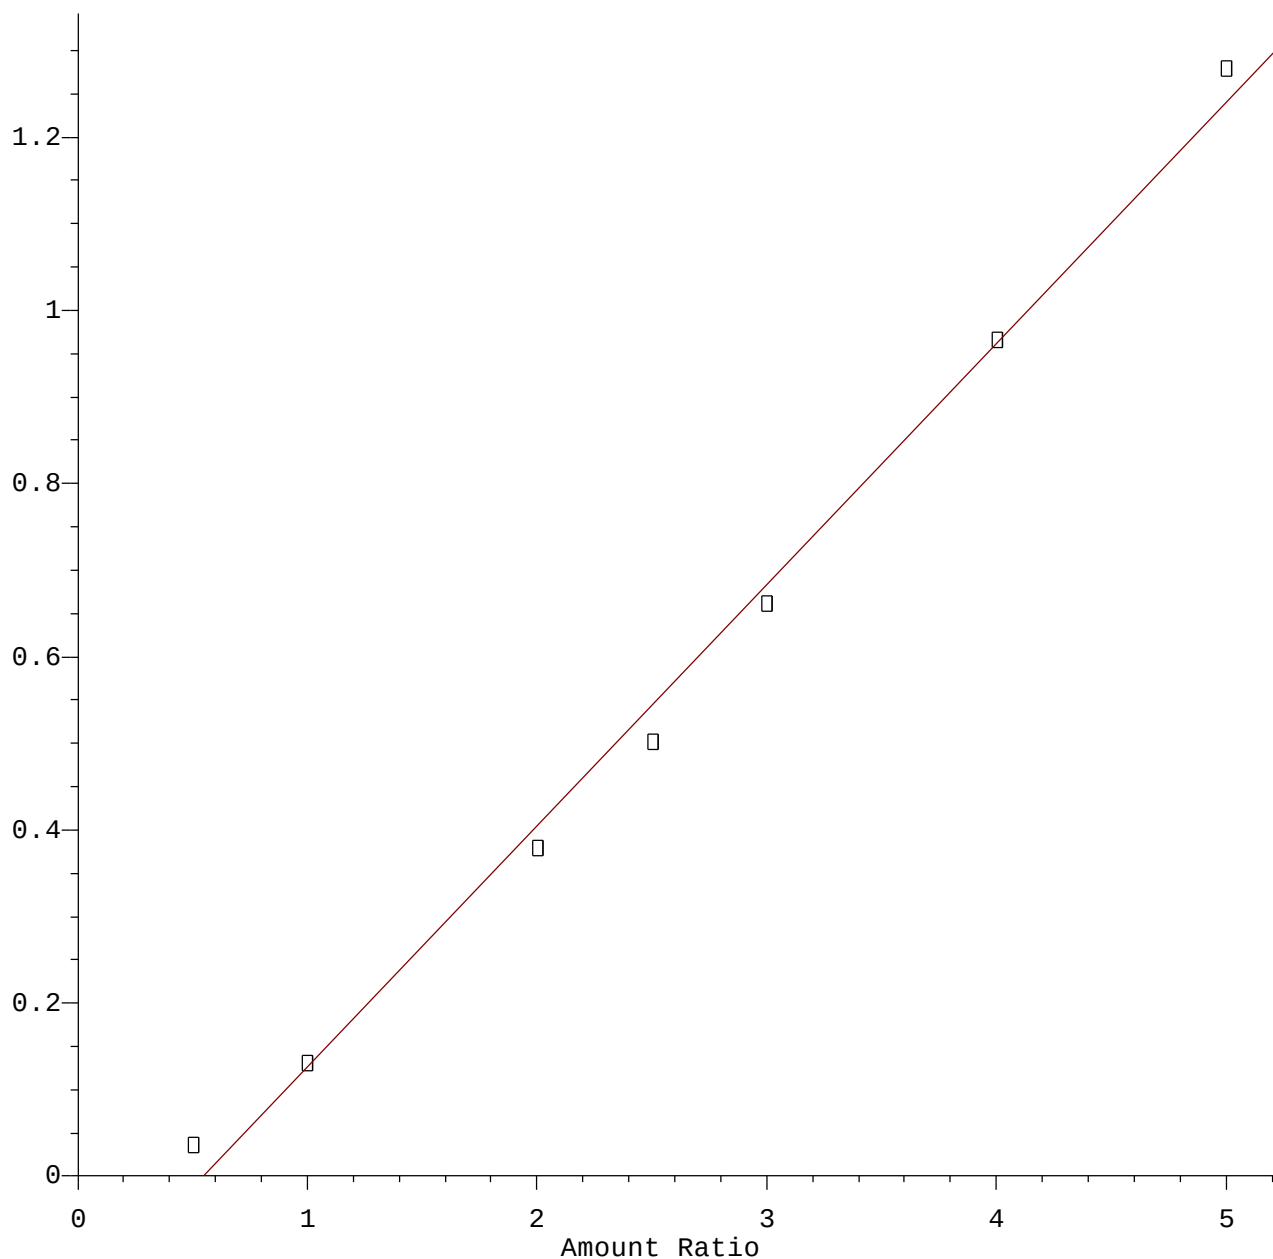

Resp Ratio = $2.78 \times 10^{-1} \times \text{Amt} - 1.52 \times 10^{-1}$
Coef of Det (r^2) = 0.994 Curve Fit: Linear


Method Name: Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM052419.M
Calibration Table Last Updated: Fri May 24 16:07:05 2019

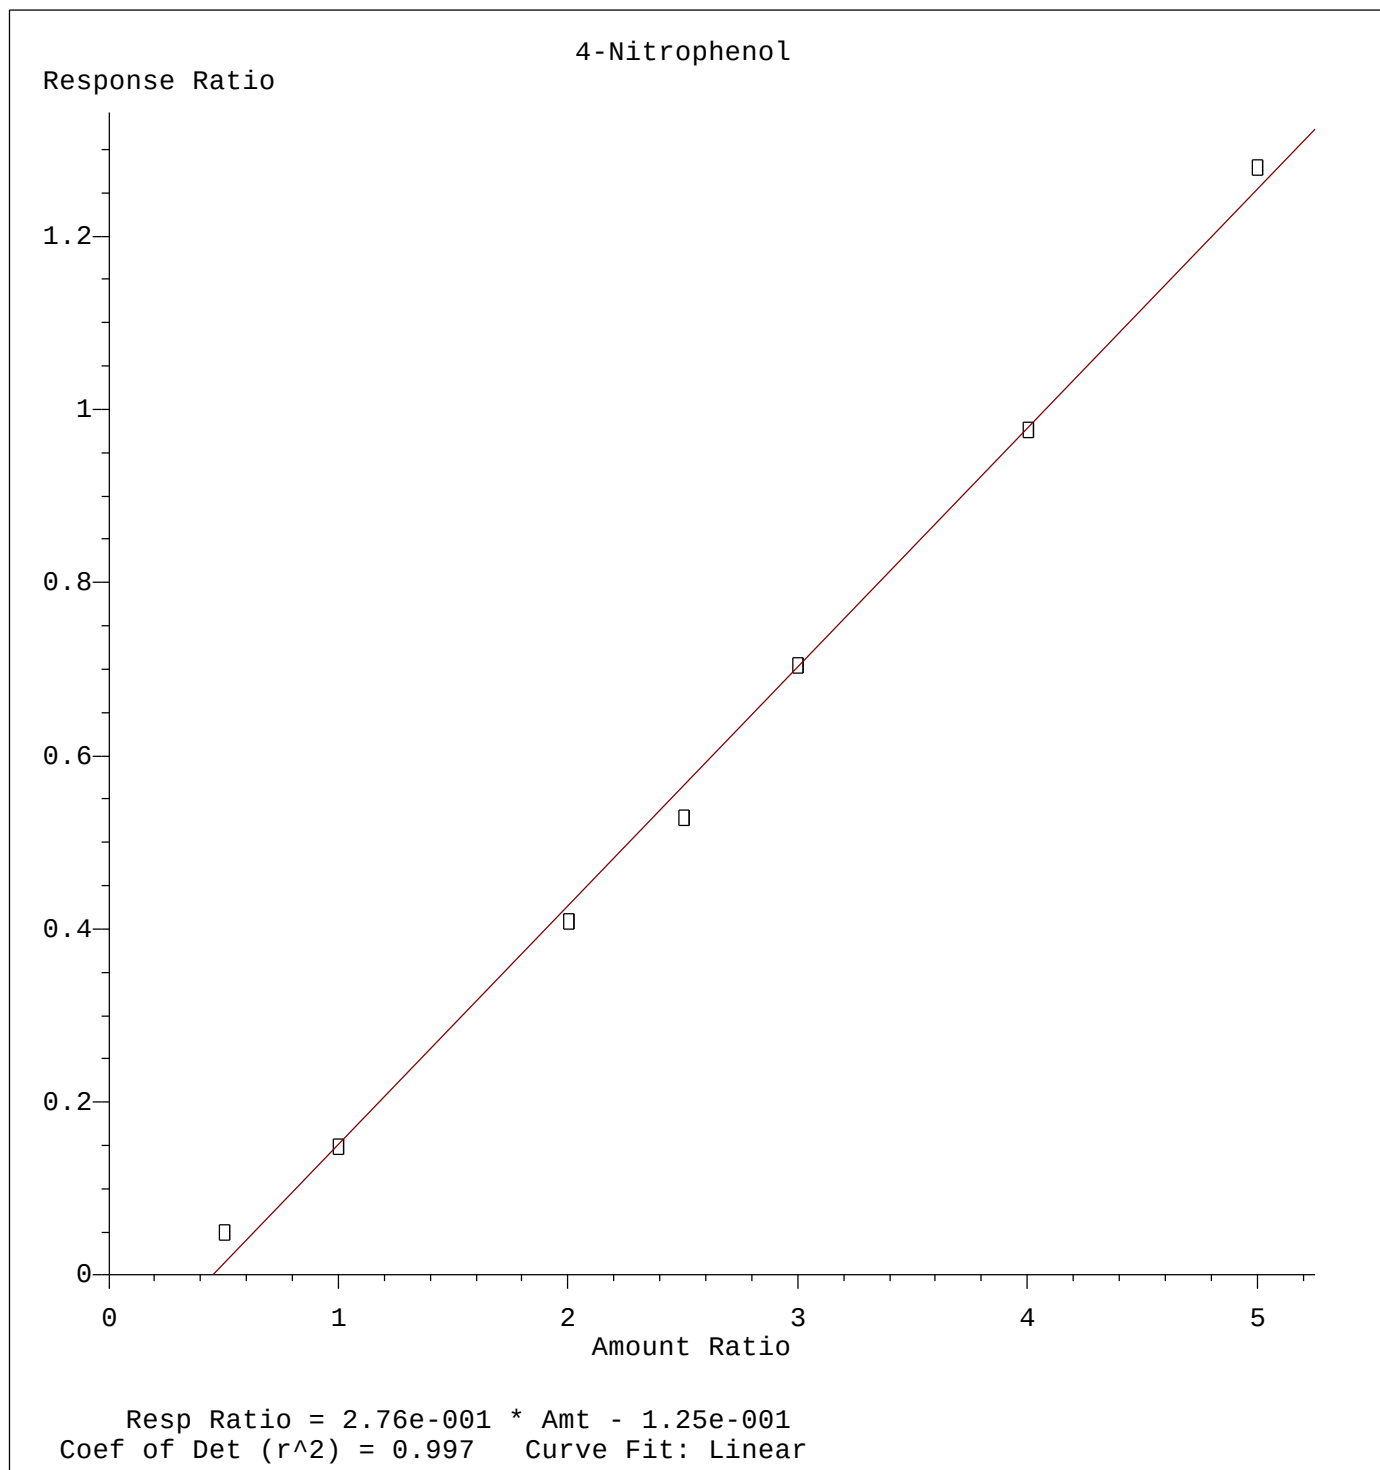

Method Name: Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM052419.M
Calibration Table Last Updated: Fri May 24 16:07:05 2019

4,6-Dinitro-2-methylphenol

Response Ratio

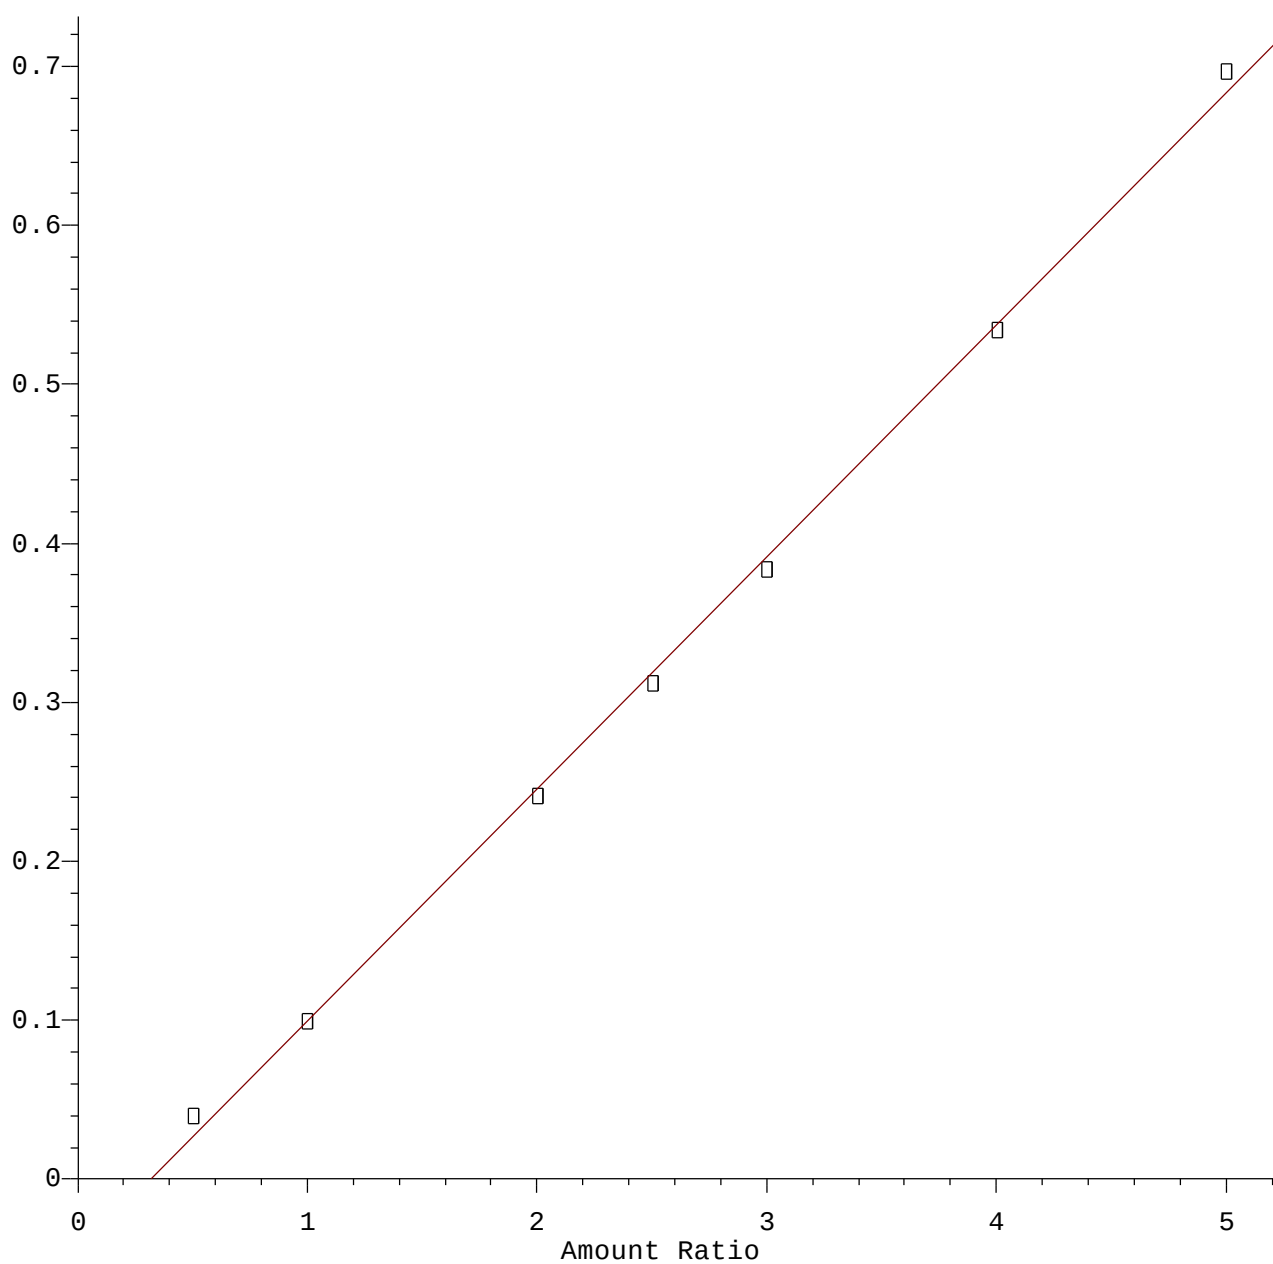

Resp Ratio = $1.46 \times 10^{-1} \times \text{Amt} - 4.62 \times 10^{-2}$
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM052419.M
Calibration Table Last Updated: Fri May 24 16:07:05 2019