

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052419\
 Data File : BM020558.D
 Acq On : 25 May 2019 01:32
 Operator : JU/SJ
 Sample : PB120010BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB120010BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM052419.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.245	378	384	401	rBV	368656	742011	15.31%	4.385%
2	6.839	649	655	674	rBV	342003	786924	16.24%	4.650%
3	7.192	708	715	736	rBV	418498	856317	17.67%	5.060%
4	7.663	788	795	806	rBV	108386	240327	4.96%	1.420%
5	7.975	841	848	871	rBV	530553	993567	20.50%	5.871%
6	8.833	985	994	1021	rBV	288752	737116	15.21%	4.356%
7	10.451	1263	1269	1290	rBV	113858	295209	6.09%	1.744%
8	12.927	1684	1690	1709	rBV	1163630	2069665	42.70%	12.230%
9	14.315	1920	1926	1944	rBV2	284060	523784	10.81%	3.095%
10	15.815	2175	2181	2200	rBV	731470	1373494	28.34%	8.116%
11	17.074	2388	2395	2419	rBV	402388	799072	16.49%	4.722%
12	19.697	2836	2841	2861	rBV	3549017	4846673	100.00%	28.640%
13	20.362	2951	2954	2960	rBV3	37374	49185	1.01%	0.291%
14	21.262	3102	3107	3122	rBV	852047	1304465	26.91%	7.708%
15	23.497	3480	3487	3500	rVB	636464	1305111	26.93%	7.712%


Sum of corrected areas: 16922920

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052419\
Data File : BM020558.D
Acq On : 25 May 2019 01:32
Operator : JU/SJ
Sample : PB120010BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB120010BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM052419.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

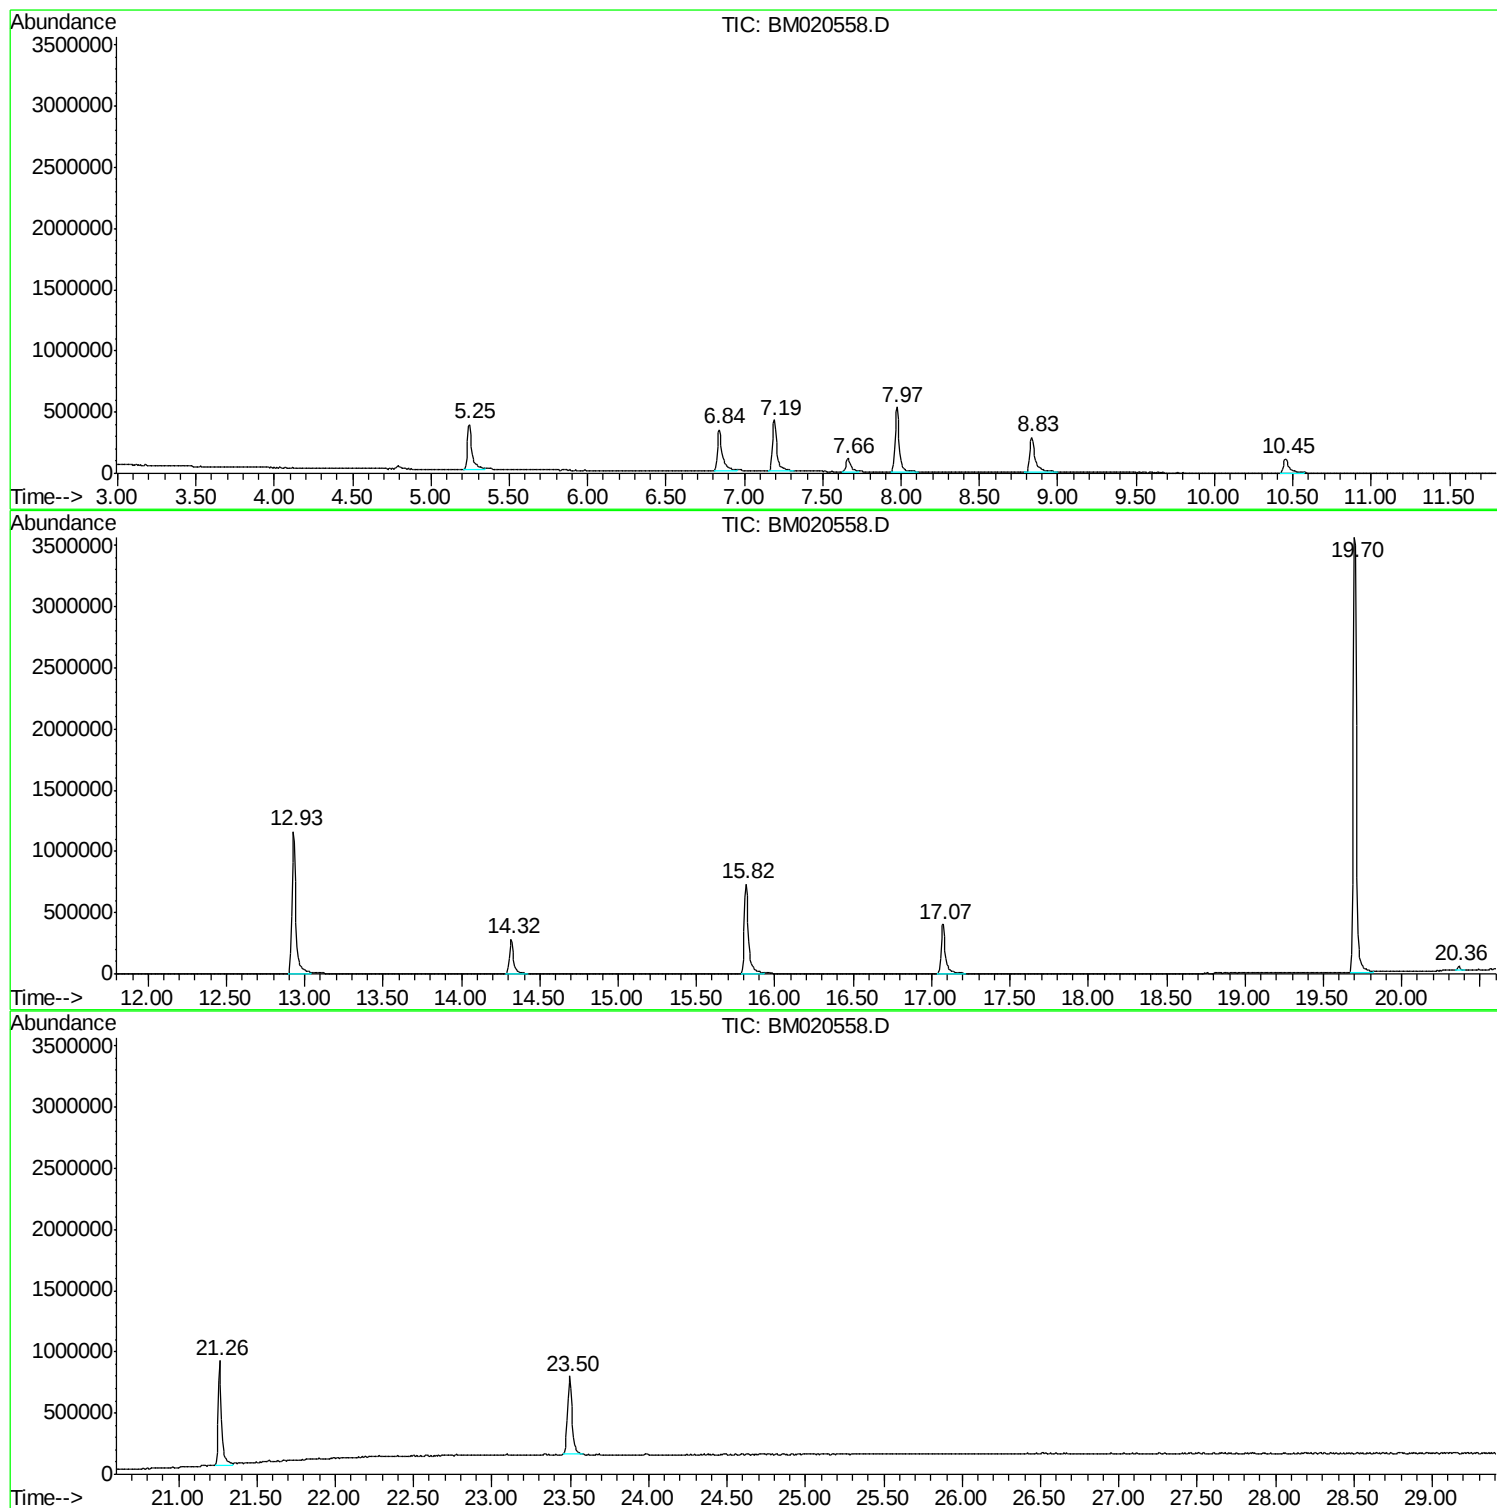

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM052419\
Data File : BM020558.D
Acq On : 25 May 2019 01:32
Operator : JU/SJ
Sample : PB120010BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB120010BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM052419.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.19 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.19	71.26 ng	856317	1,4-Dichlorobenzene-d4	7.66

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	27
2			(5-METHYL-2-PYRIDYL)ACETONITRILE	132	C8H8N2	1000241-93-9	22
3			1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	22
4			3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	16
5			2H-Cyclopenta[d]pyridazine, 2-me...	132	C8H8N2	022291-85-6	16

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM052419\
Data File : BM020558.D
Acq On : 25 May 2019 01:32
Operator : JU/SJ
Sample : PB120010BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB120010BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM052419.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.19	7.19	71.3	ng	856317	1	7.66	240327	20.0