


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM052419\
 Data File : BM020542.D
 Acq On : 24 May 2019 10:58
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM052419.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri May 24 16:07:05 2019

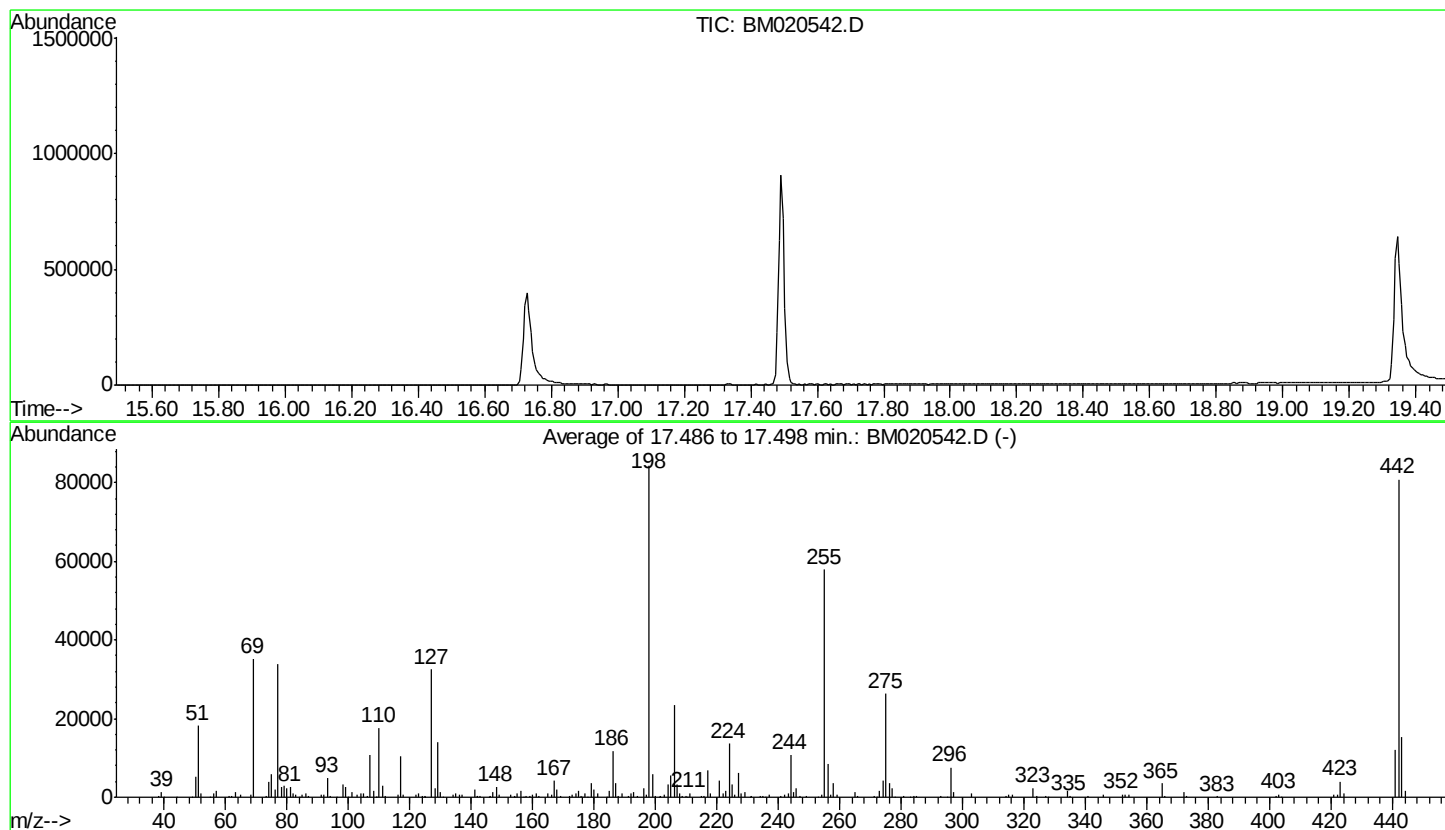

AutoFind: Scans 2465, 2466, 2467; Background Corrected with Scan 2459

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	21.5	18130	PASS
68	69	0.00	2	1.9	654	PASS
69	198	0.00	100	41.8	35216	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	38.4	32426	PASS
197	198	0.00	2	0.8	649	PASS
198	198	100	100	100.0	84338	PASS
199	198	5	9	6.9	5842	PASS
275	198	10	60	31.3	26360	PASS
365	198	1	100	4.1	3495	PASS
441	198	0.01	100	14.2	11939	PASS
442	198	50	100	95.8	80808	PASS
443	442	15	24	18.8	15212	PASS